
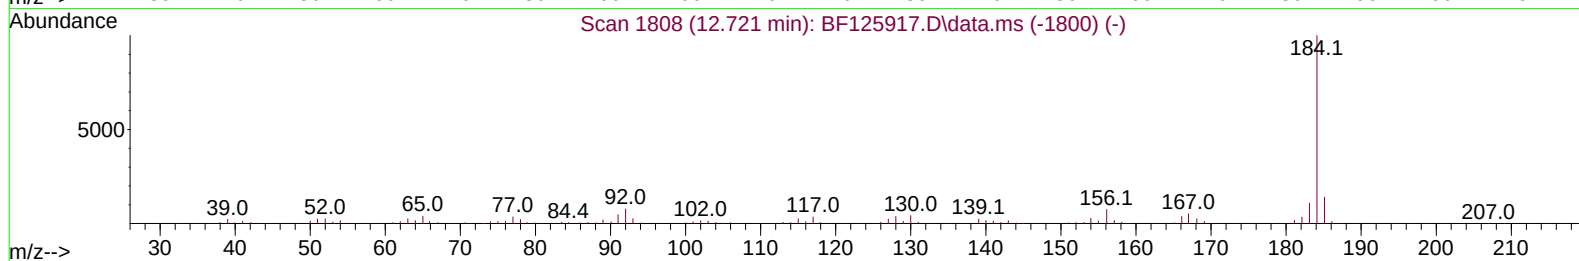
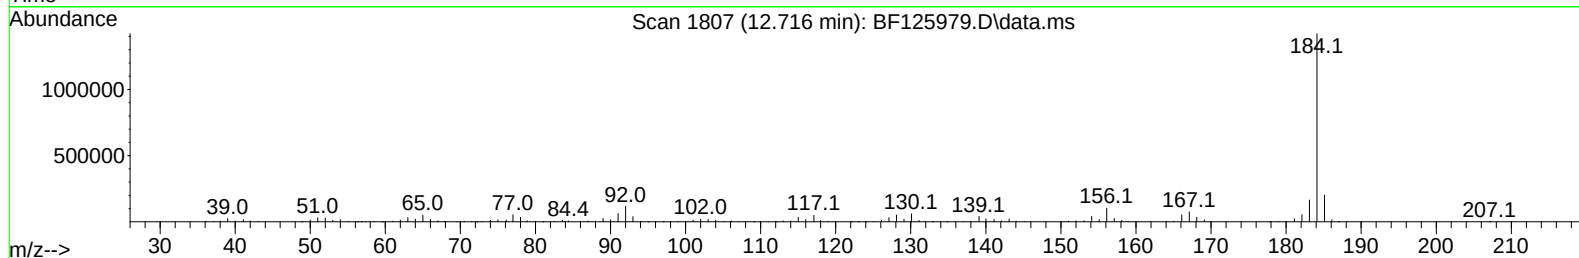


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102821\
Data File : BF125979.D
Acq On : 28 Oct 2021 9:14
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 12:36:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 28 12:01:54 2021
Response via : Initial Calibration

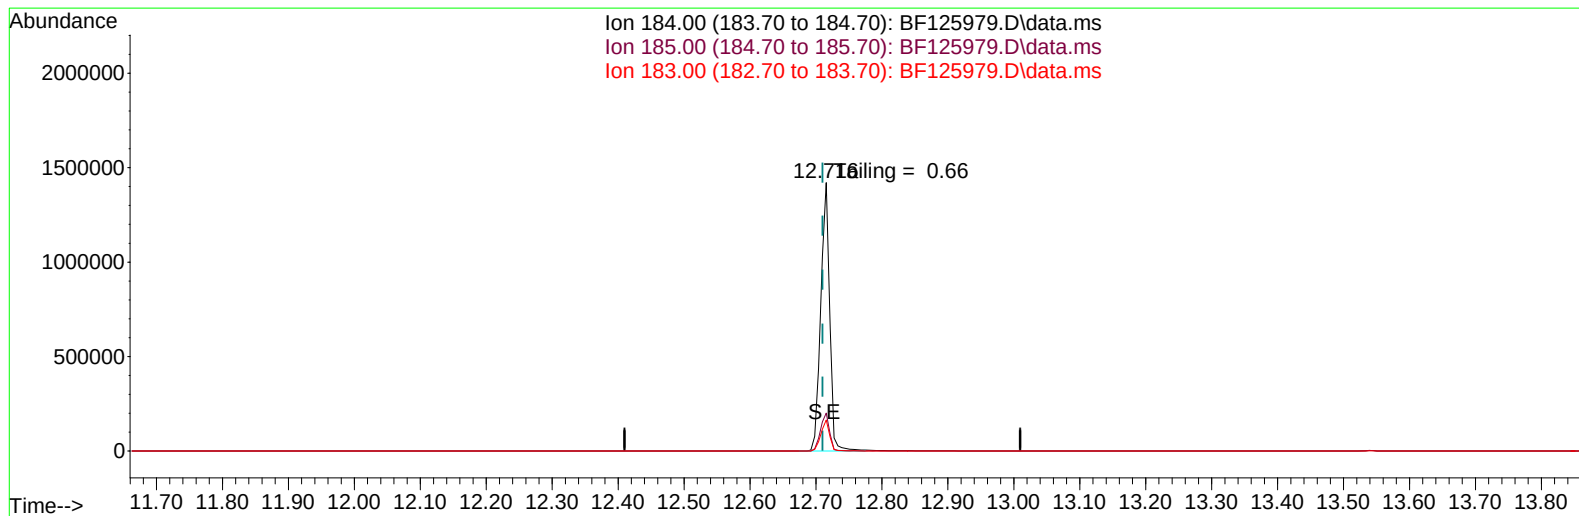

TIC: BF125979.D\data.ms

(77) Benzidine




12.716min (+ 0.006) 0.00 ng

response 1346123

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.17
183.00	10.10	11.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102821\
 Data File : BF125979.D
 Acq On : 28 Oct 2021 9:14
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 12:36:48 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 28 12:01:54 2021
 Response via : Initial Calibration

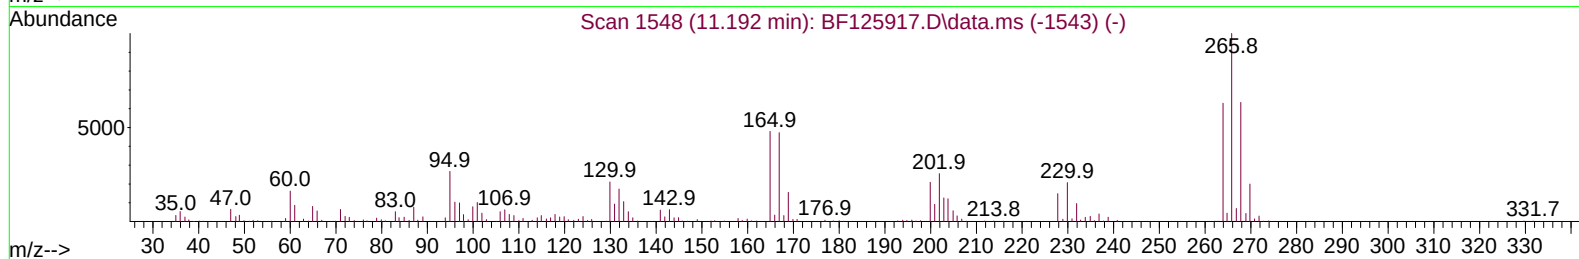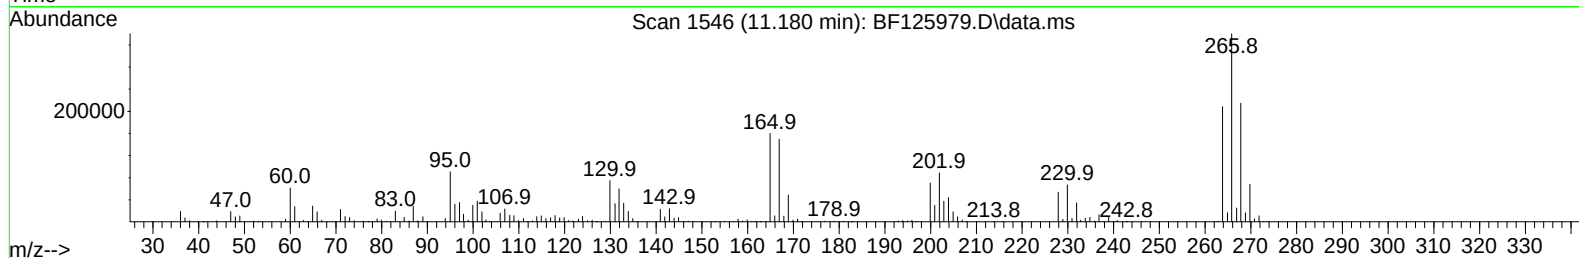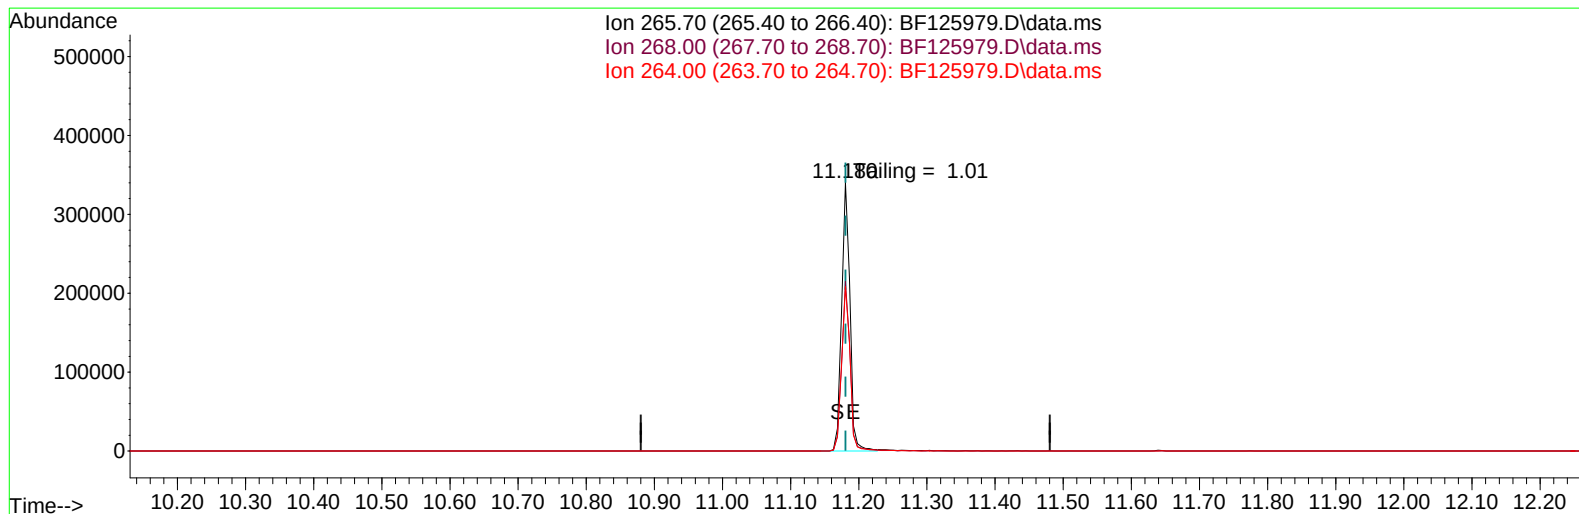

TIC: BF125979.D\data.ms

(70) Pentachlorophenol (C)

11.180min (-0.000) 41462.92 ng

response 291827

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	63.13
264.00	69.90	61.23
0.00	0.00	0.00