


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102821\
 Data File : BF125979.D
 Acq On : 28 Oct 2021 9:14
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 28 12:01:54 2021

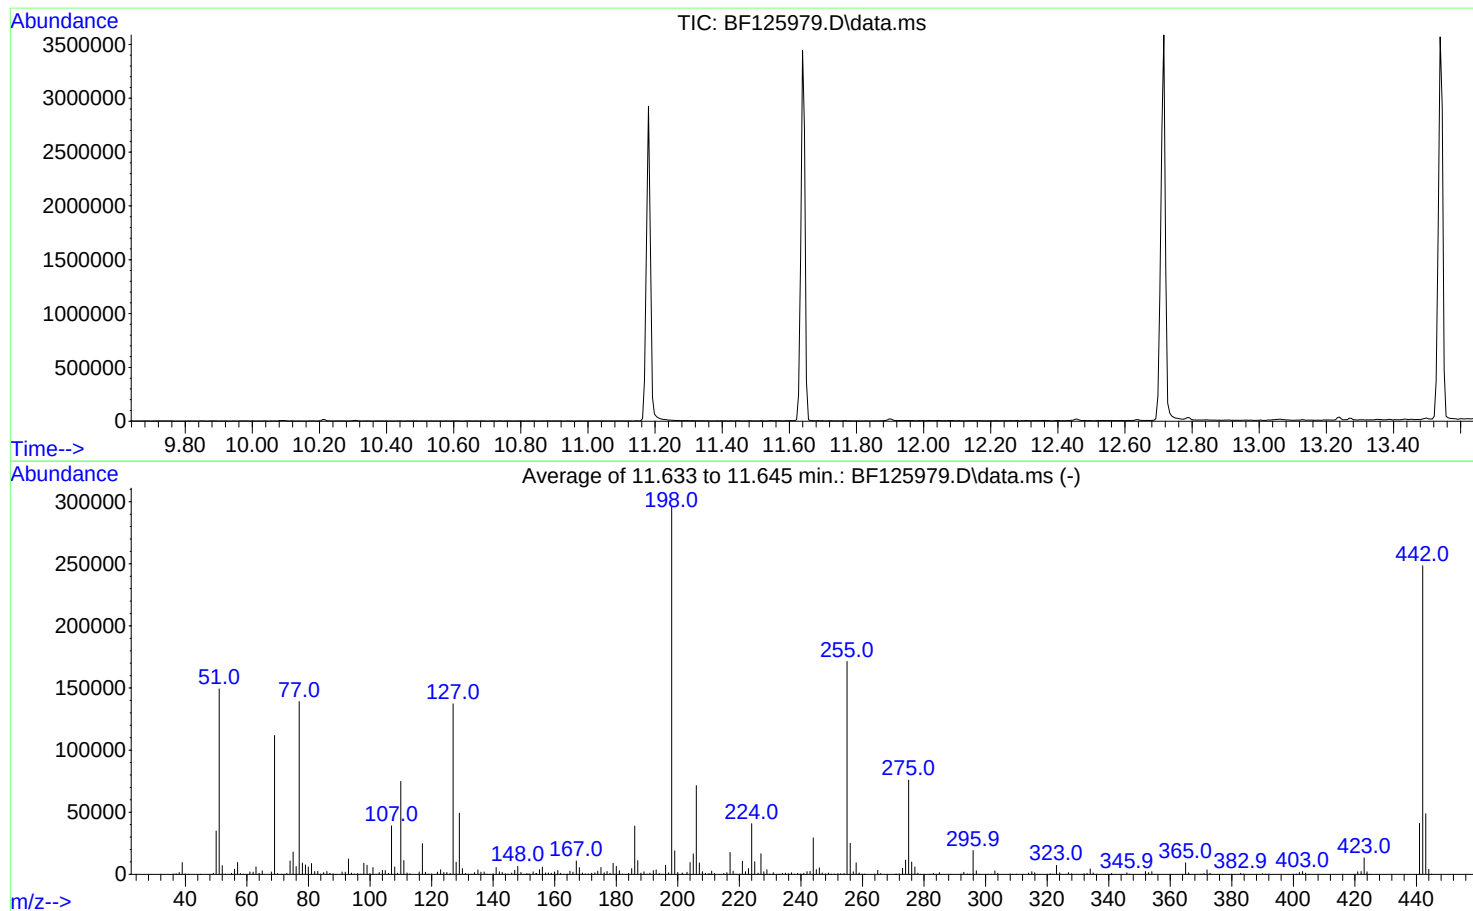




AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.4	149323	PASS
68	69	0.00	2	1.7	1913	PASS
69	198	0.00	100	37.7	111754	PASS
70	69	0.00	2	0.6	668	PASS
127	198	10	80	46.4	137331	PASS
197	198	0.00	2	0.4	1311	PASS
198	198	100	100	100.0	296128	PASS
199	198	5	9	6.4	18989	PASS
275	198	10	60	25.6	75899	PASS
365	198	1	100	3.1	9274	PASS
441	198	0.01	100	13.9	41070	PASS
442	442	50	100	100.0	248443	PASS
443	442	15	24	19.7	48875	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102821\
Data File : BF125979.D
Acq On : 28 Oct 2021 9:14
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 28 12:36:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 28 12:01:54 2021
Response via : Initial Calibration

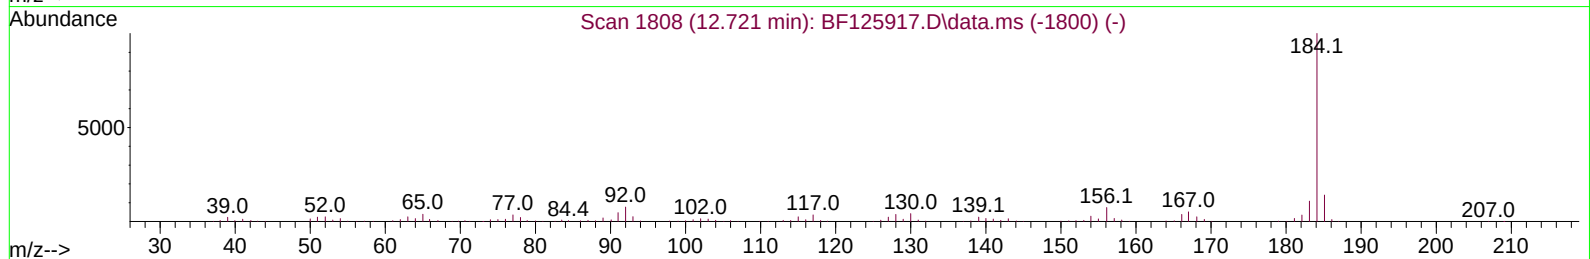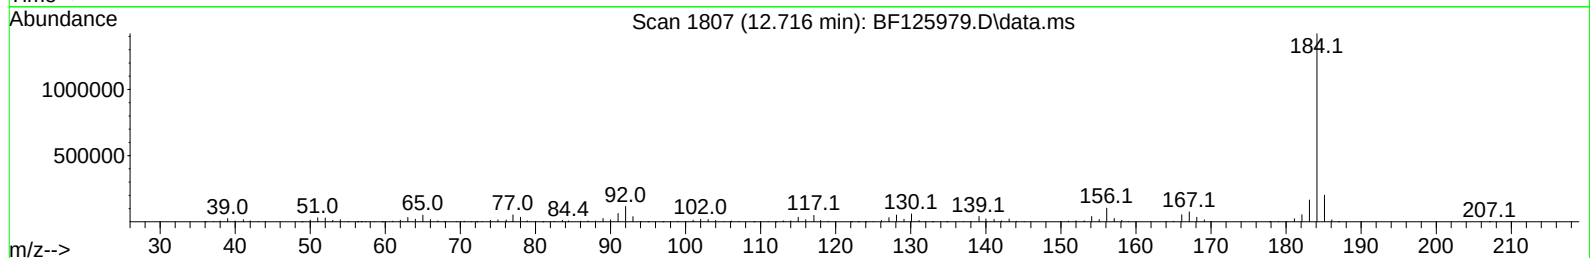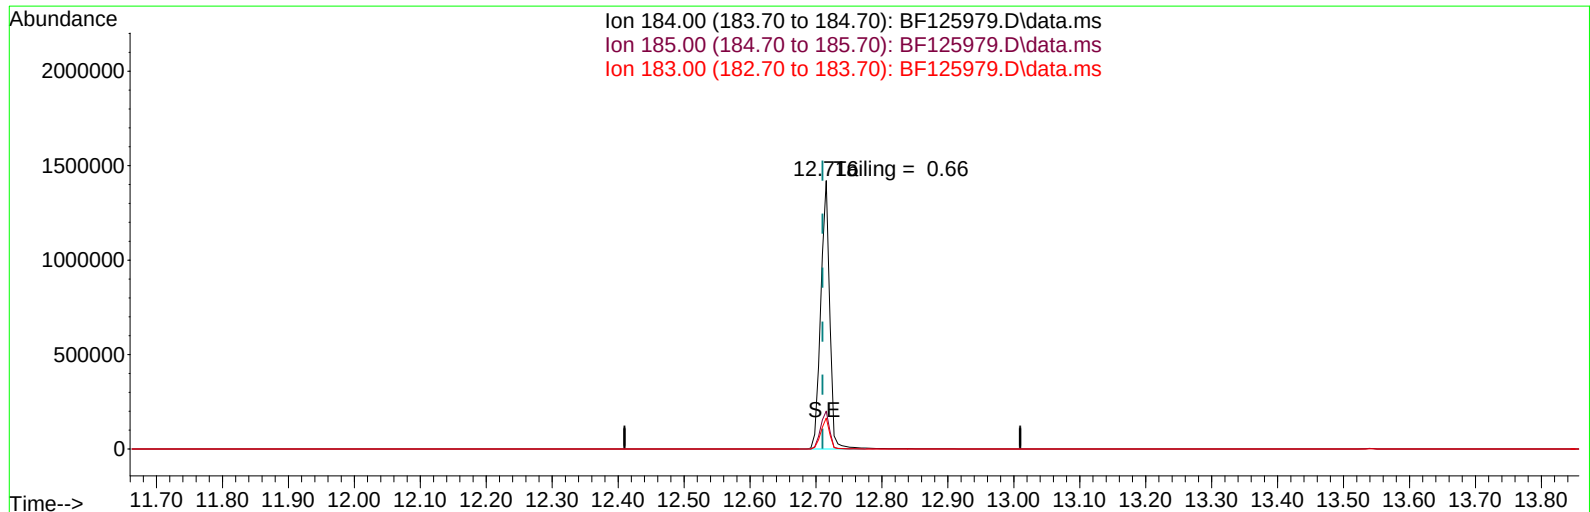

TIC: BF125979.D\data.ms

(77) Benzidine

12.716min (+ 0.006) 0.00 ng




response 1346123

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.17
183.00	10.10	11.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102821\
 Data File : BF125979.D
 Acq On : 28 Oct 2021 9:14
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 28 12:36:48 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 28 12:01:54 2021
 Response via : Initial Calibration

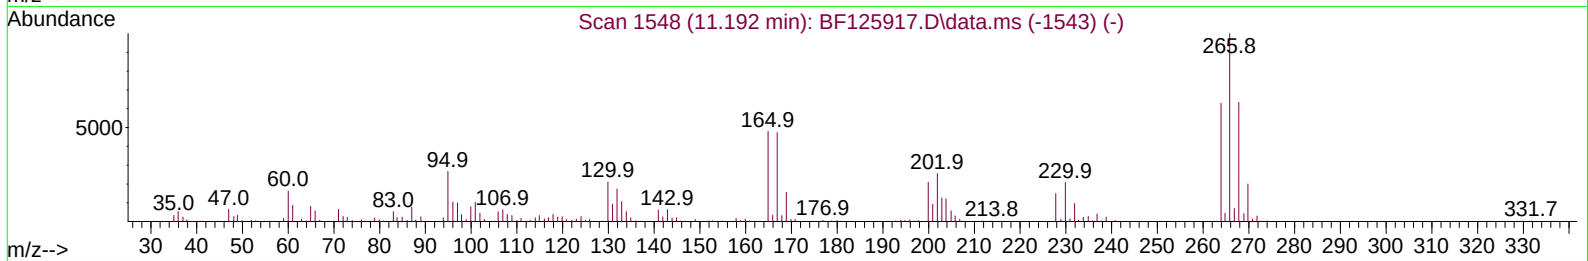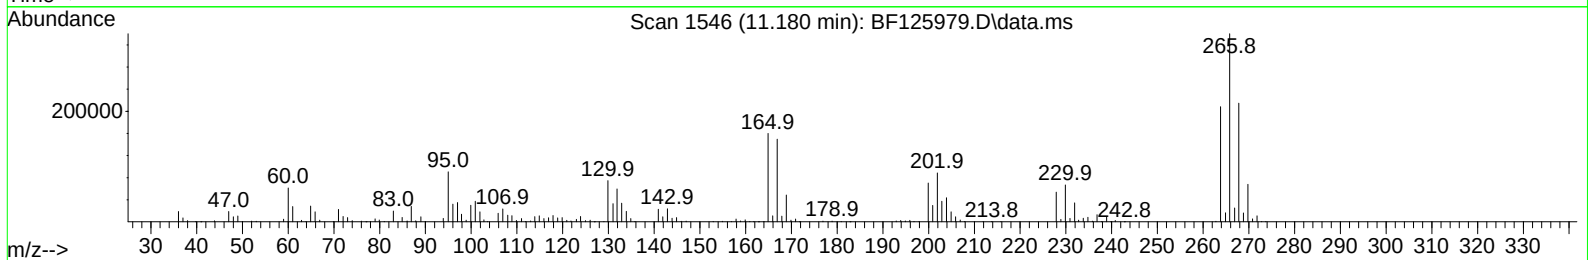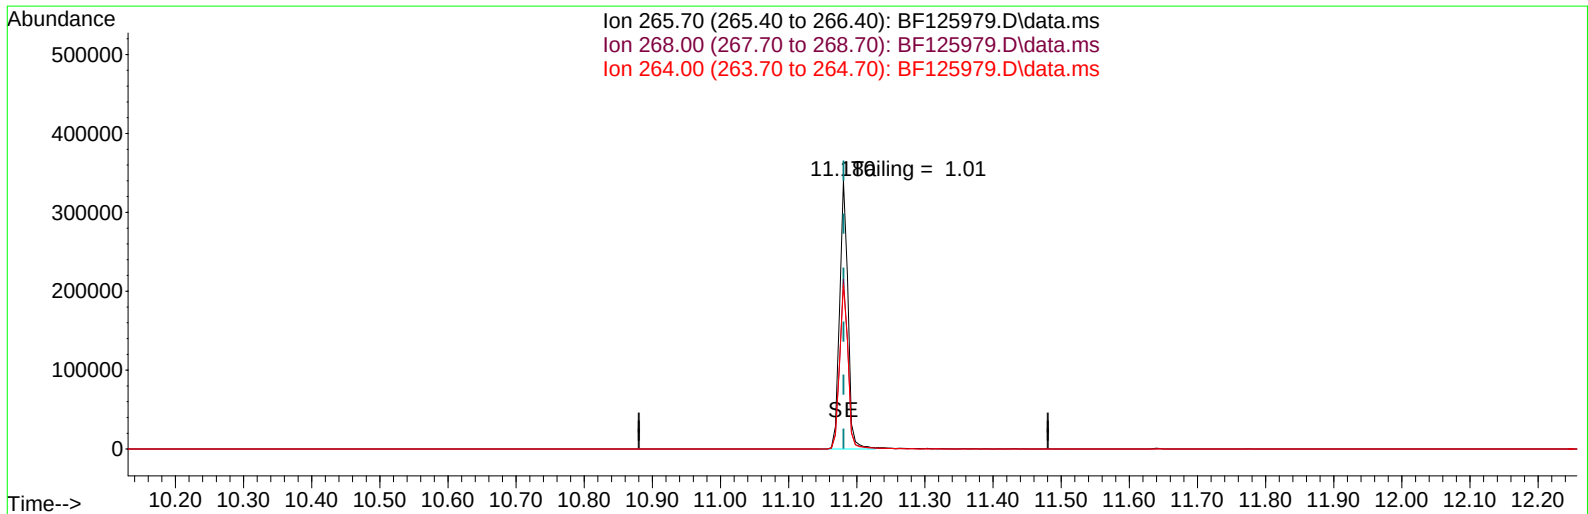

TIC: BF125979.D\data.ms

(70) Pentachlorophenol (C)

11.180min (-0.000) 41462.92 ng

response 291827

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	63.13
264.00	69.90	61.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/28/2021	BNA_F	BF125979.D
Compound Name	Response	Retention Time
DDT	629952	20.53
DDD	5737	20.23
DDE	724	19.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6461	636413	1.02