
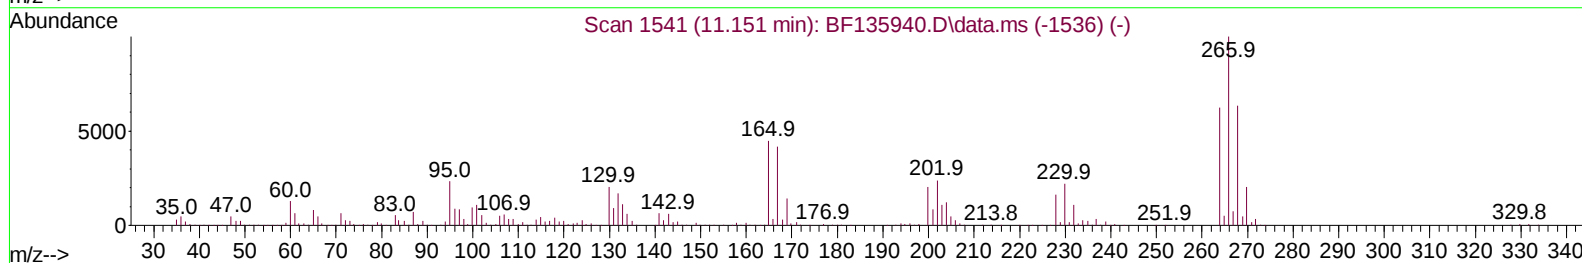
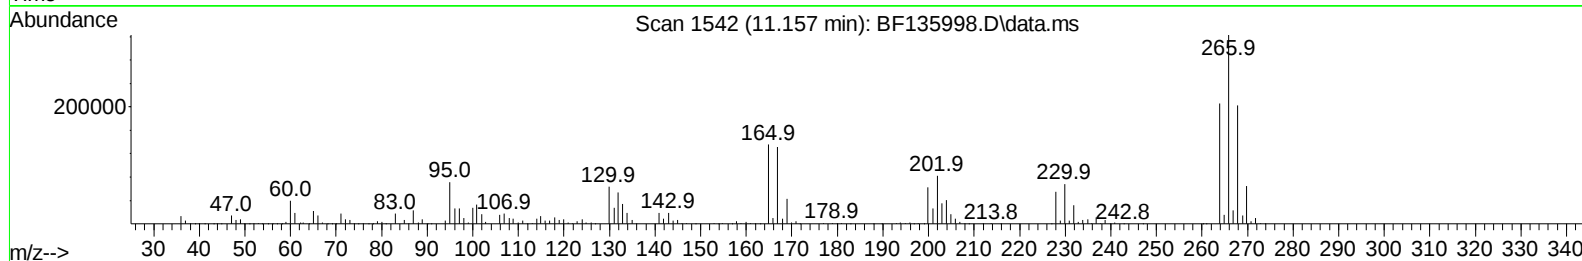


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102823\
Data File : BF135998.D
Acq On : 28 Oct 2023 11:26
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 11:57:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 26 03:58:01 2023
Response via : Initial Calibration

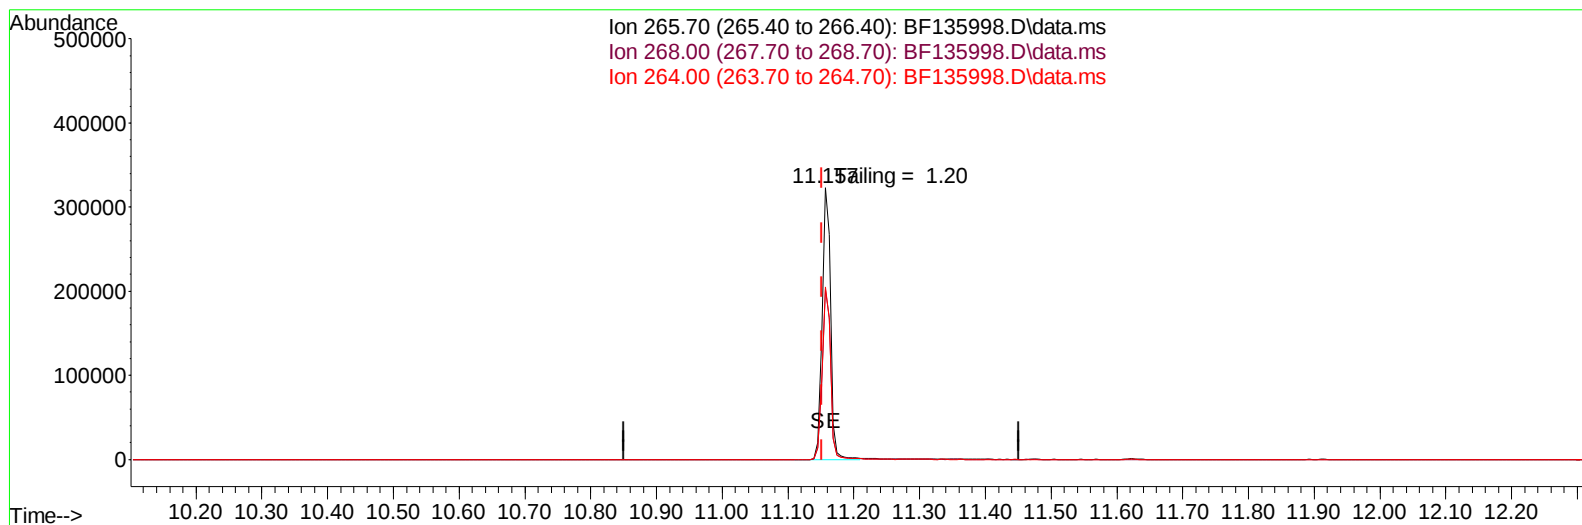

TIC: BF135998.D\data.ms

(70) Pentachlorophenol (C)




11.157min (+ 0.006) 614157.86 ng

response 292332

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	62.64
264.00	62.20	63.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102823\
Data File : BF135998.D
Acq On : 28 Oct 2023 11:26
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 11:57:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 26 03:58:01 2023
Response via : Initial Calibration

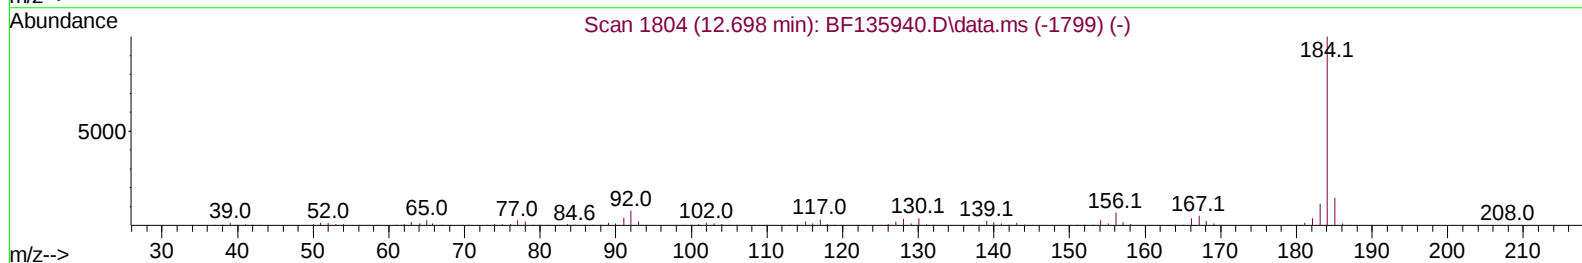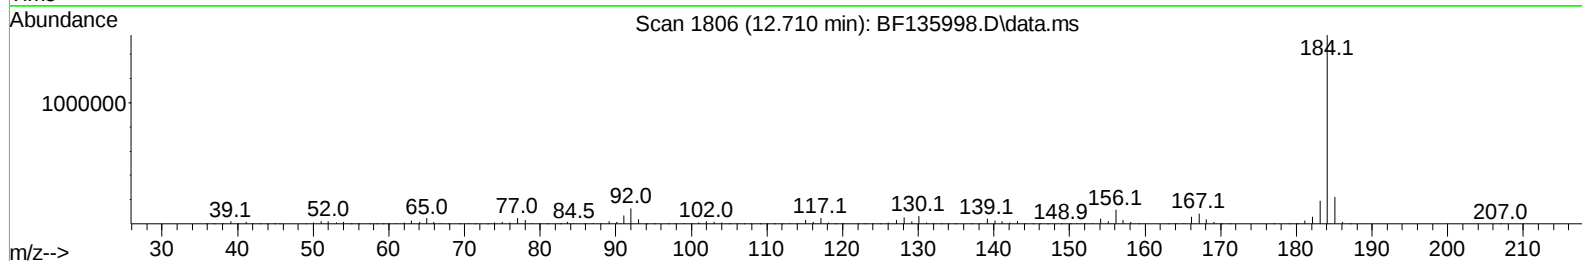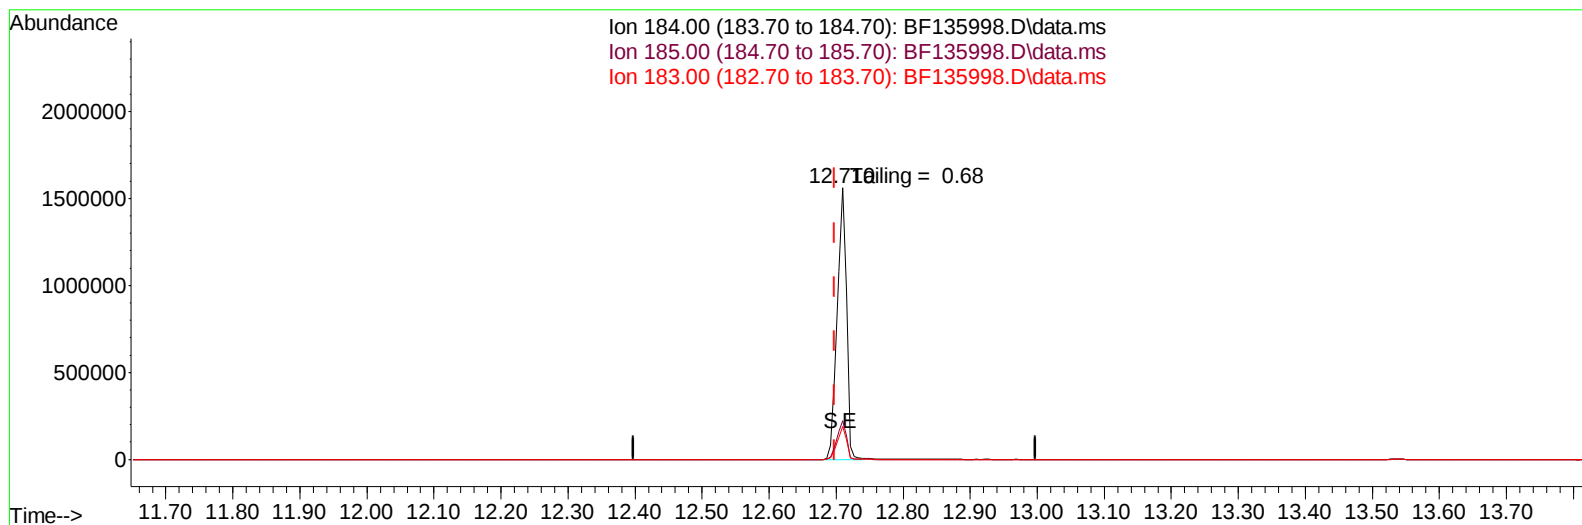

TIC: BF135998.D\data.ms

(77) Benzidine**12.710min (+ 0.012) 131097.97 ng****response 1516716**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.19
183.00	11.50	12.07
0.00	0.00	0.00