


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102823\
Data File : BF135998.D
Acq On : 28 Oct 2023 11:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 26 03:58:01 2023

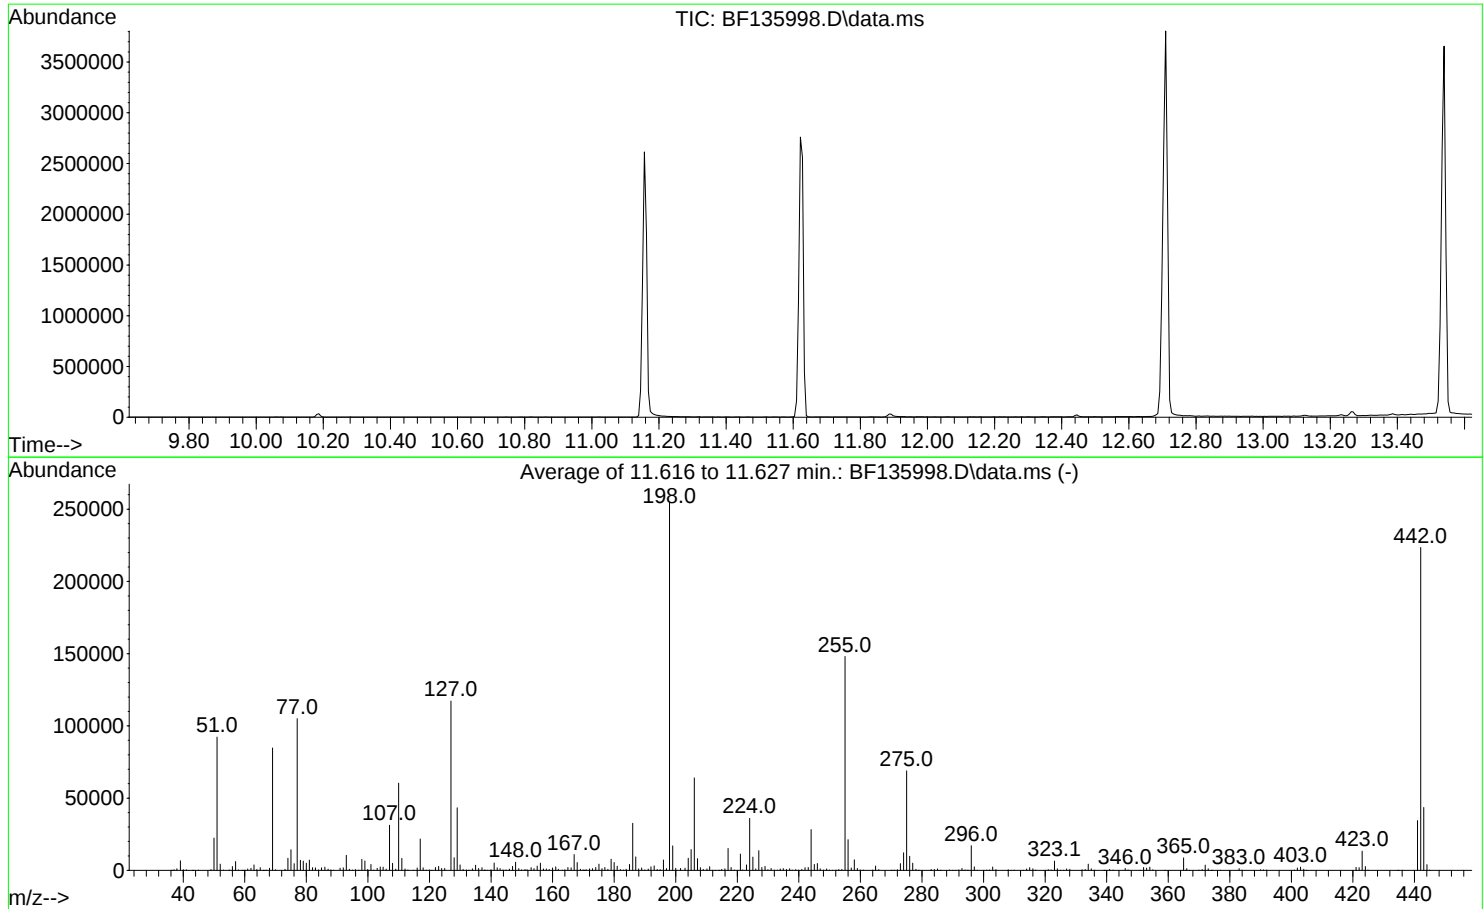




AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	92253	PASS
68	69	0.00	2	1.7	1425	PASS
69	198	0.00	100	33.3	84781	PASS
70	69	0.00	2	0.5	464	PASS
127	198	10	80	46.0	117224	PASS
197	198	0.00	2	0.5	1184	PASS
198	198	100	100	100.0	254635	PASS
199	198	5	9	6.7	16965	PASS
275	198	10	60	27.1	68939	PASS
365	198	1	100	3.4	8592	PASS
441	198	0.01	100	13.5	34501	PASS
442	442	50	100	100.0	223520	PASS
443	442	15	24	19.5	43557	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102823\
Data File : BF135998.D
Acq On : 28 Oct 2023 11:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 28 11:57:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 26 03:58:01 2023
Response via : Initial Calibration

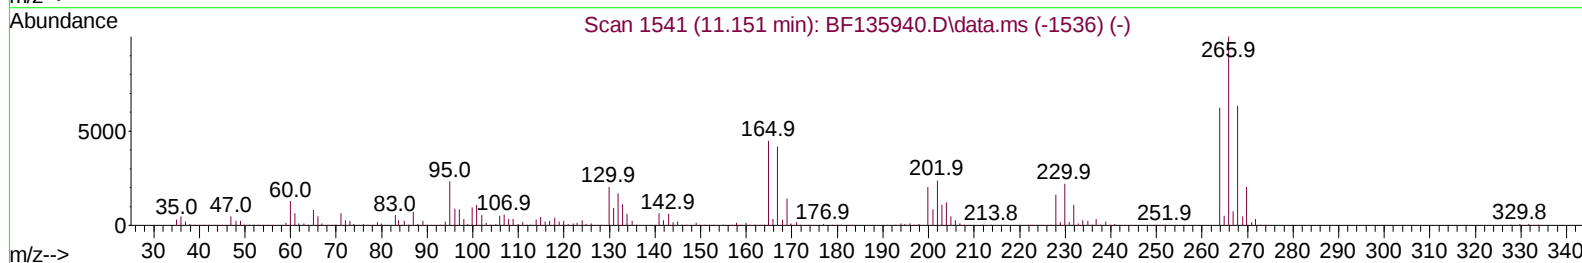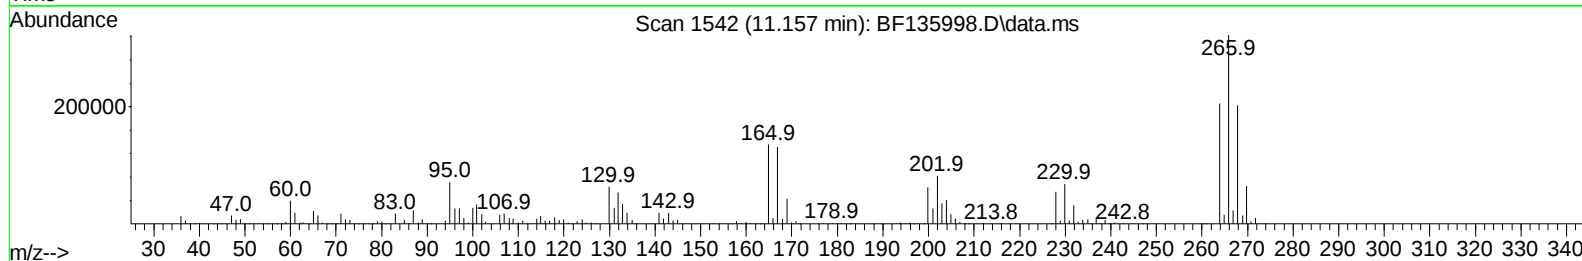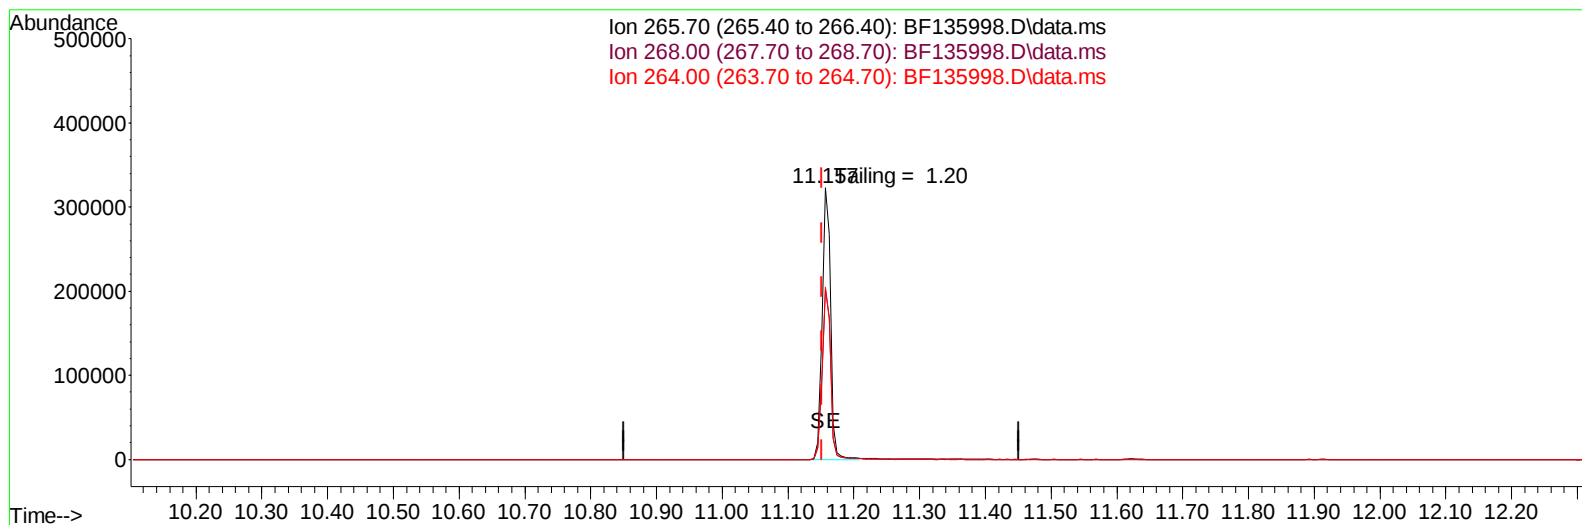

TIC: BF135998.D\data.ms

(70) Pentachlorophenol (C)

11.157min (+ 0.006) 614157.86 ng




response 292332

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	62.64
264.00	62.20	63.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102823\
Data File : BF135998.D
Acq On : 28 Oct 2023 11:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 28 11:57:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 26 03:58:01 2023
Response via : Initial Calibration

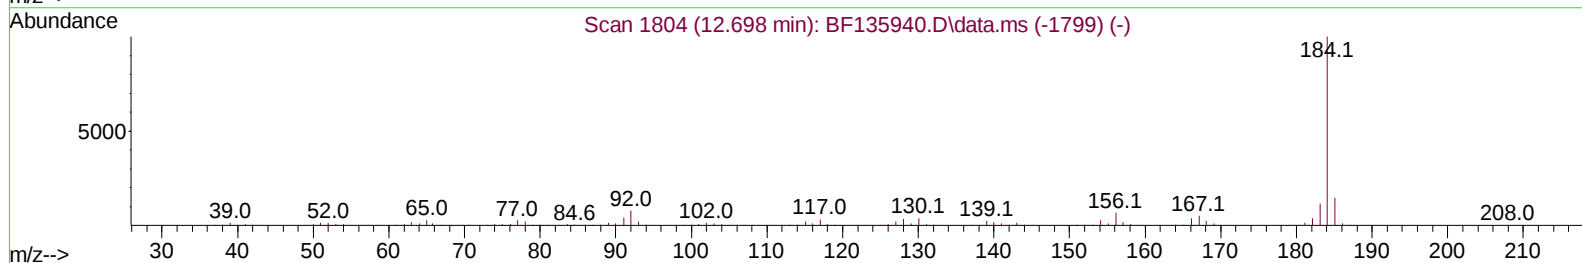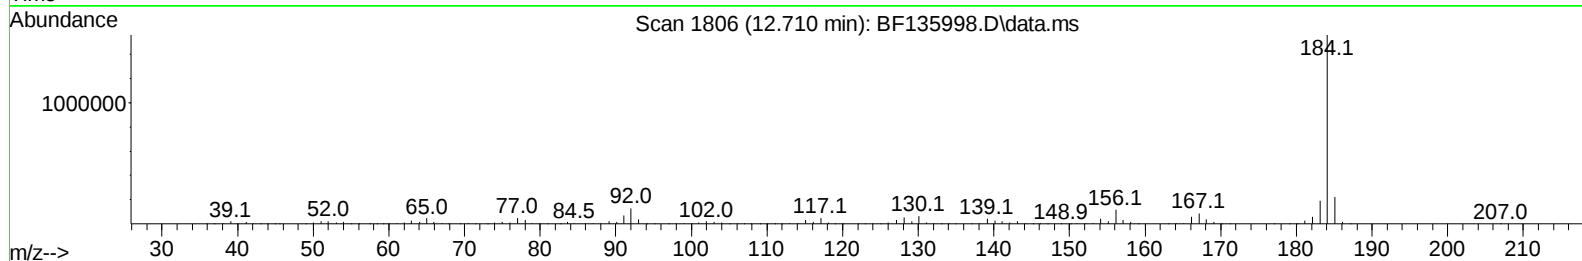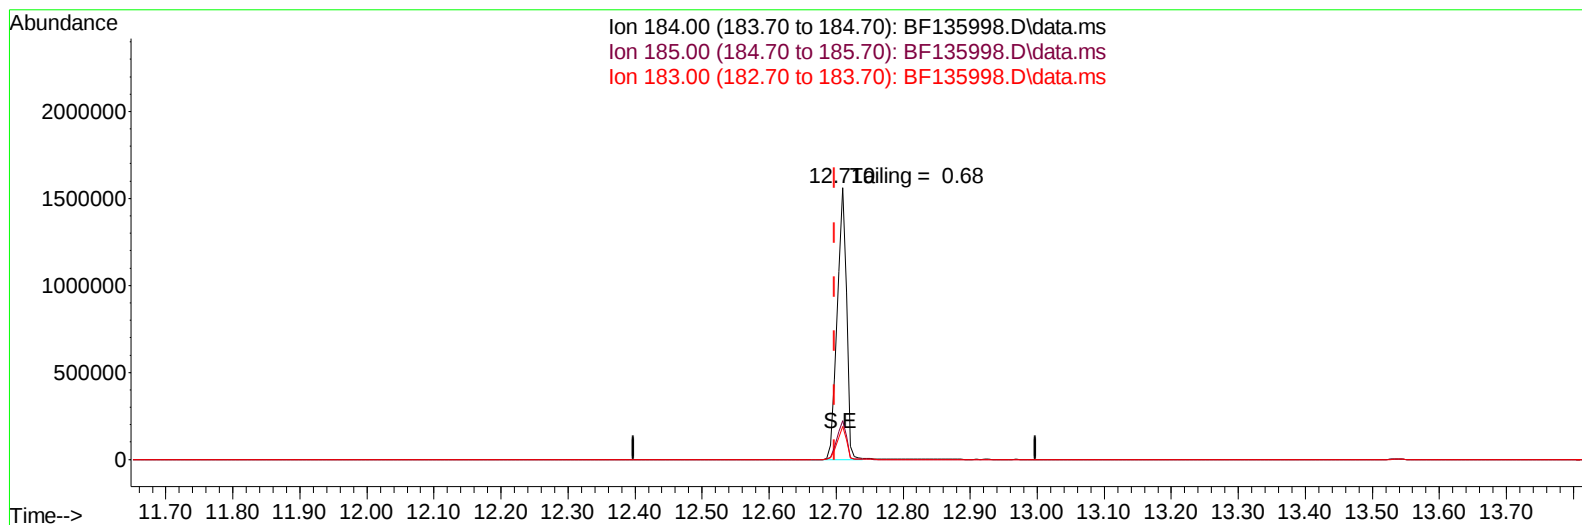

TIC: BF135998.D\data.ms

(77) Benzidine

12.710min (+ 0.012) 131097.97 ng

response 1516716

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.19
183.00	11.50	12.07
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/28/2023	BNA_F	<u>BF135998.D</u>
Compound Name	Response	Retention Time
DDT	649862	13.539
DDD	8425	13.263
DDE	389	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8814	658676	1.34

Instrument :
BNA_F
ClientSampleId :
DFTPP