

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102824\
 Data File : BF140079.D
 Acq On : 28 Oct 2024 11:31
 Operator : RC/JU
 Sample : PB164444BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB164444BL

Quant Time: Oct 28 12:04:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 18 15:07:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.886	152	122619	20.000	ng	0.00
21) Naphthalene-d8	8.169	136	482544	20.000	ng	0.00
39) Acenaphthene-d10	9.922	164	271379	20.000	ng	0.00
64) Phenanthrene-d10	11.410	188	481831	20.000	ng	0.00
76) Chrysene-d12	14.045	240	230845	20.000	ng	0.00
86) Perylene-d12	15.527	264	282080	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.516	112	938931	119.874	ng	0.02
7) Phenol-d6	6.510	99	1179585	116.278	ng	0.00
23) Nitrobenzene-d5	7.445	82	780064	89.596	ng	0.00
42) 2,4,6-Tribromophenol	10.710	330	319315	125.794	ng	0.00
45) 2-Fluorobiphenyl	9.245	172	1416027	86.236	ng	0.00
79) Terphenyl-d14	12.998	244	1362075	96.146	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102824\
Data File : BF140079.D
Acq On : 28 Oct 2024 11:31
Operator : RC/JU
Sample : PB164444BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164444BL

Quant Time: Oct 28 12:04:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration




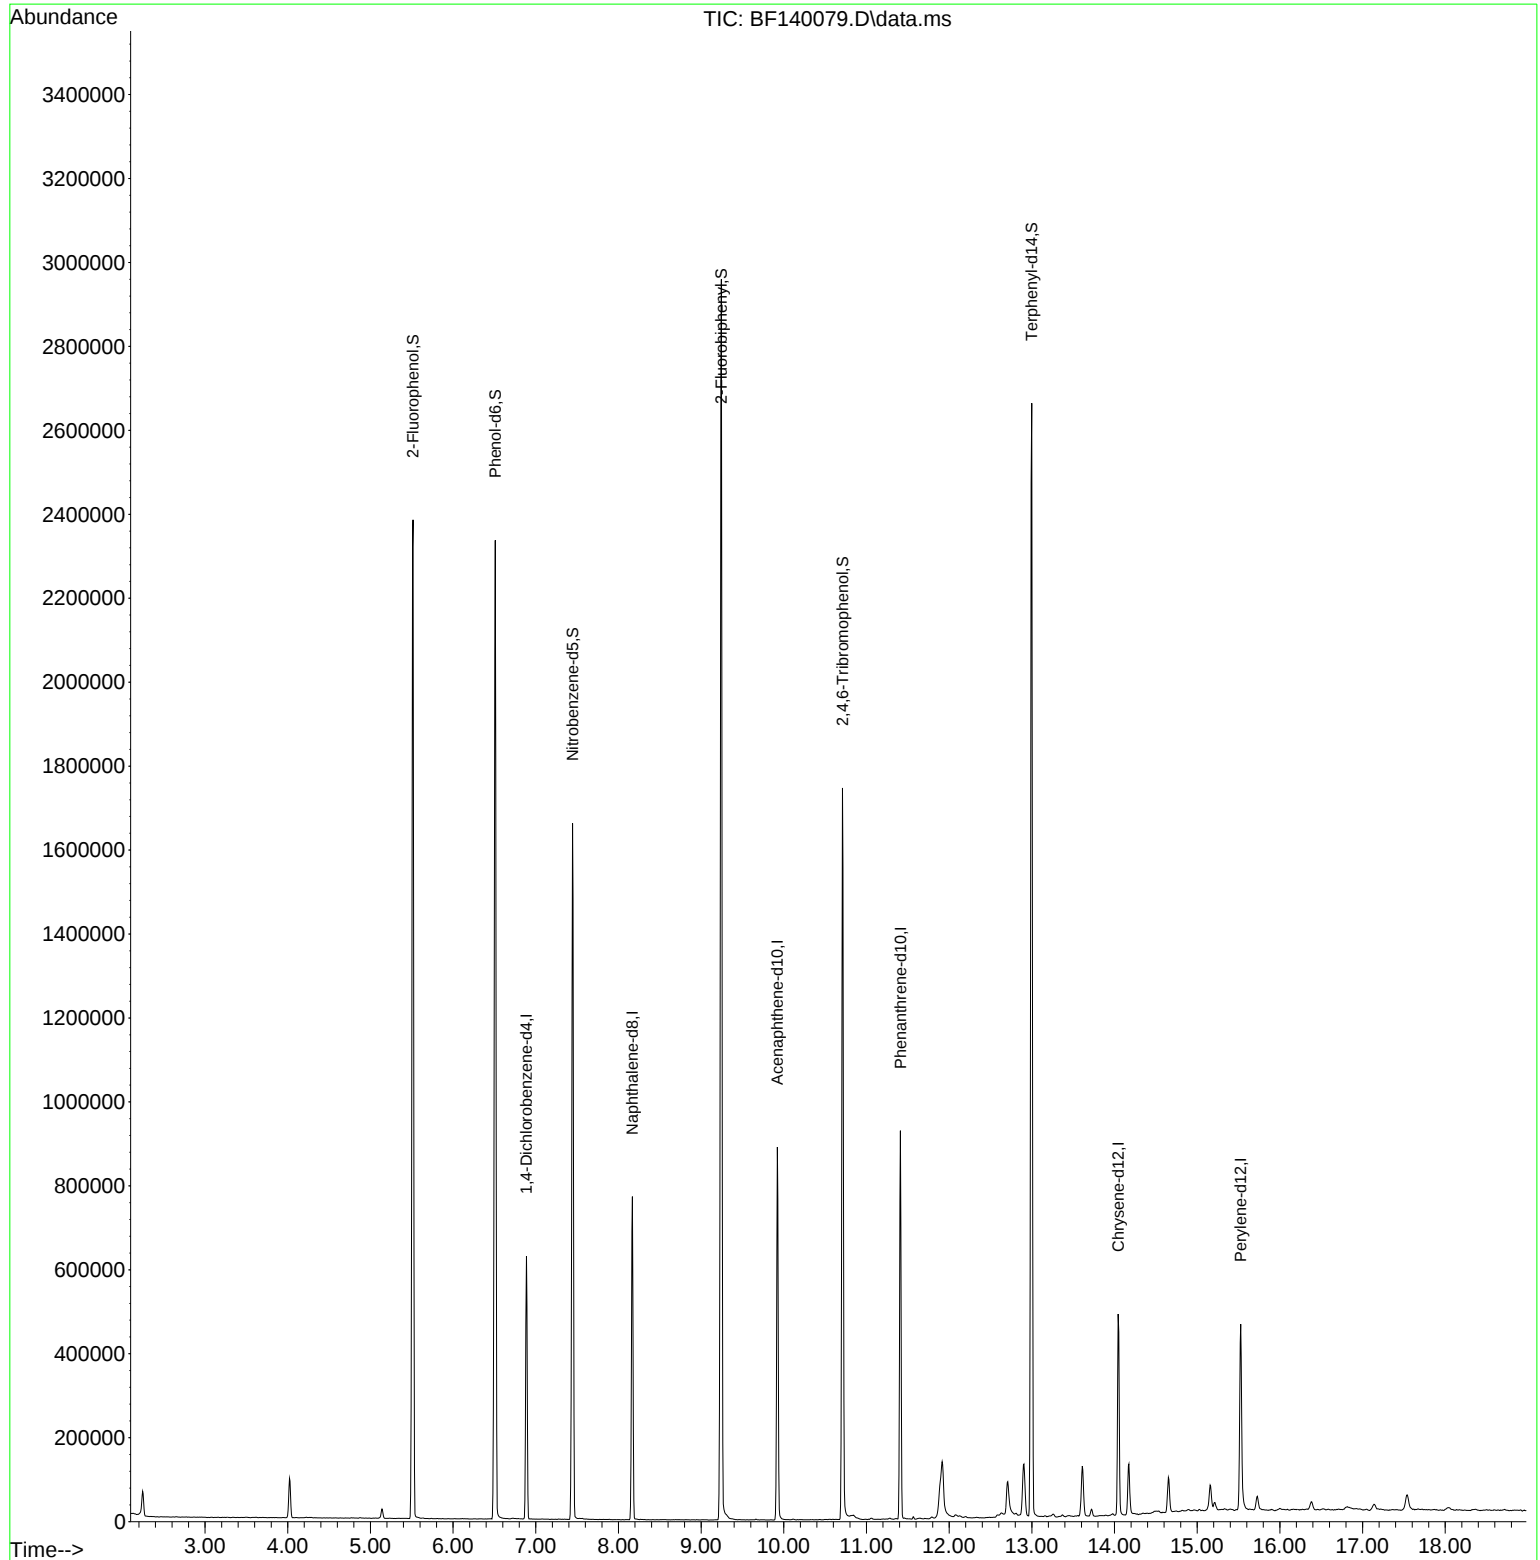


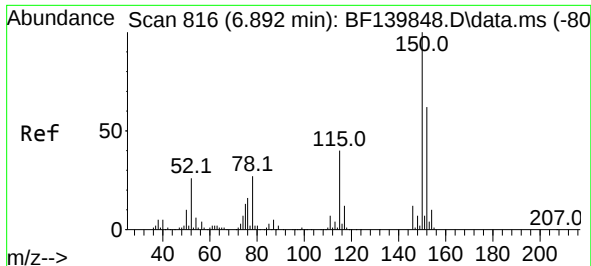

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.886 min Scan# 816
Delta R.T. -0.006 min
Lab File: BF140079.D
Acq: 28 Oct 2024 11:31




Instrument :
BNA_F
ClientSampleId :
PB164444BL


Tgt Ion:152 Resp: 122619
Ion Ratio Lower Upper
152 100
150 158.4 130.2 195.2
115 65.1 51.4 77.2

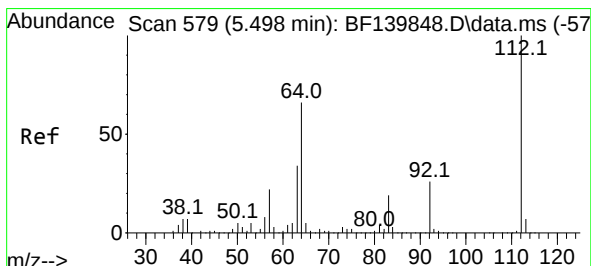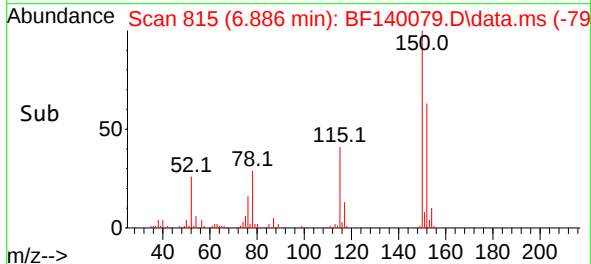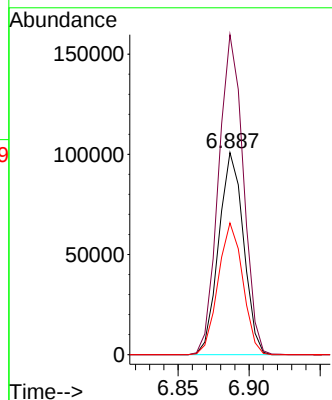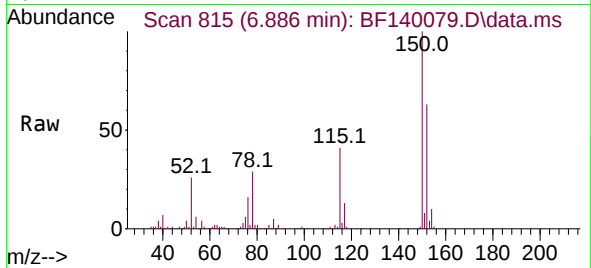

#5
2-Fluorophenol
Concen: 119.874 ng
RT: 5.516 min Scan# 582
Delta R.T. 0.018 min
Lab File: BF140079.D
Acq: 28 Oct 2024 11:31

Tgt Ion:112 Resp: 938931
Ion Ratio Lower Upper
112 100
64 63.3 53.0 79.6
63 33.4 27.0 40.4


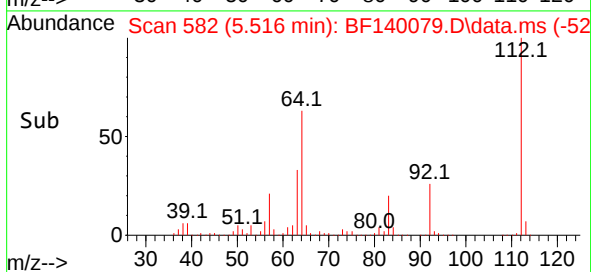
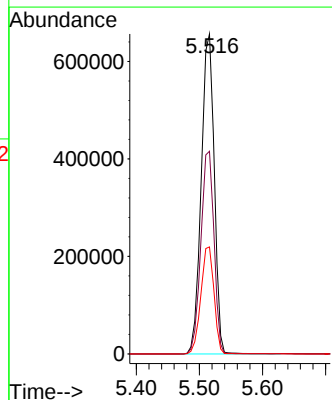
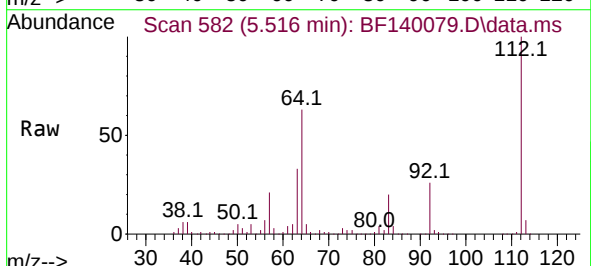


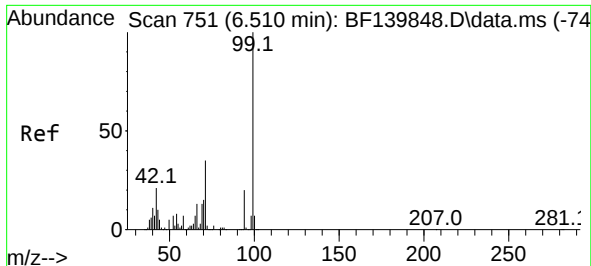

#7
Phenol-d6
Concen: 116.278 ng
RT: 6.510 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF140079.D
Acq: 28 Oct 2024 11:31




Instrument :
BNA_F
ClientSampleId :
PB164444BL


Tgt Ion: 99 Resp: 1179585
Ion Ratio Lower Upper
99 100
42 19.8 16.7 25.1
71 35.6 27.7 41.5

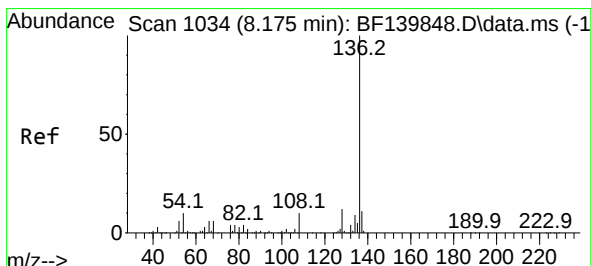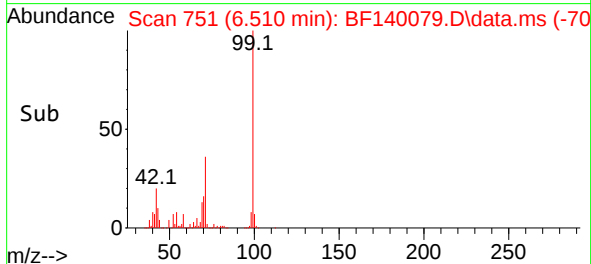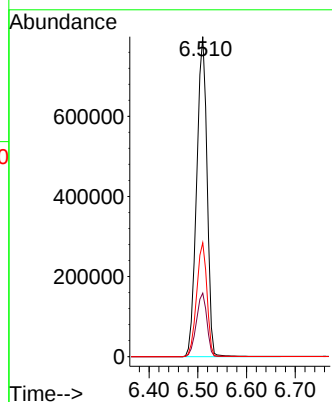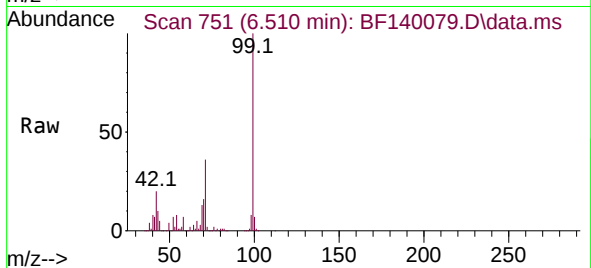

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.169 min Scan# 1033
Delta R.T. -0.006 min
Lab File: BF140079.D
Acq: 28 Oct 2024 11:31

Tgt Ion:136 Resp: 482544
Ion Ratio Lower Upper
136 100
137 10.8 8.6 12.8
54 9.6 8.4 12.6
68 5.9 5.1 7.7


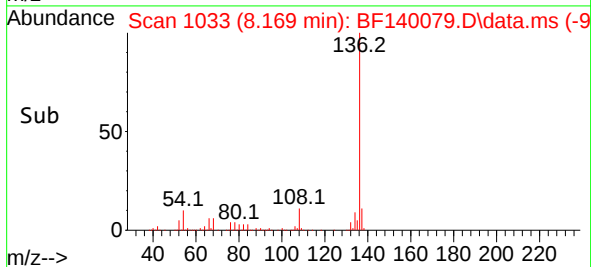
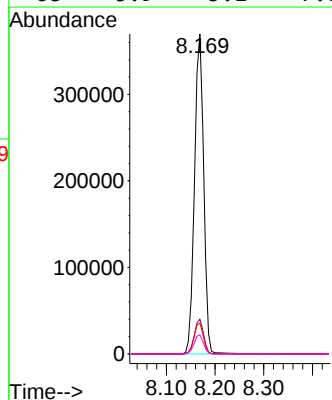
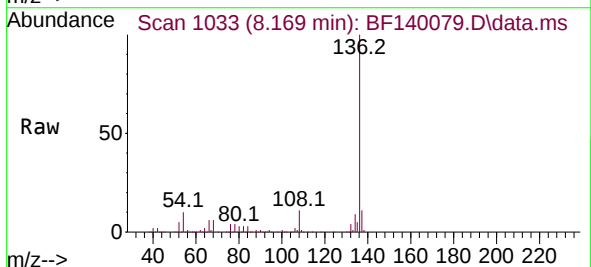


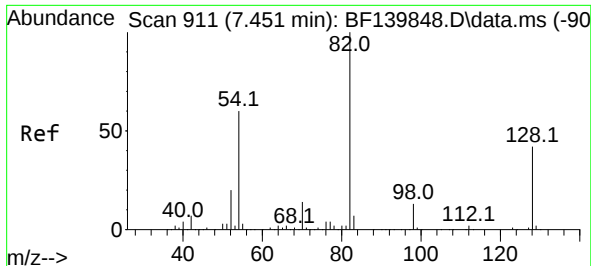

#23
Nitrobenzene-d5
Concen: 89.596 ng
RT: 7.445 min Scan# 911
Delta R.T. -0.006 min
Lab File: BF140079.D
Acq: 28 Oct 2024 11:31




Instrument :
BNA_F
ClientSampleId :
PB164444BL


Tgt Ion: 82 Resp: 780064
Ion Ratio Lower Upper
82 100
128 42.3 33.4 50.0
54 57.7 47.8 71.8

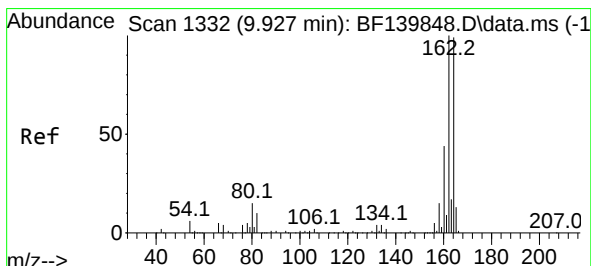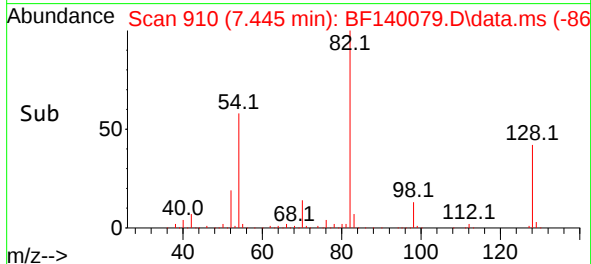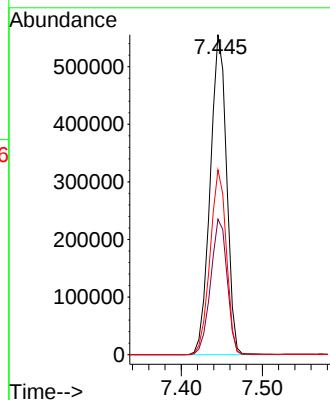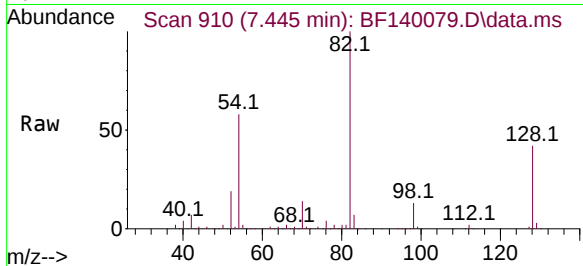

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.922 min Scan# 1331
Delta R.T. -0.005 min
Lab File: BF140079.D
Acq: 28 Oct 2024 11:31


Tgt Ion:164 Resp: 271379
Ion Ratio Lower Upper
164 100
162 101.7 81.0 121.4
160 44.7 35.4 53.0

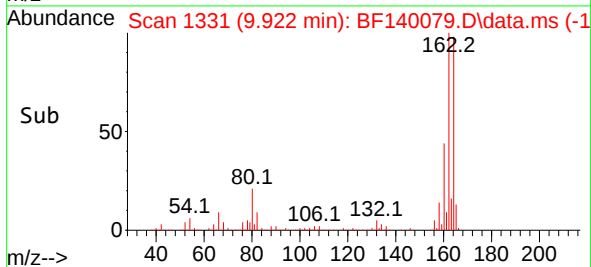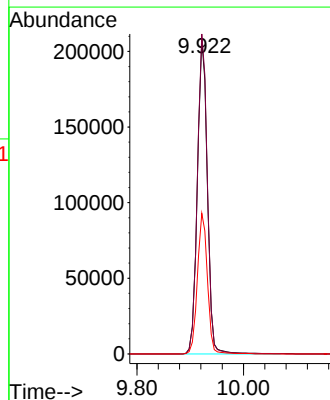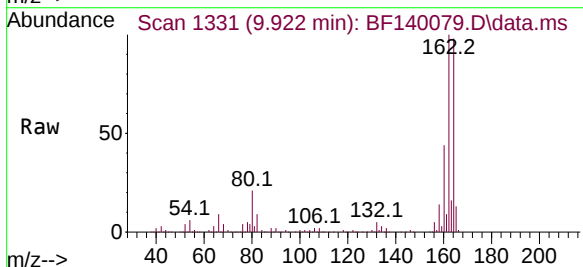



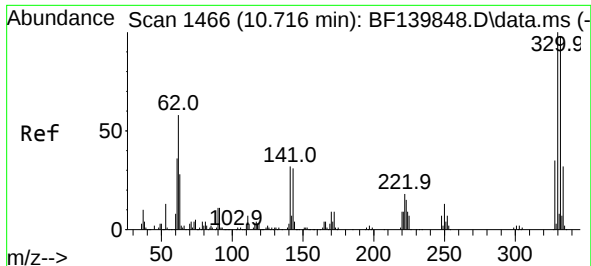


#42
2,4,6-Tribromophenol
Concen: 125.794 ng
RT: 10.710 min Scan# 1465
Delta R.T. -0.006 min
Lab File: BF140079.D
Acq: 28 Oct 2024 11:31

Instrument :
BNA_F
ClientSampleId :
PB164444BL



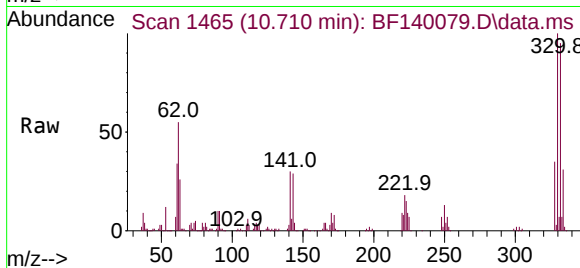



Tgt Ion:330 Resp: 319315
Ion Ratio Lower Upper
330 100
332 95.4 78.1 117.1
141 29.1 26.6 39.8

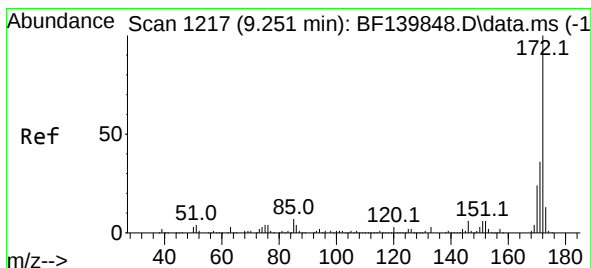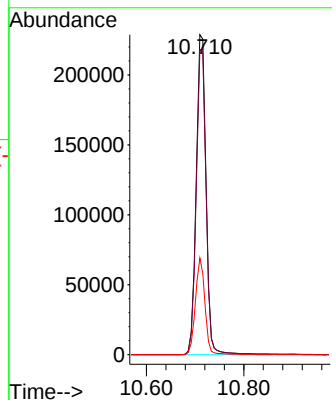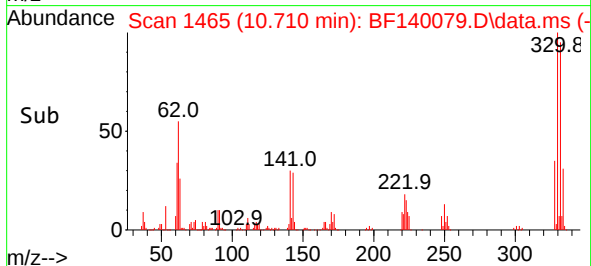

#45
2-Fluorobiphenyl
Concen: 86.236 ng
RT: 9.245 min Scan# 1216
Delta R.T. -0.006 min
Lab File: BF140079.D
Acq: 28 Oct 2024 11:31

Tgt Ion:172 Resp: 1416027
Ion Ratio Lower Upper
172 100
171 35.9 28.6 43.0
170 23.9 19.1 28.7


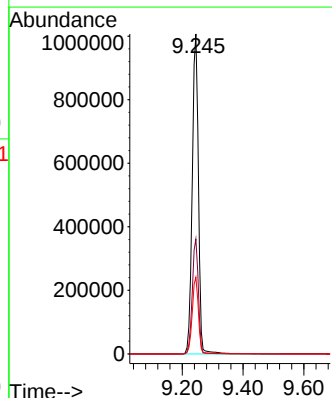
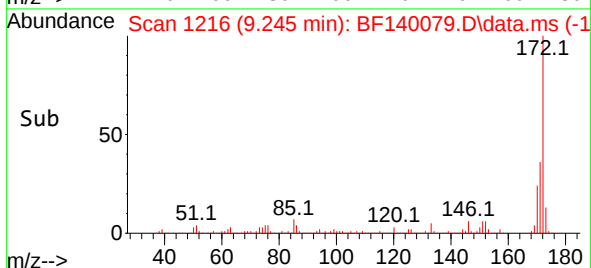
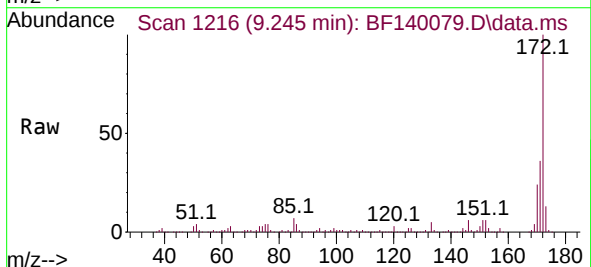


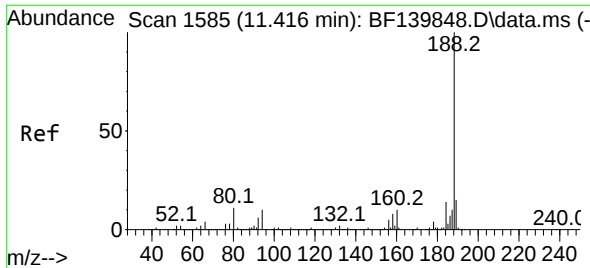

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.410 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF140079.D
Acq: 28 Oct 2024 11:31




Instrument :
BNA_F
ClientSampleId :
PB164444BL


Tgt Ion:188 Resp: 481831
Ion Ratio Lower Upper
188 100
94 9.5 7.9 11.9
80 10.5 9.0 13.4

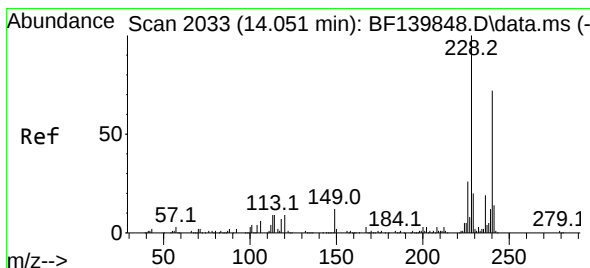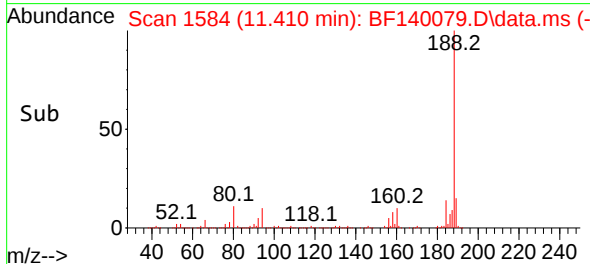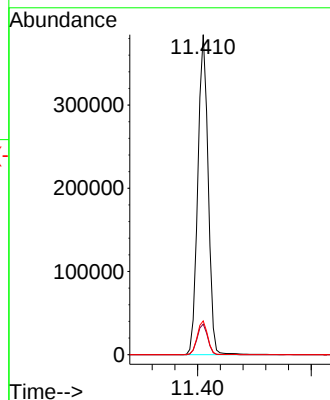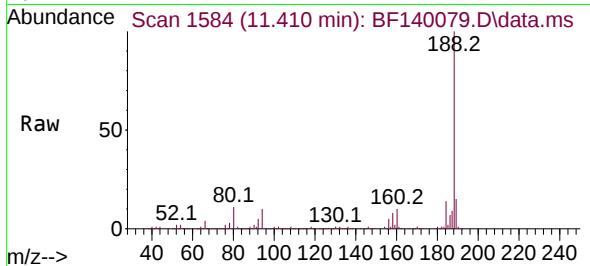

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.045 min Scan# 2032
Delta R.T. -0.006 min
Lab File: BF140079.D
Acq: 28 Oct 2024 11:31


Tgt Ion:240 Resp: 230845
Ion Ratio Lower Upper
240 100
120 11.1 9.4 14.2
236 26.2 20.9 31.3

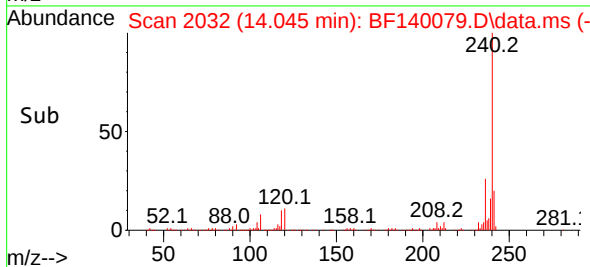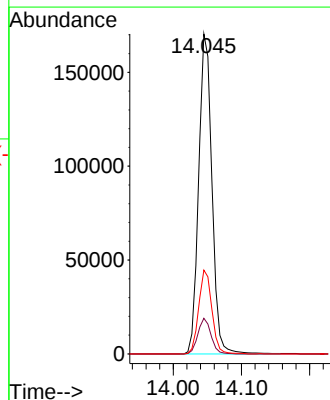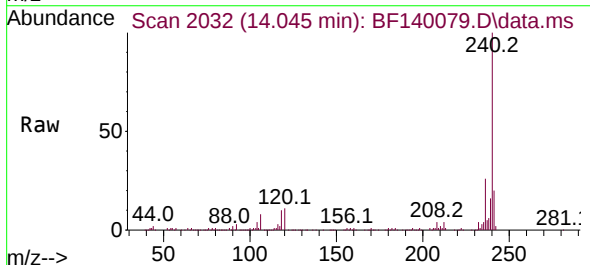



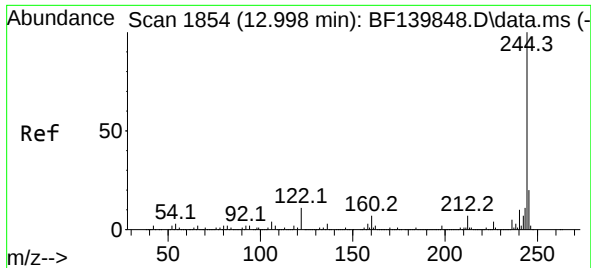


#79
 Terphenyl-d14
 Concen: 96.146 ng
 RT: 12.998 min Scan# 1854
 Delta R.T. 0.000 min
 Lab File: BF140079.D
 Acq: 28 Oct 2024 11:31

Instrument :
 BNA_F
 ClientSampleId :
 PB164444BL

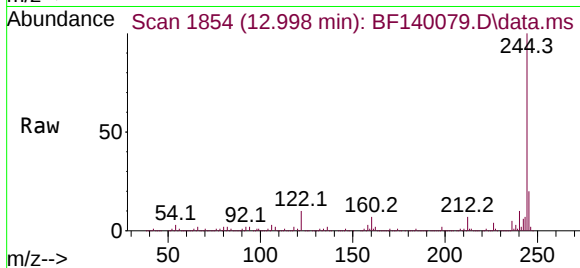

Tgt Ion:244 Resp: 1362075
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.7 8.5
 122 10.0 8.6 13.0

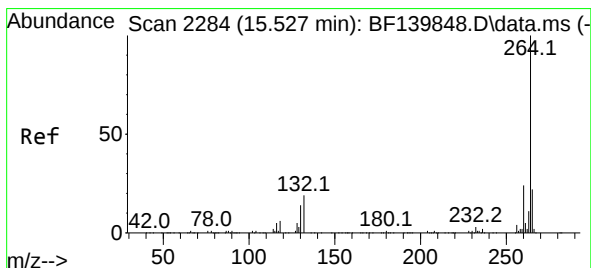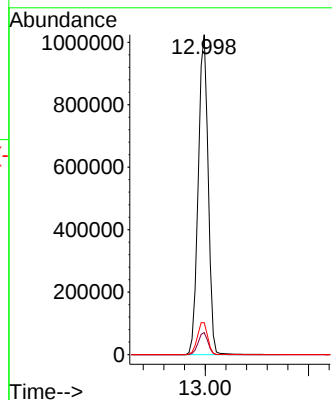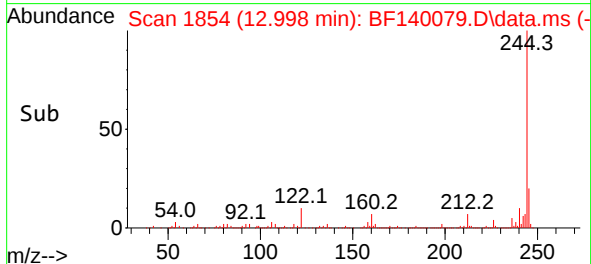

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.527 min Scan# 2284
 Delta R.T. 0.000 min
 Lab File: BF140079.D
 Acq: 28 Oct 2024 11:31

Tgt Ion:264 Resp: 282080
 Ion Ratio Lower Upper
 264 100
 260 23.7 19.4 29.2
 265 21.5 17.4 26.0

