


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102825\
Data File : BF144096.D
Acq On : 28 Oct 2025 12:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 24 17:30:25 2025

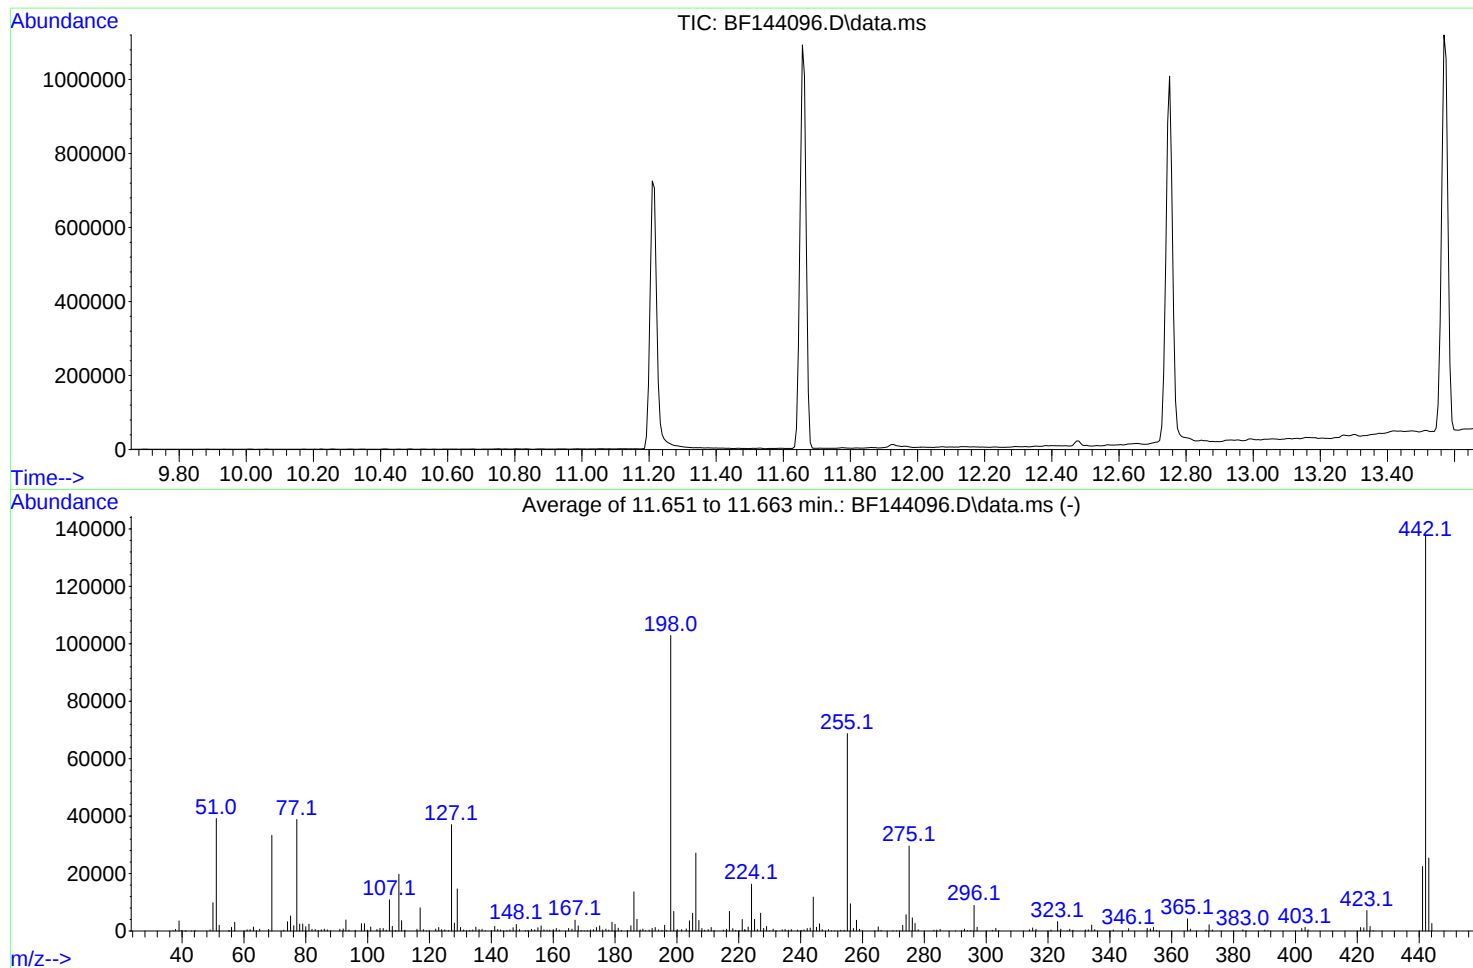

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	551	PASS
69	69	100	100	100.0	33349	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	102923	PASS
199	198	5	9	6.6	6806	PASS
365	198	1	100	4.1	4261	PASS
441	443	0.01	150	88.4	22452	PASS
442	442	100	100	100.0	137480	PASS
443	442	15	24	18.5	25399	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/28/2025	BNA_F	<u>BF144096.D</u>
Compound Name	Response	Retention Time
DDT	289356	13.569
DDD	3978	13.274
DDE	557	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4535	293891	1.54

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102825\
Data File : BF144096.D
Acq On : 28 Oct 2025 12:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 28 14:08:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 17:30:25 2025
Response via : Initial Calibration

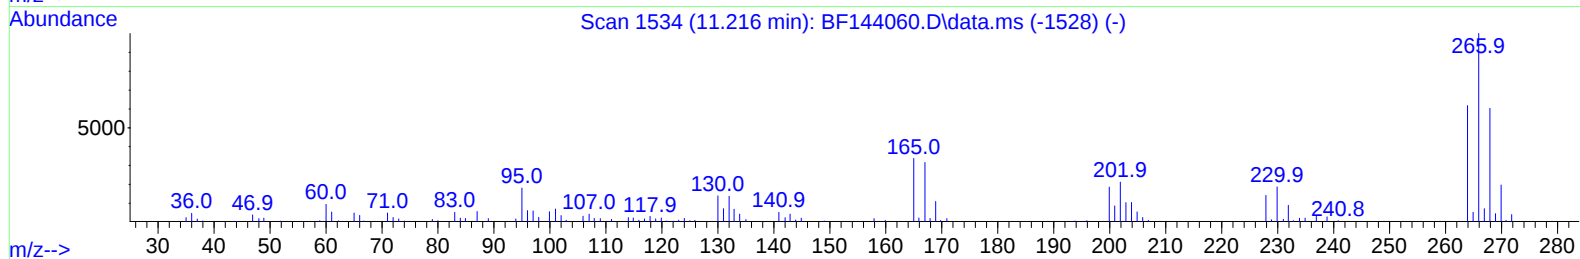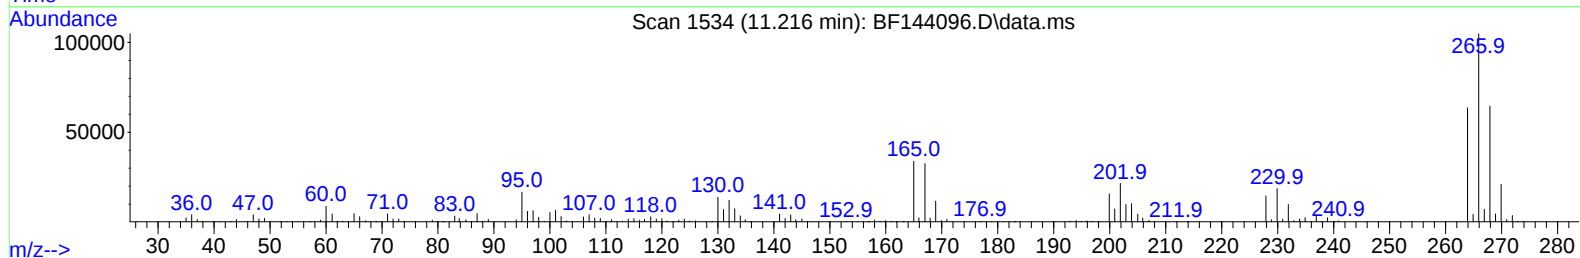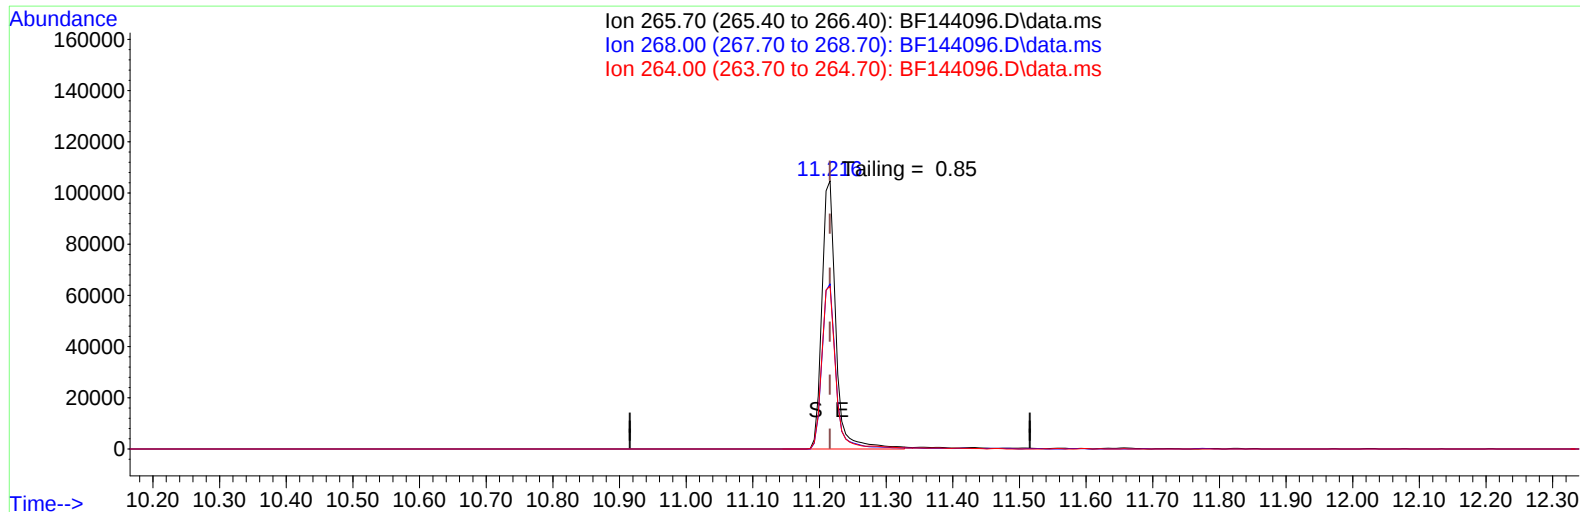

TIC: BF144096.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.000) 40706.49 ng m




response 152337

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.30	61.51
264.00	61.70	60.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102825\
Data File : BF144096.D
Acq On : 28 Oct 2025 12:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 28 14:08:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 17:30:25 2025
Response via : Initial Calibration

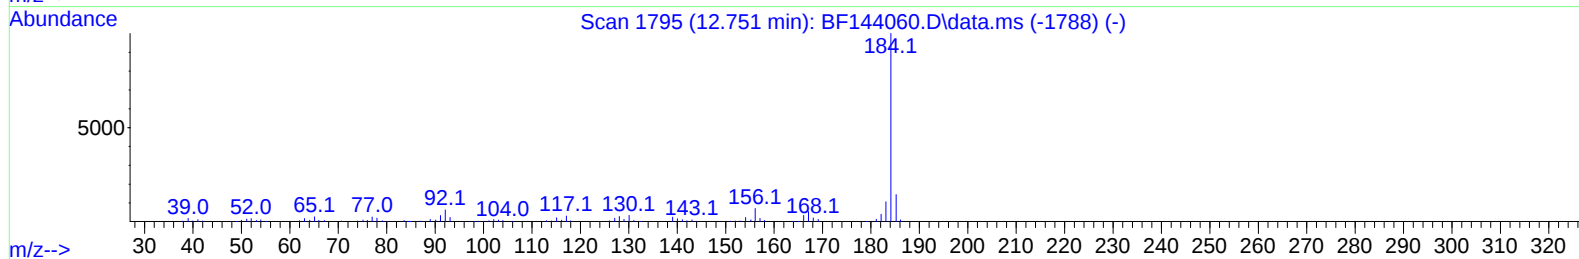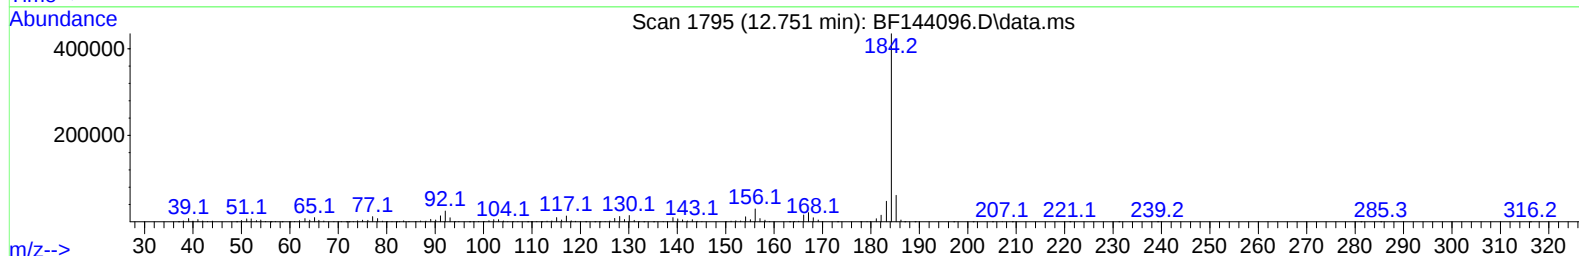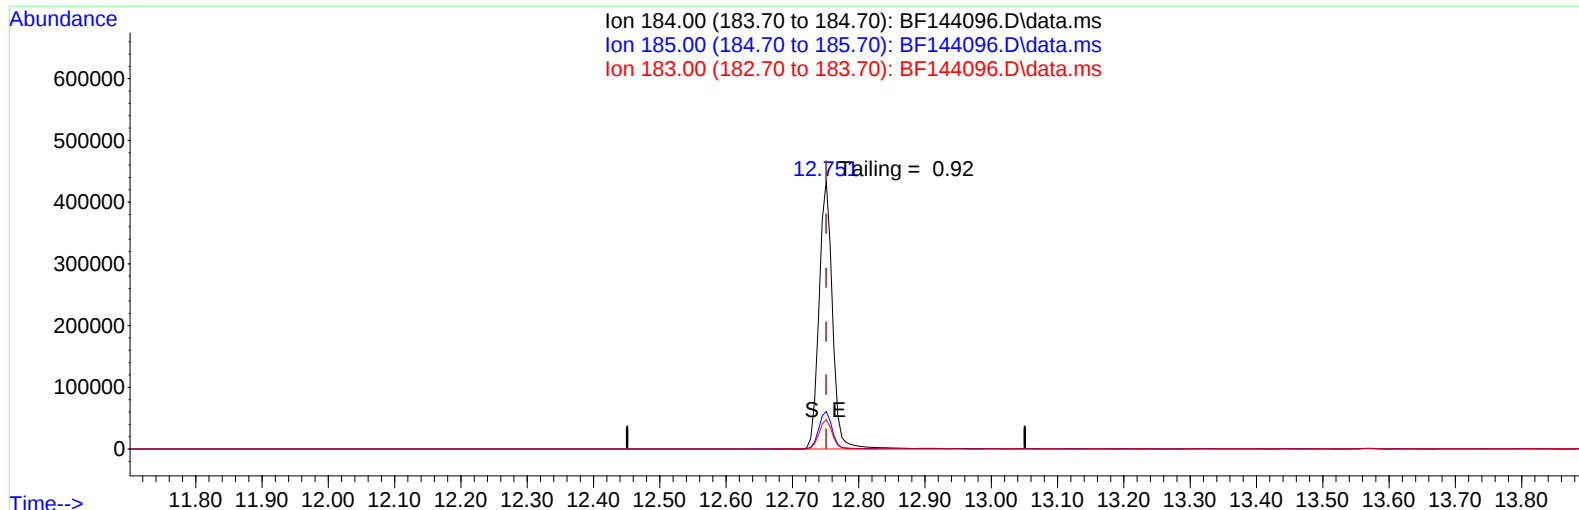

TIC: BF144096.D\data.ms

(77) Benzidine

12.751min (+ 0.000) 31665.53 ng

response 613959

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.04
183.00	10.60	10.96
0.00	0.00	0.00