

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102919\
 Data File : BF117608.D
 Acq On : 29 Oct 2019 23:53
 Operator : JU
 Sample : K5576-14 5X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Oct 30 04:22:59 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 18 18:53:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	32681	20.00	ng	0.00
21) Naphthalene-d8	8.01	136	120336	20.00	ng	0.00
39) Acenaphthene-d10	9.76	164	50315	20.00	ng	0.00
64) Phenanthrene-d10	11.25	188	81339	20.00	ng	0.00
76) Chrysene-d12	13.90	240	61507	20.00	ng	0.00
87) Perylene-d12	15.34	264	47121	20.00	ng	0.02

System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	42222	19.22	ng	0.02
7) Phenol-d6	6.40	99	54591	18.50	ng	0.02
23) Nitrobenzene-d5	7.30	82	29223	11.99	ng	0.00
42) 2,4,6-Tribromophenol	10.56	330	7787	17.89	ng	0.00
45) 2-Fluorobiphenyl	9.08	172	51491	14.42	ng	-0.01
79) Terphenyl-d14	12.83	244	53541	14.20	ng	0.00


Target Compounds				Qvalue		
9) Benzaldehyde	6.51	77	847	Below Cal	#	76
25) Isophorone	7.30	82	29223	6.930	ng	65
49) Acenaphthylene	9.62	152	125619	27.231	ng	99
51) 2,6-Dinitrotoluene	9.76	165	6972	9.315	ng	22
56) 4-Nitrophenol	9.97	139	2408	9.593	ng	6
58) Fluorene	10.32	166	12716	3.750	ng	98
71) Phenanthrene	11.27	178	161371	34.167	ng	97
72) Anthracene	11.33	178	152912	31.553	ng	100
73) Carbazole	11.49	167	36260	8.187	ng	98
75) Fluoranthene	12.47	202	716035	151.441	ng	98
77) Benzidine	12.66	184	108	Below Cal	#	67
78) Pylene	12.70	202	642552	121.624	ng	99
80) Butylbenzylphthalate	13.30	149	45728	17.394	ng	97
81) Benzo(a)anthracene	13.89	228	378615	91.257	ng	97
83) Chrysene	13.93	228	343829	84.558	ng	97
84) Bis(2-ethylhexyl)phthalate	13.86	149	12453	3.381	ng	98
86) Indeno(1,2,3-cd)pyrene	16.76	276	91001	29.976	ng	96
88) Benzo(b)fluoranthene	14.93	252	416212	149.579	ng	98
89) Benzo(k)fluoranthene	14.93	252	416212	145.940	ng	# 97
90) Benzo(a)pyrene	15.29	252	165039	65.235	ng	97
91) Dibenzo(a,h)anthracene	16.75	278	23744	10.854	ng	# 92
92) Benzo(g,h,i)perylene	17.19	276	82162	39.696	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102919\
Data File : BF117608.D
Acq On : 29 Oct 2019 23:53
Operator : JU
Sample : K5576-14 5X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Oct 30 04:22:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

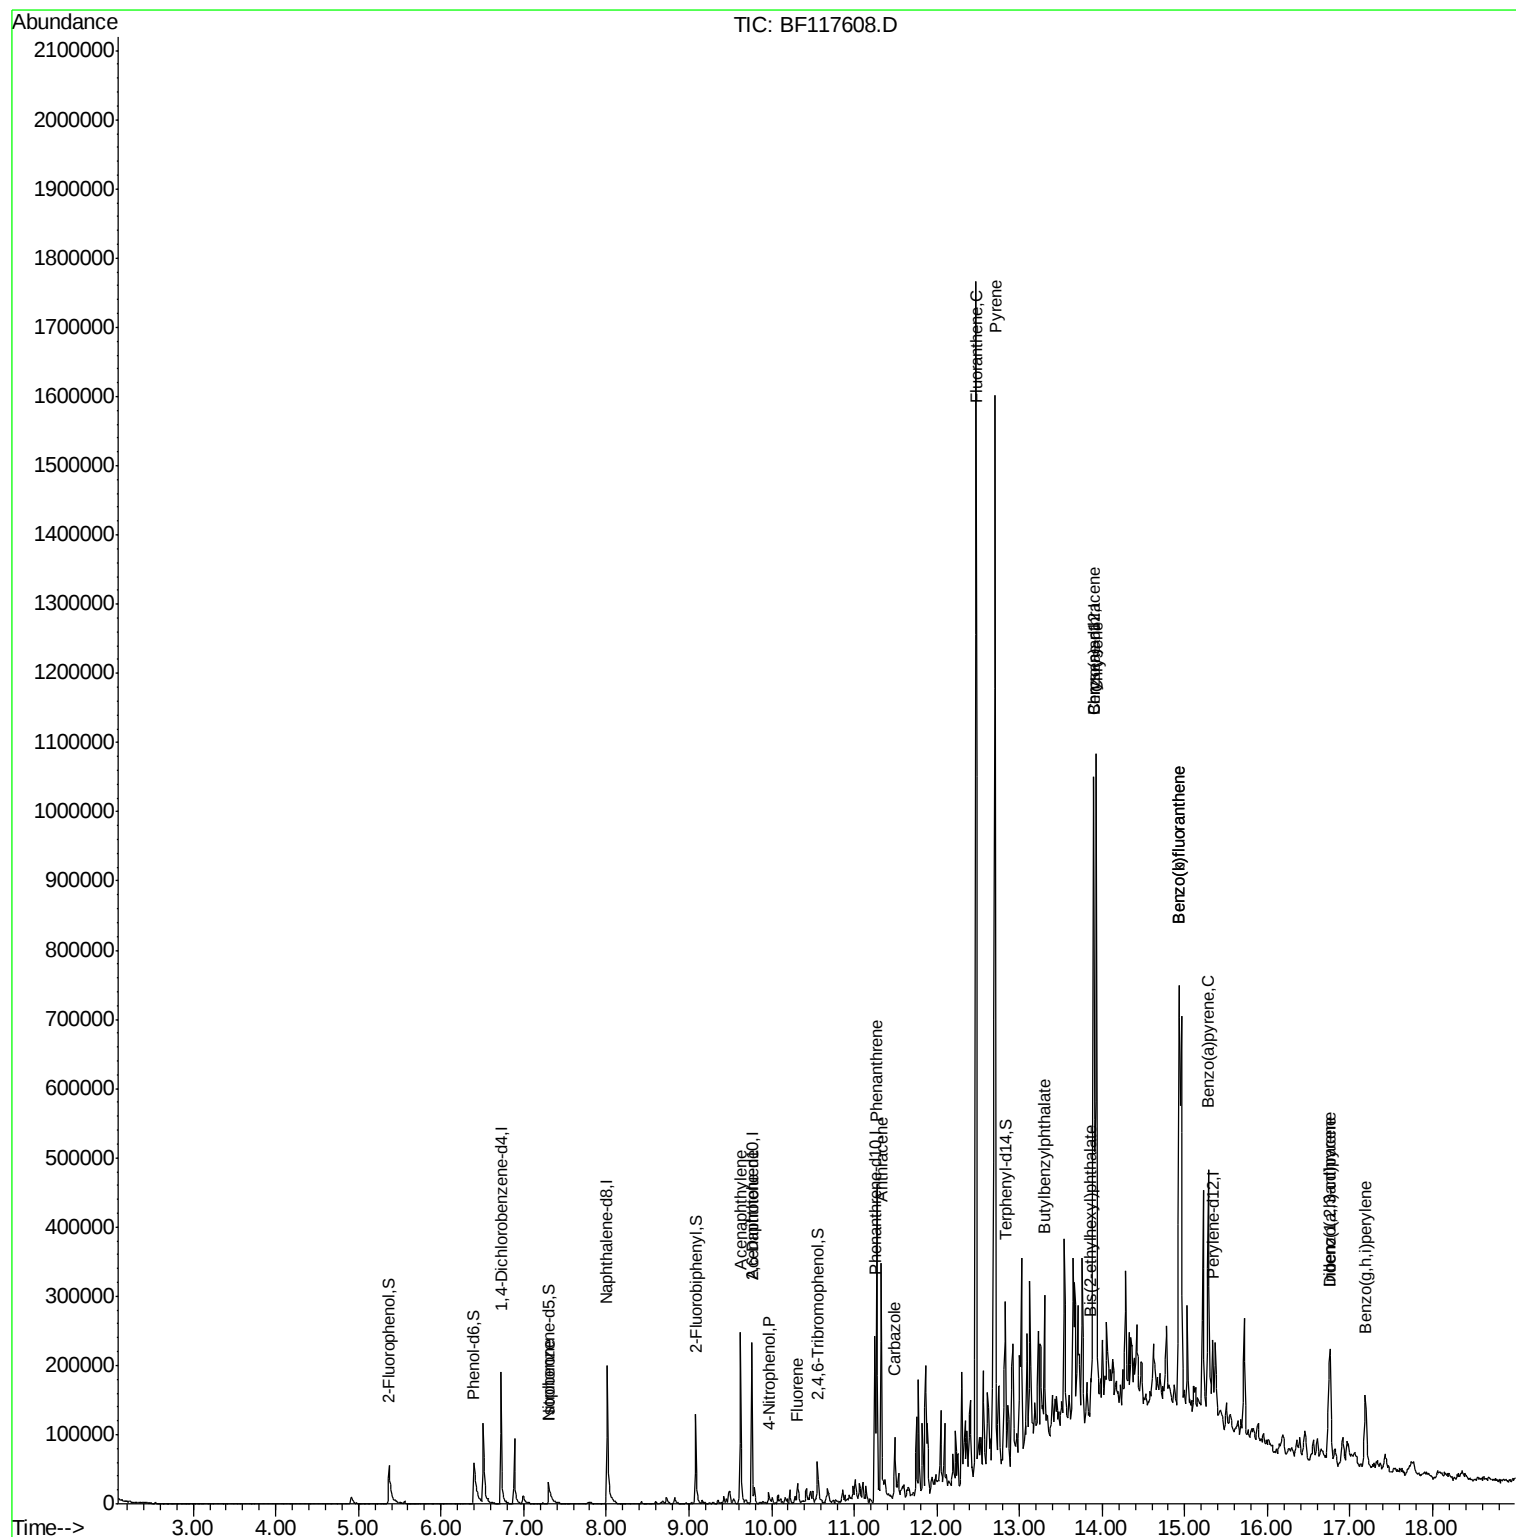




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.73 min Scan# 789
Delta R.T. -0.01 min
Lab File: BF117608.D
Acq: 29 Oct 2019 23:53

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 32681
Ion Ratio Lower Upper
152 100
150 158.2 126.8 190.2
115 66.5 51.6 77.4

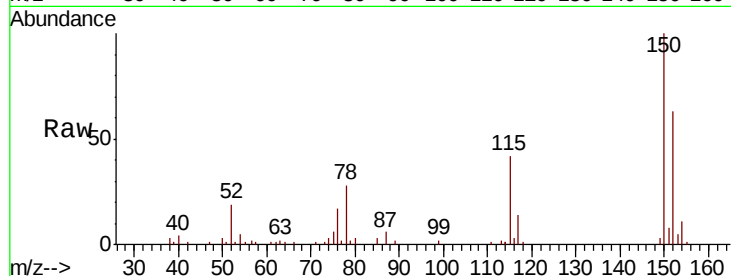


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

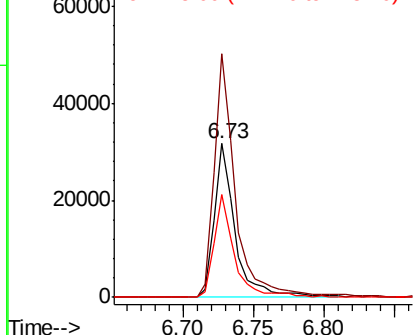



#5

2-Fluorophenol
Concen: 19.220 ng
RT: 5.37 min Scan# 558
Delta R.T. 0.02 min
Lab File: BF117608.D
Acq: 29 Oct 2019 23:53

Tgt Ion:112 Resp: 42222
Ion Ratio Lower Upper
112 100
64 53.6 44.1 66.1
63 30.3 23.4 35.2



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

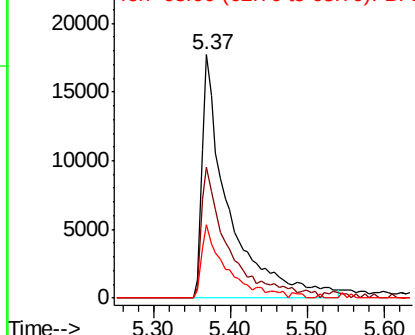



#7

Phenol-d6

Concen: 18.502 ng

RT: 6.40 min Scan# 733

Delta R.T. 0.02 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 54591

Ion Ratio Lower Upper




99 100

42 15.4 12.8 19.2

71 39.7 28.6 43.0

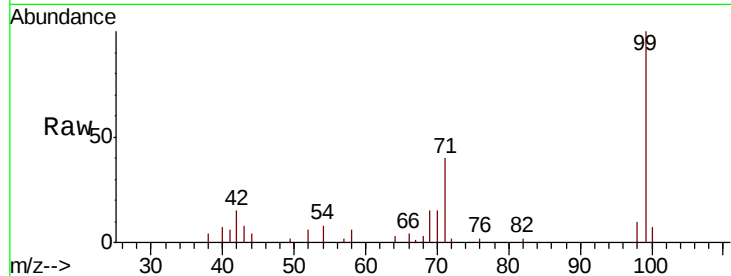

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

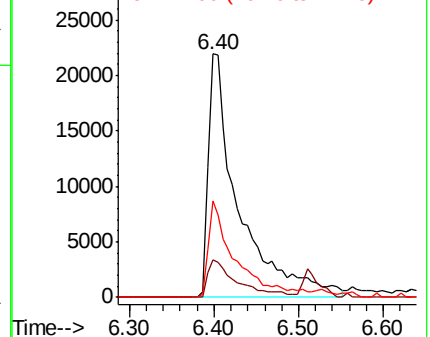

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.01 min Scan# 1007

Delta R.T. -0.01 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53

Tgt Ion: 136 Resp: 120336


Ion Ratio Lower Upper

136 100



137 10.3 8.2 12.4

54 6.2 4.5 6.7

68 5.3 4.3 6.5



Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1




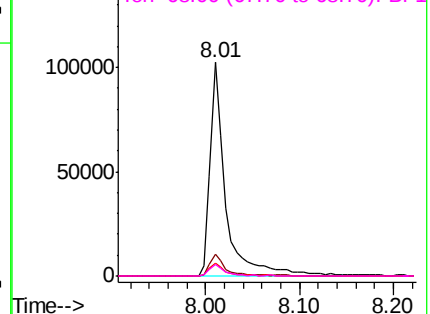




#23
Nitrobenzene-d5
Concen: 11.989 ng
RT: 7.30 min Scan# 887
Delta R.T. -0.00 min
Lab File: BF117608.D
Acq: 29 Oct 2019 23:53




Instrument :
BNA_F
ClientSampleId :


Tot Ion	82	Resp	29223
Ion Ratio	Lower	Upper	
82	100		
128	39.5	32.2	48.2
54	39.8	34.2	51.2

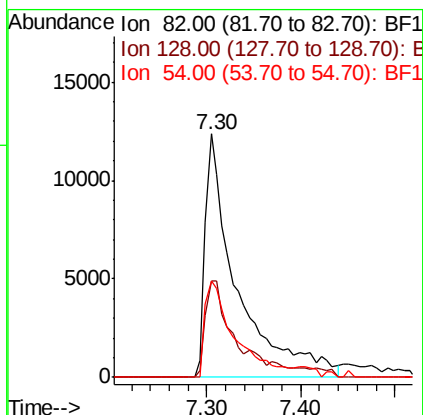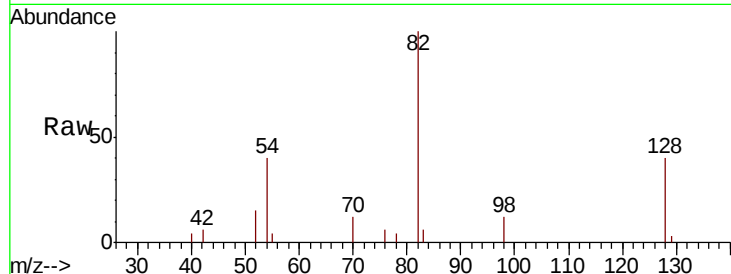

#25
Isophorone
Concen: 6.930 ng
RT: 7.30 min Scan# 887
Delta R.T. -0.26 min
Lab File: BF117608.D
Acq: 29 Oct 2019 23:53

Tgt Ion	82	Resp	29223
Ion Ratio	Lower	Upper	
82	100		
95	0.0	5.4	8.0#
138	0.0	14.2	21.2#

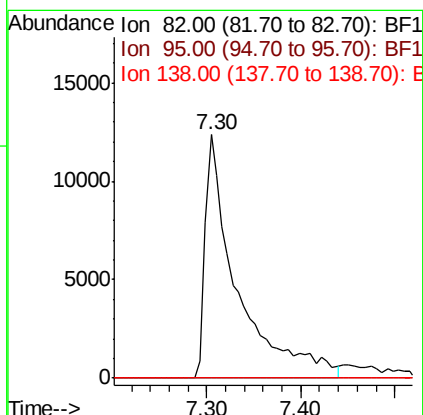







#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.76 min Scan# 1305
 Delta R.T. -0.01 min
 Lab File: BF117608.D
 Acq: 29 Oct 2019 23:53

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:164 Resp: 50315
 Ion Ratio Lower Upper
 164 100
 162 107.3 81.8 122.6
 160 44.0 34.4 51.6




Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

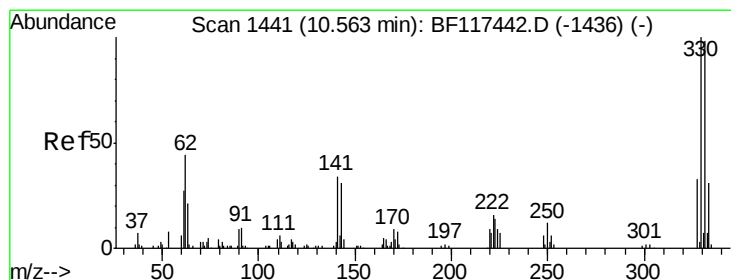
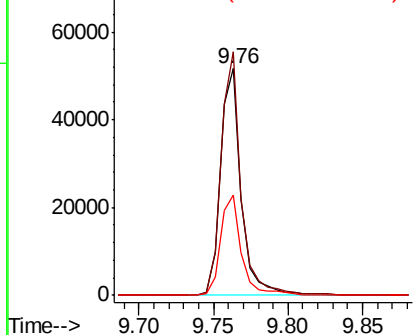



#42
 2,4,6-Tribromophenol
 Concen: 17.887 ng
 RT: 10.56 min Scan# 1441
 Delta R.T. 0.00 min
 Lab File: BF117608.D
 Acq: 29 Oct 2019 23:53

Tgt Ion:330 Resp: 7787
 Ion Ratio Lower Upper
 330 100
 332 98.2 78.5 117.7
 141 55.5 37.0 55.6

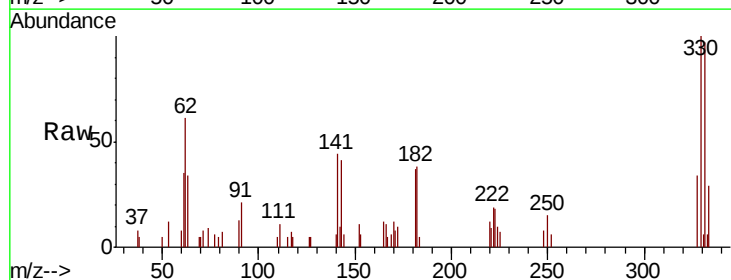

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

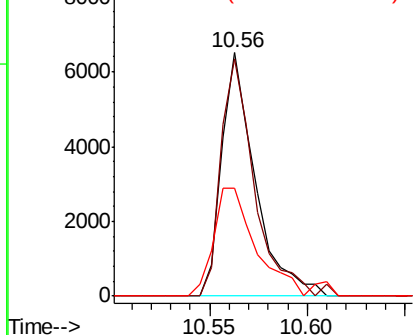


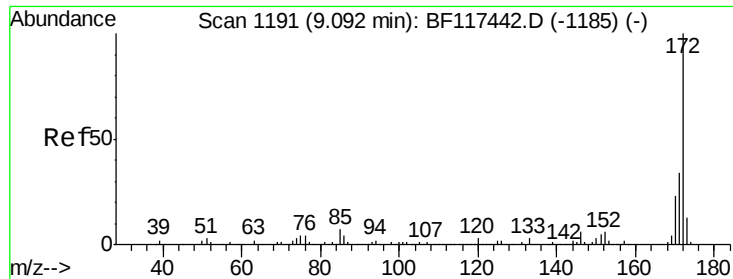




#45
2-Fluorobiphenyl
Concen: 14.419 ng
RT: 9.08 min Scan# 1189
Delta R.T. -0.01 min
Lab File: BF117608.D
Acq: 29 Oct 2019 23:53

Instrument :
BNA_F
ClientSampleId :

Tot Ion:172 Resp: 51491
Ion Ratio Lower Upper
172 100
171 33.3 27.5 41.3
170 22.5 18.6 27.8

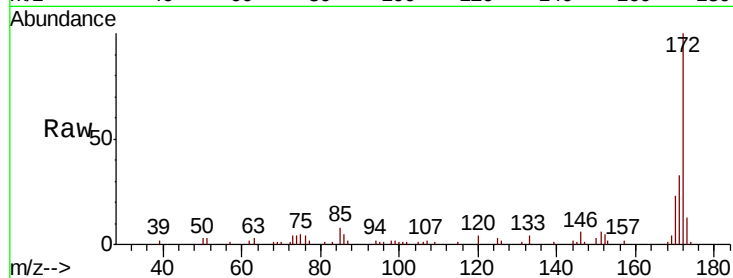


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

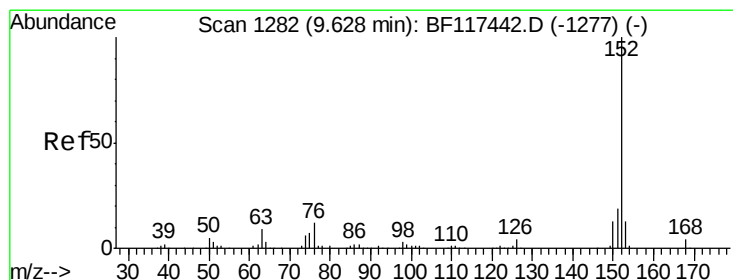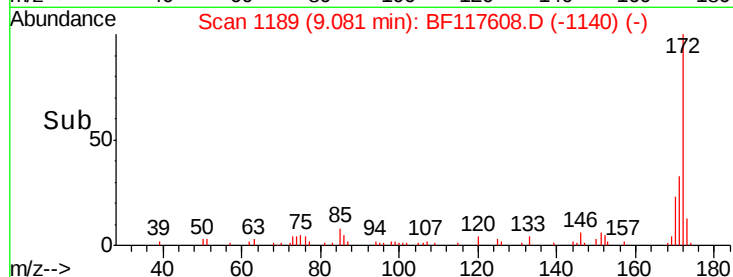
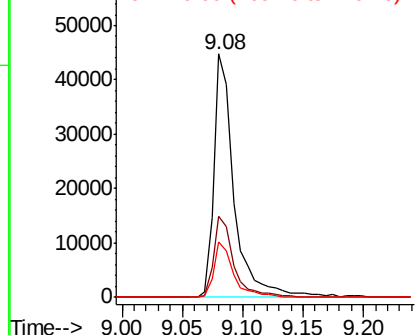



#49
Acenaphthylene
Concen: 27.231 ng
RT: 9.62 min Scan# 1281
Delta R.T. -0.01 min
Lab File: BF117608.D
Acq: 29 Oct 2019 23:53

Tgt Ion:152 Resp: 125619
Ion Ratio Lower Upper
152 100
151 19.2 15.4 23.0
153 14.1 10.3 15.5

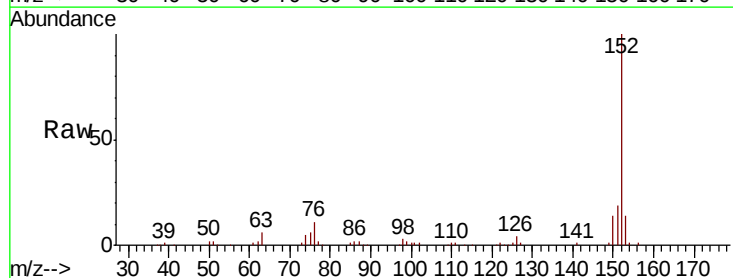

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E

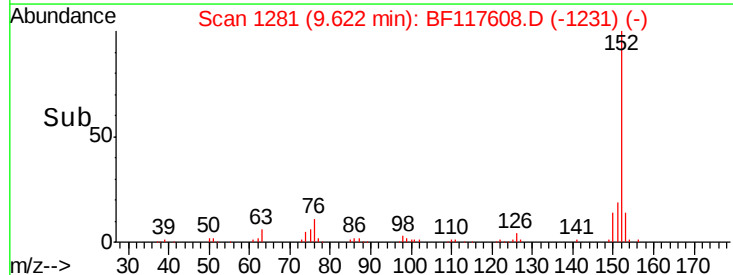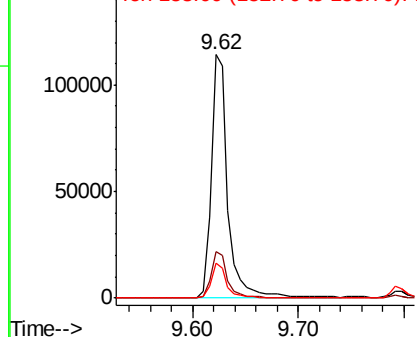

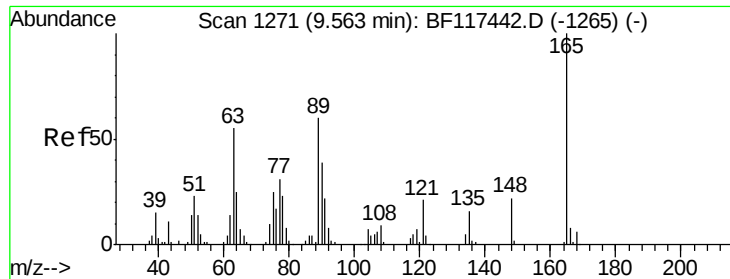

#51

2,6-Dinitrotoluene

Concen: 9.315 ng

RT: 9.76 min Scan# 1304

Delta R.T. 0.19 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53

Instrument :

BNA_F

ClientSampleId :


Tot Ion:165 Resp: 6972

Ion Ratio Lower Upper

165 100

63 0.0 43.8 65.8#




89 0.0 47.6 71.4#

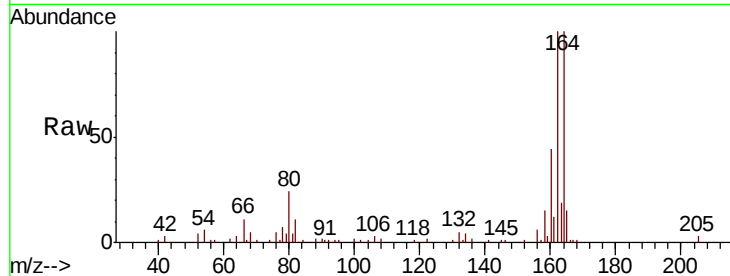

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

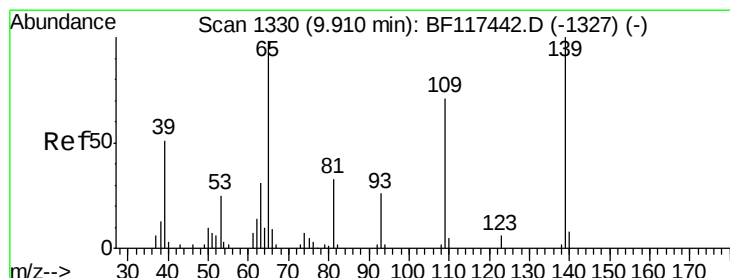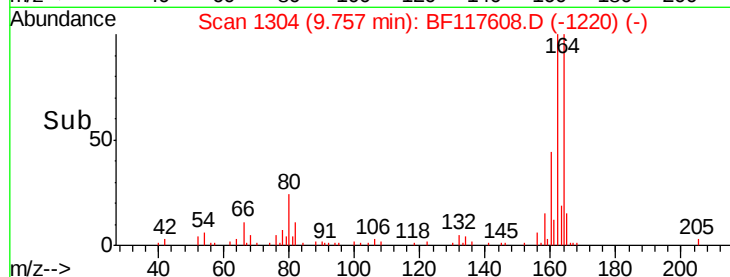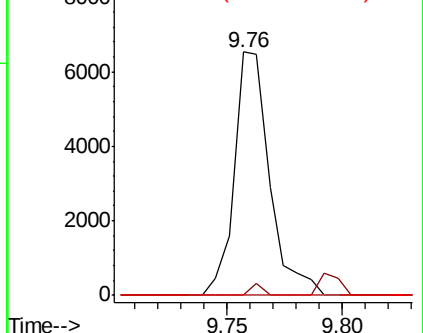

#56

4-Nitrophenol

Concen: 9.593 ng

RT: 9.97 min Scan# 1340

Delta R.T. 0.06 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53


Tgt Ion:139 Resp: 2408

Ion Ratio Lower Upper

139 100

109 0.0 51.4 91.4#



65 0.0 79.4 119.4#

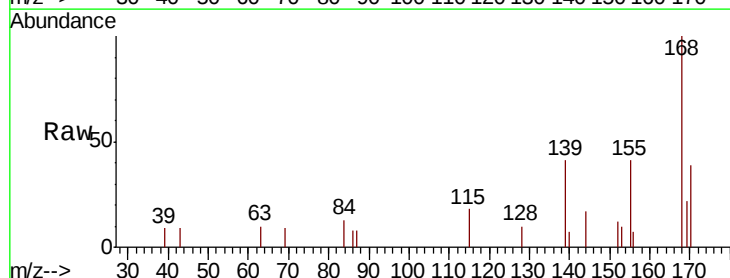


Abundance Ion 139.00 (138.70 to 139.70): E

Ion 109.00 (108.70 to 109.70): E

Ion 65.00 (64.70 to 65.70): BF1

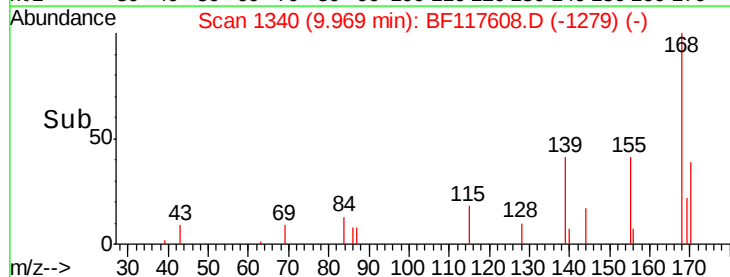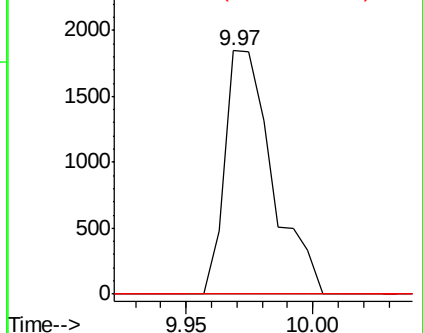



#58

Fluorene

Concen: 3.750 ng

RT: 10.32 min Scan# 1399

Delta R.T. 0.00 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53


Instrument :

BNA_F

ClientSampleId :

Tot Ion:166 Resp: 12716

Ion	Ratio	Lower	Upper
166	100		
165	98.5	77.6	116.4
167	14.9	11.0	16.4






Abundance

Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

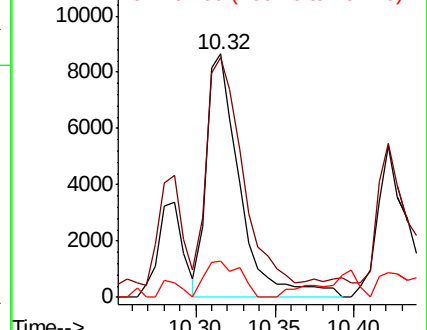

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.25 min Scan# 1558


Delta R.T. 0.00 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53

Tgt Ion:188 Resp: 81339

Ion	Ratio	Lower	Upper
188	100		
94	10.2	8.0	12.0
80	10.7	9.5	14.3






Abundance

Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

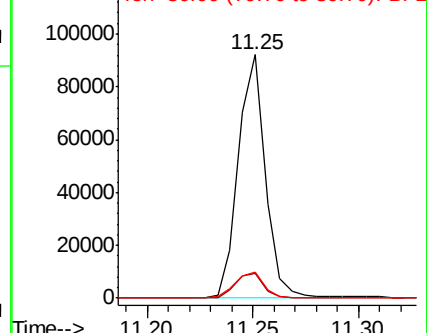



#71

Phenanthrene

Concen: 34.167 ng

RT: 11.27 min Scan# 1562

Delta R.T. -0.00 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53

Instrument :

BNA_F

ClientSampled :


Tot Ion:178 Resp: 161371

Ion Ratio Lower Upper

178 100

176 18.5 14.6 22.0




179 13.6 12.6 19.0

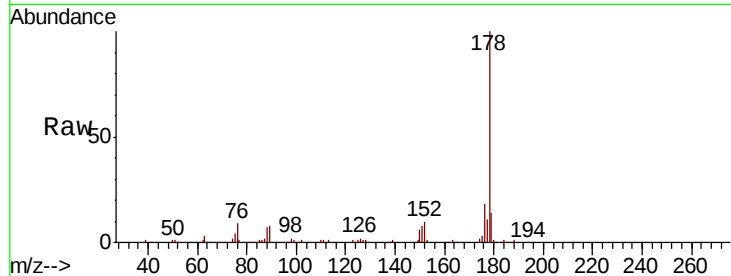

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

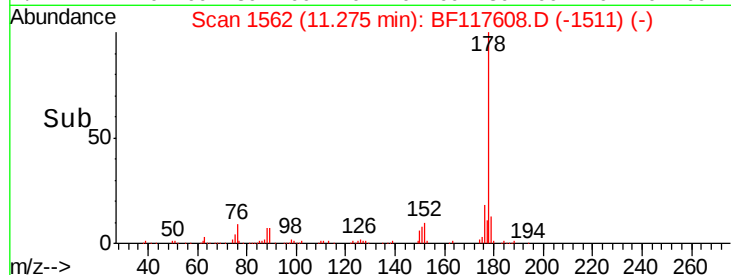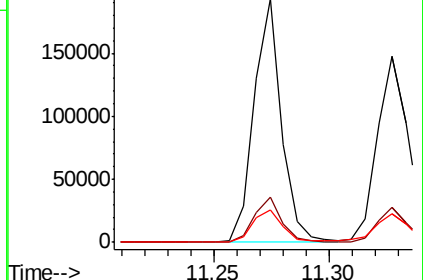

#72

Anthracene

Concen: 31.553 ng

RT: 11.33 min Scan# 1571

Delta R.T. 0.00 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53


Tgt Ion:178 Resp: 152912

Ion Ratio Lower Upper

178 100

176 18.5 14.7 22.1



179 15.4 12.2 18.2




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E




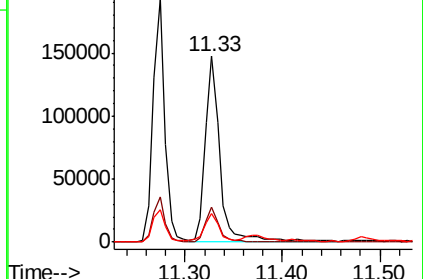




#73
 Carbazole
 Concen: 8.187 ng
 RT: 11.49 min Scan# 1599
 Delta R.T. 0.01 min
 Lab File: BF117608.D
 Acq: 29 Oct 2019 23:53




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:167 Resp: 36260
 Ion Ratio Lower Upper
 167 100
 166 22.5 17.0 25.6
 139 13.0 10.6 16.0

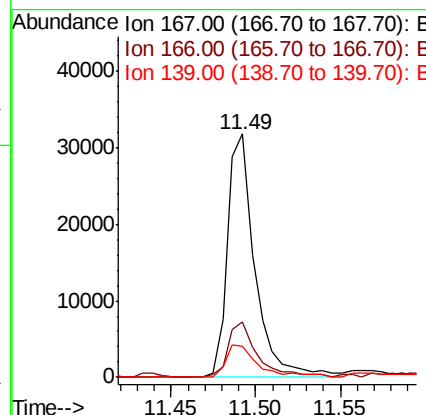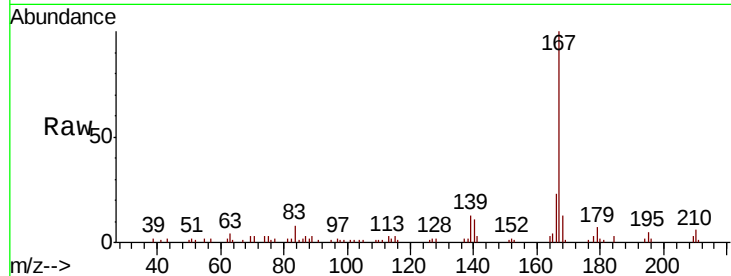

#75
 Fluoranthene
 Concen: 151.441 ng
 RT: 12.47 min Scan# 1766
 Delta R.T. 0.01 min
 Lab File: BF117608.D
 Acq: 29 Oct 2019 23:53

Tgt Ion:202 Resp: 716035
 Ion Ratio Lower Upper
 202 100
 101 14.0 0.0 32.7
 203 17.2 0.0 37.6



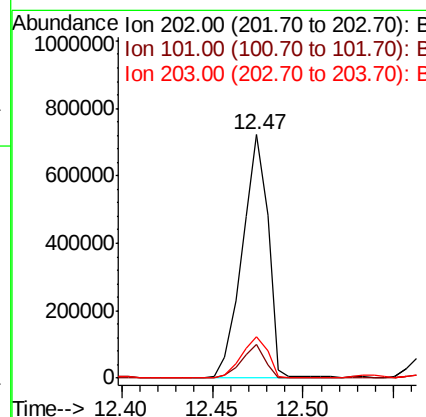
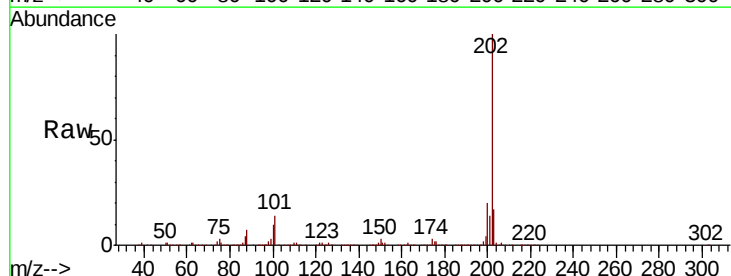




#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 13.90 min Scan# 2009
 Delta R.T. 0.01 min
 Lab File: BF117608.D
 Acq: 29 Oct 2019 23:53




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
240	100		
120	12.7	8.4	12.6#
236	25.2	20.0	30.0

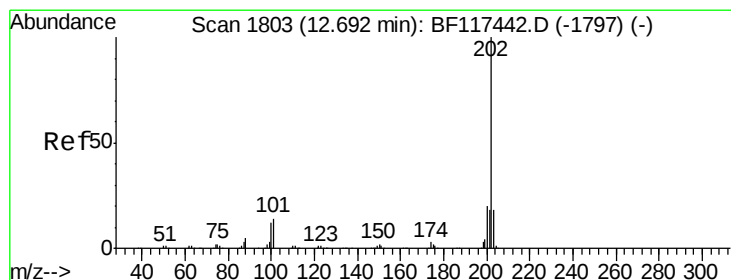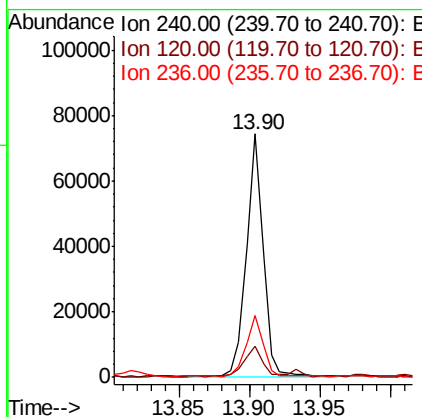

#78
 Pyrene
 Concen: 121.624 ng
 RT: 12.70 min Scan# 1805
 Delta R.T. 0.01 min
 Lab File: BF117608.D
 Acq: 29 Oct 2019 23:53

Tgt Ion	Ratio	Lower	Upper
202	100		
200	20.7	16.2	24.2
203	18.1	14.0	21.0

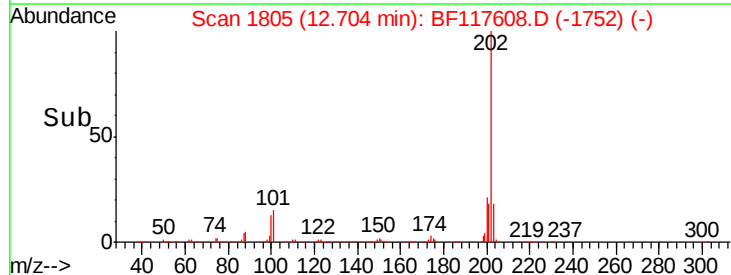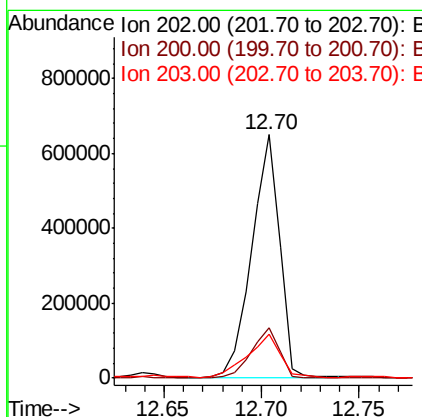



#79

Terphenyl-d14

Concen: 14.199 ng

RT: 12.83 min Scan# 1826

Delta R.T. -0.01 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 53541

Ion Ratio Lower Upper

244 100

212 7.5 5.8 8.6




122 13.6 11.8 17.8

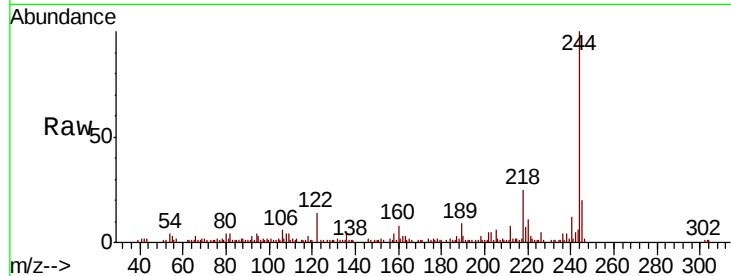

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

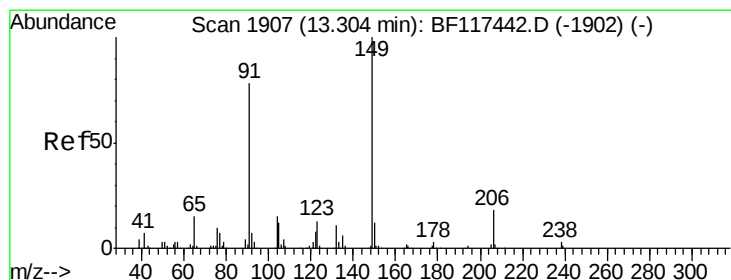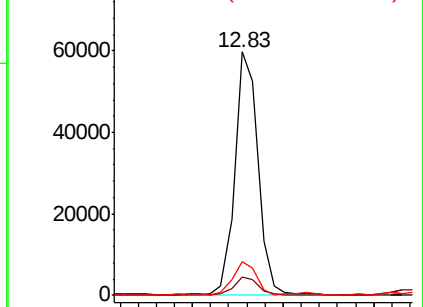

#80

Butylbenzylphthalate

Concen: 17.394 ng

RT: 13.30 min Scan# 1907

Delta R.T. 0.00 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53


Tgt Ion:149 Resp: 45728

Ion Ratio Lower Upper

149 100

91 74.4 62.1 93.1



206 19.1 14.3 21.5




Abundance Ion 149.00 (148.70 to 149.70): E

Ion 91.00 (90.70 to 91.70): BF1

Ion 206.00 (205.70 to 206.70): E

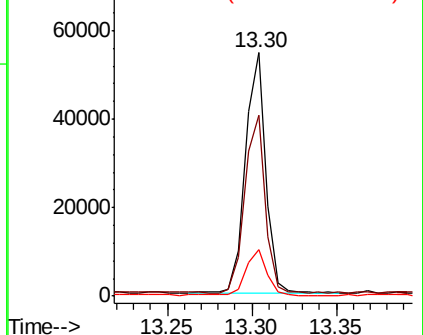



#81

Benzo(a)anthracene

Concen: 91.257 ng

RT: 13.89 min Scan# 2007

Delta R.T. 0.01 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53

Instrument :

BNA_F

ClientSampleId :


Tot Ion:228 Resp: 378615

Ion Ratio Lower Upper




228 100

226 28.9 21.0 31.4

229 20.7 16.4 24.6



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

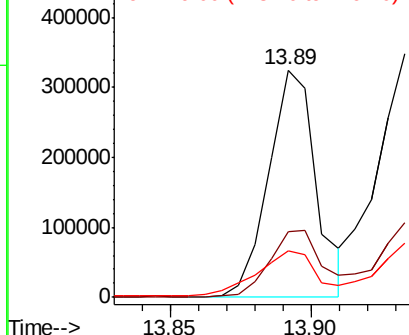

#83

Chrysene

Concen: 84.558 ng

RT: 13.93 min Scan# 2014

Delta R.T. 0.01 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53


Tgt Ion:228 Resp: 343829

Ion Ratio Lower Upper



228 100


226 30.5 23.9 35.9

229 22.3 15.8 23.6



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

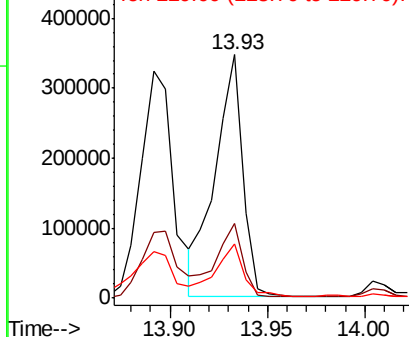



#84

Bis(2-ethylhexyl)phthalate

Concen: 3.381 ng

RT: 13.86 min Scan# 2002

Delta R.T. -0.01 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53

Instrument :

BNA_F

ClientSampleId :


Tot Ion:149 Resp: 12453

Ion Ratio Lower Upper




149 100

167 28.2 23.3 34.9

279 3.6 3.2 4.8

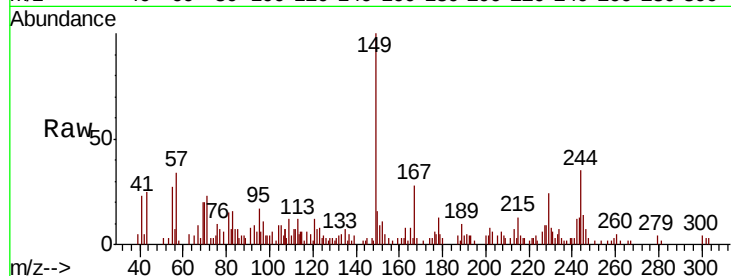

Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

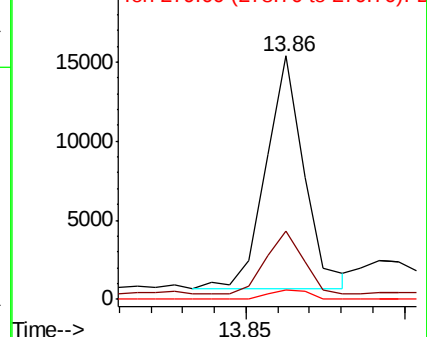

#86

Indeno(1,2,3-cd)pyrene

Concen: 29.976 ng

RT: 16.76 min Scan# 2495

Delta R.T. 0.03 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53


Tgt Ion:276 Resp: 91001

Ion Ratio Lower Upper



276 100


138 24.6 21.8 32.8

277 24.1 20.0 30.0



Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

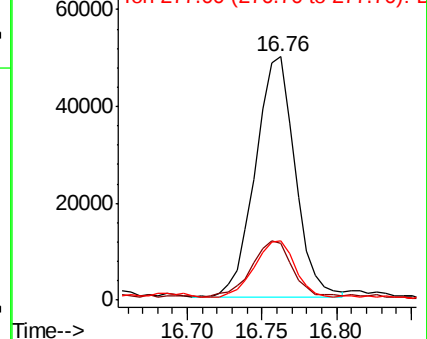

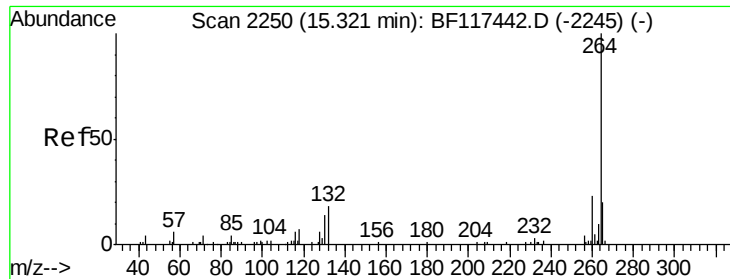

#87

Pervlene-d12

Concen: 20.000 ng

RT: 15.34 min Scan# 2253

Delta R.T. 0.02 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53

Instrument :

BNA_F

ClientSampled :


Tot Ion:264 Resp: 47121

Ion Ratio Lower Upper

264 100

260 24.8 18.4 27.6




265 26.1 16.1 24.1#

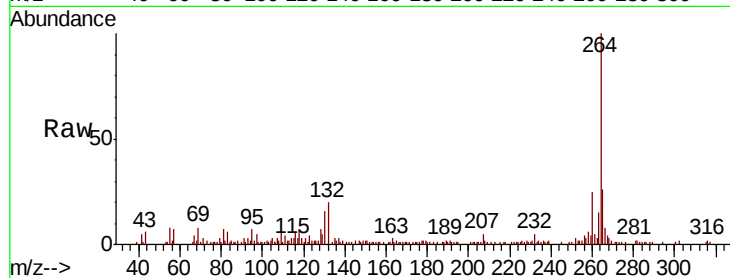

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

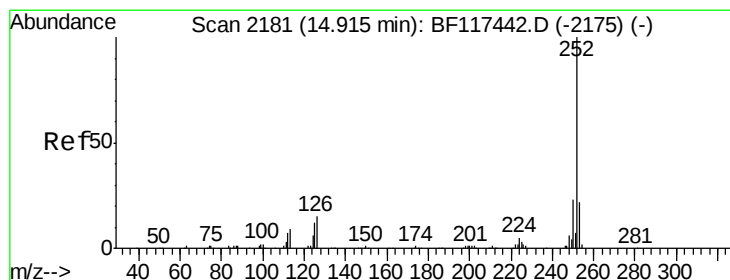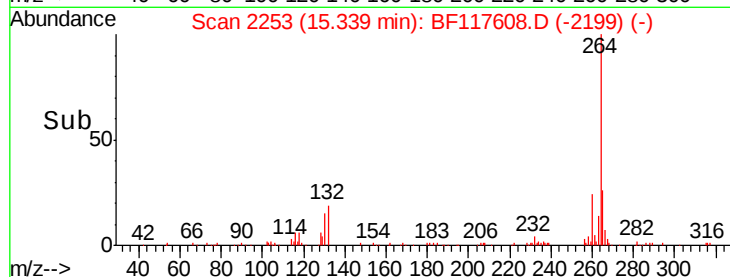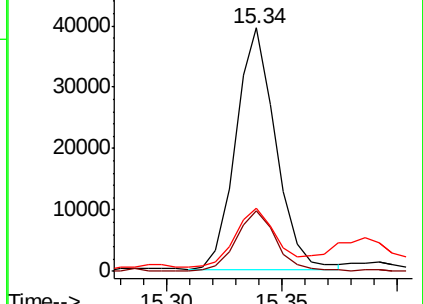

#88

Benzo(b)fluoranthene

Concen: 149.579 ng

RT: 14.93 min Scan# 2184

Delta R.T. 0.02 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53


Tgt Ion:252 Resp: 416212

Ion Ratio Lower Upper

252 100

253 22.4 17.8 26.6



125 14.3 9.9 14.9

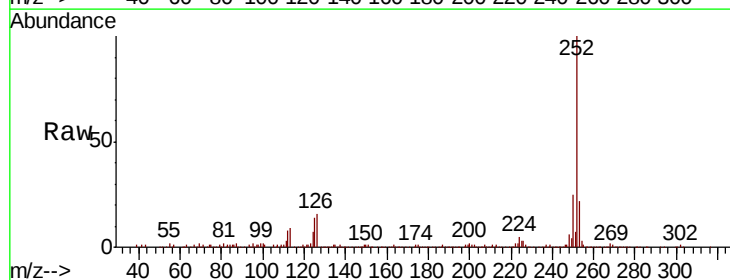


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



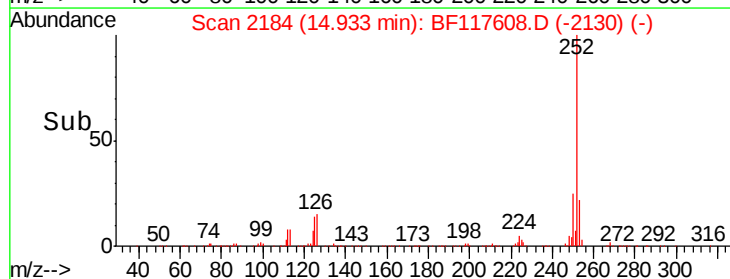
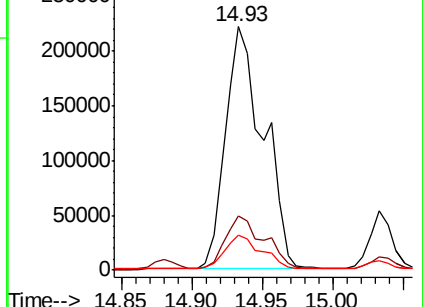




#89
Benzo(k)fluoranthene
Concen: 145.940 ng
RT: 14.93 min Scan# 2184
Delta R.T. -0.01 min
Lab File: BF117608.D
Acq: 29 Oct 2019 23:53




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
252	100		
253	22.4	18.0	27.0
125	14.3	8.9	13.3

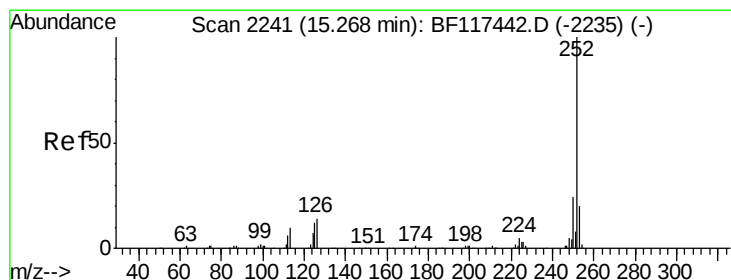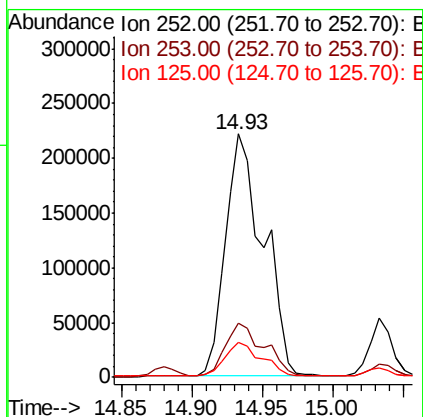

#90
Benzo(a)pyrene
Concen: 65.235 ng
RT: 15.29 min Scan# 2244
Delta R.T. 0.02 min
Lab File: BF117608.D
Acq: 29 Oct 2019 23:53

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.4	16.3	24.5
125	11.7	9.2	13.8

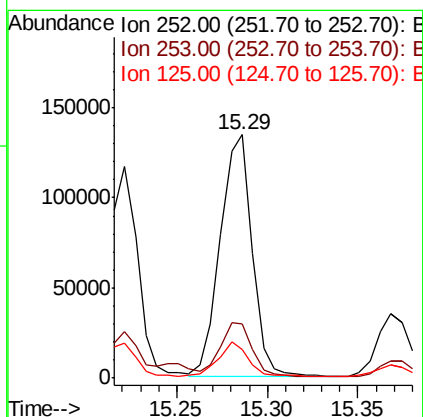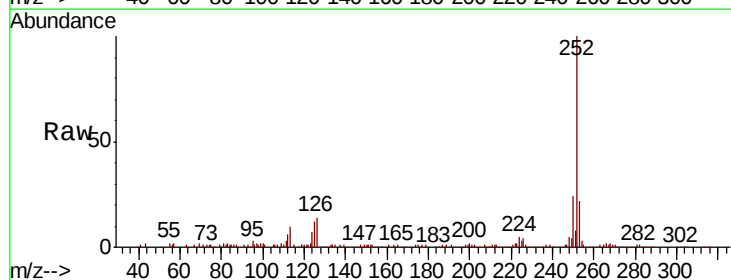



#91

Dibenzo(a,h)anthracene

Concen: 10.854 ng

RT: 16.75 min Scan# 2493

Delta R.T. 0.02 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53

Instrument :

BNA_F

ClientSampleId :


Tot Ion:278 Resp: 23744

Ion Ratio Lower Upper

278 100

139 19.2 13.4 20.0




279 27.1 17.8 26.6#

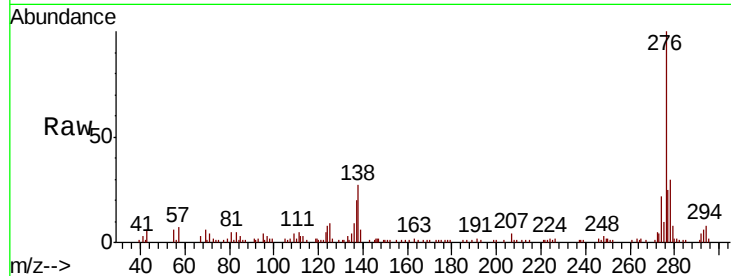

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

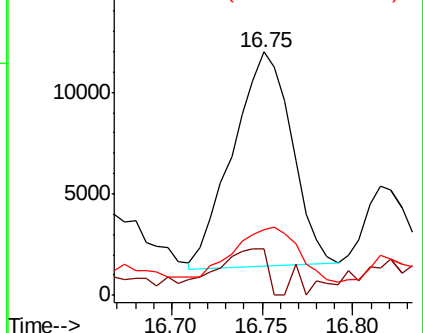

#92

Benzo(g,h,i)perylene

Concen: 39.696 ng

RT: 17.19 min Scan# 2567

Delta R.T. 0.04 min

Lab File: BF117608.D

Acq: 29 Oct 2019 23:53


Tgt Ion:276 Resp: 82162

Ion Ratio Lower Upper

276 100

277 22.9 18.4 27.6

138 23.3 17.8 26.6



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

