
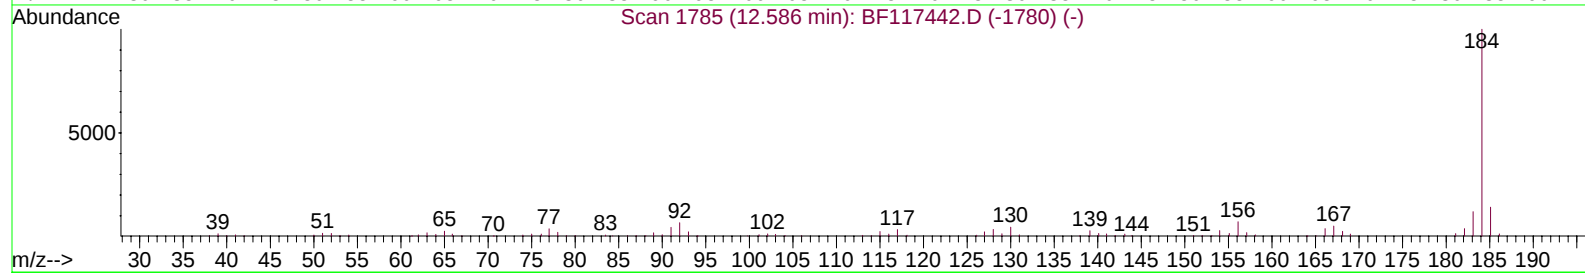
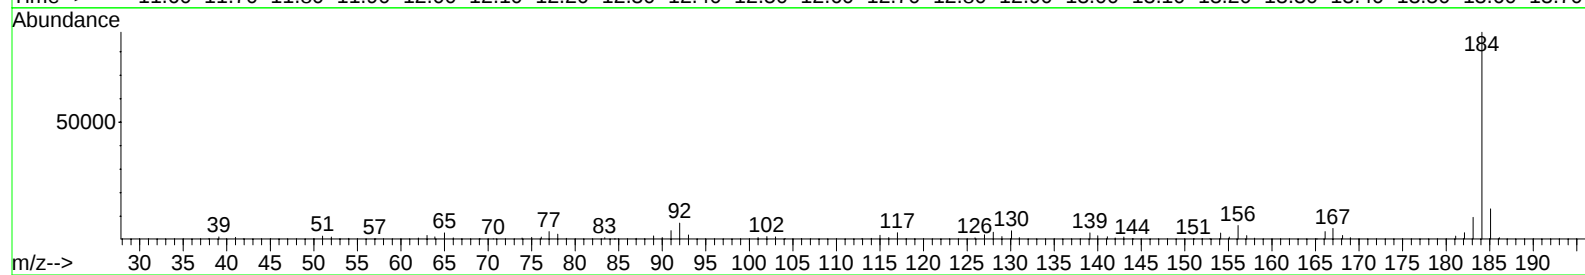


```

Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF102919\
Data File   : BF117603.D
Acq On      : 29 Oct 2019   21:39
Operator    : JU
Sample      : DFTPP
Misc        :
ALS Vial    : 1      Sample Multiplier: 1

```

Quant Time: Oct 30 18:28:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

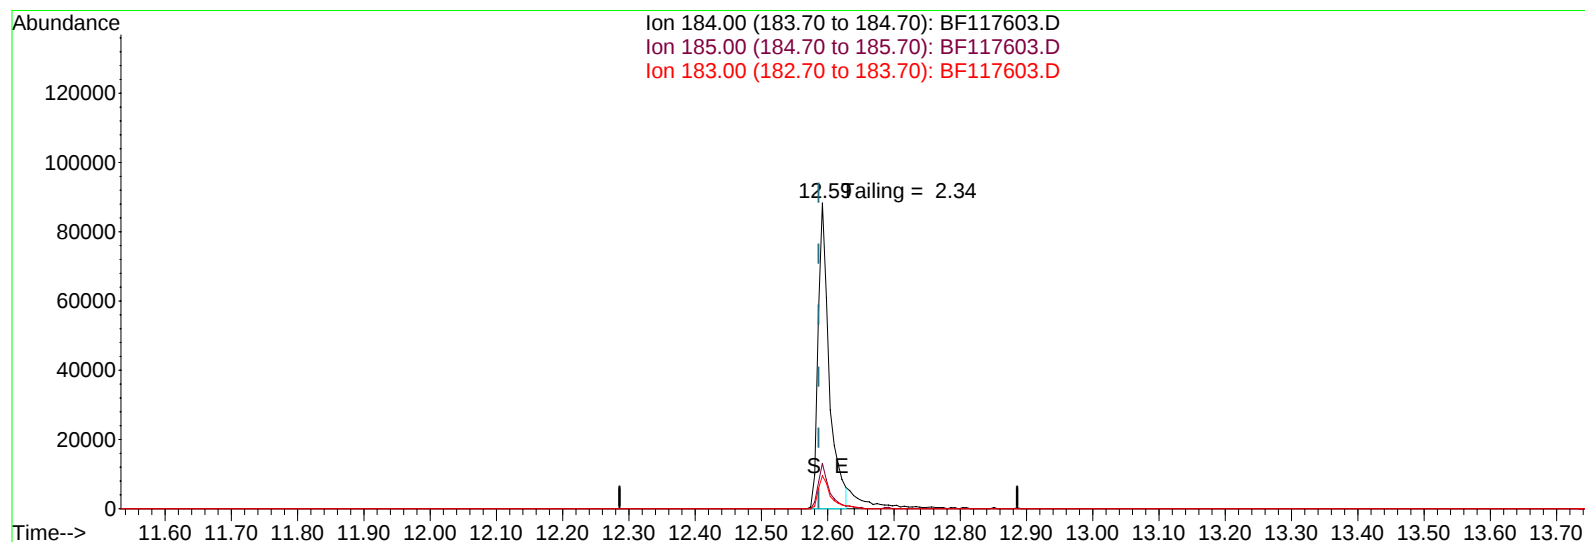

TIC: BF117603.D

(77) Benzidine




12.592min (+0.006) 0.00ng

```
response 113413
```

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.87
183.00	12.00	10.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF102919\
Data File : BF117603.D
Acq On : 29 Oct 2019 21:39
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 18:28:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

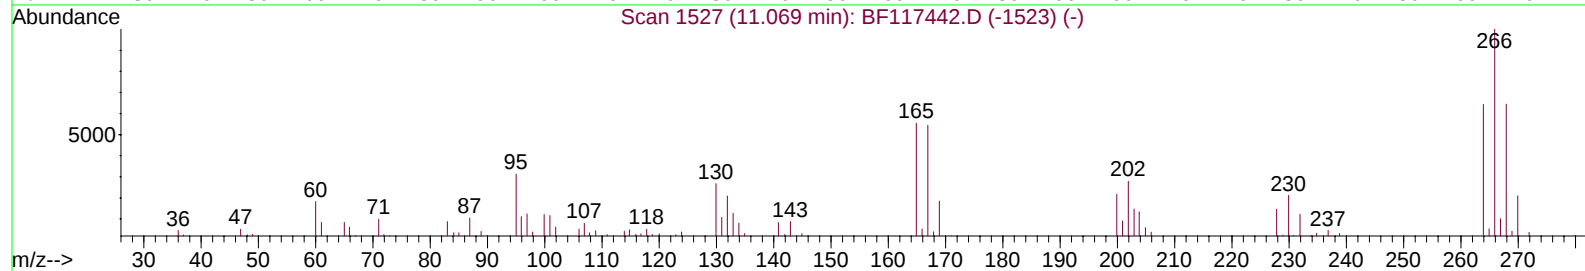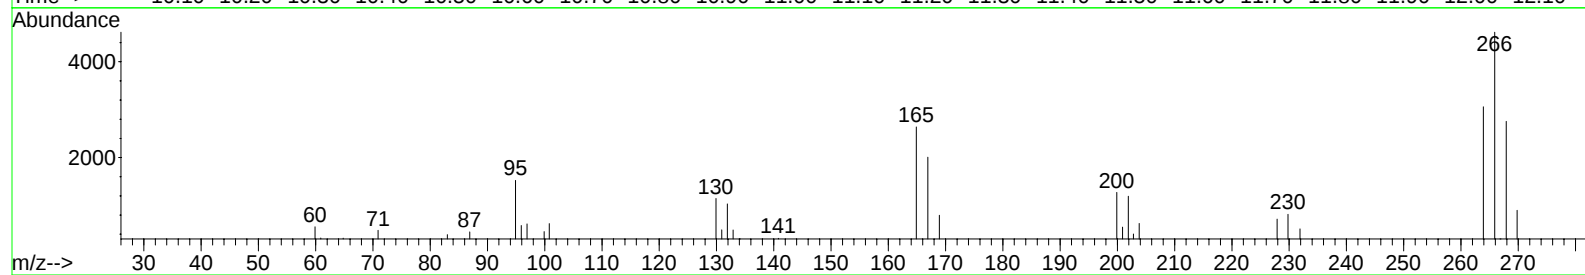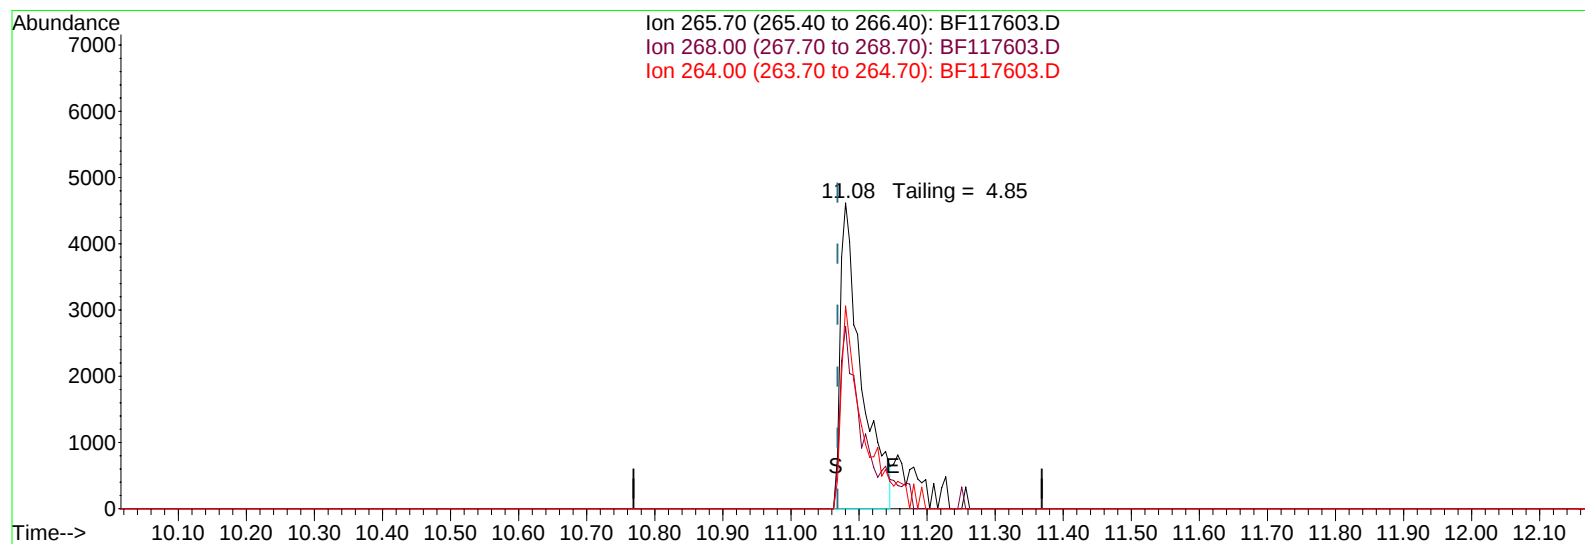

TIC: BF117603.D

(70) Pentachlorophenol (C)

11.080min (+0.012) 0.00ng

response 10667

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	59.68
264.00	64.30	66.29
0.00	0.00	0.00