

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102919\
 Data File : BF117600.D
 Acq On : 29 Oct 2019 19:25
 Operator : JU
 Sample : K5498-01 2X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 189-62-(0-1)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.387	558	561	576	rBV2	12838	35081	12.99%	1.959%
2	6.416	733	736	745	rBV	16574	38463	14.24%	2.148%
3	6.522	751	754	763	rBV	34268	54210	20.07%	3.027%
4	6.728	786	789	801	rBV	208816	211792	78.39%	11.825%
5	6.804	801	802	809	rVB2	2088	2851	1.06%	0.159%
6	6.887	812	816	826	rBV	41573	47955	17.75%	2.677%
7	7.316	886	889	902	rBV3	9146	23799	8.81%	1.329%
8	8.010	1004	1007	1024	rBV	227407	269279	99.67%	15.035%
9	9.086	1187	1190	1200	rBV	40430	50591	18.73%	2.825%
10	9.763	1301	1305	1322	rBB	259854	270163	100.00%	15.084%
11	10.569	1439	1442	1450	rBB	11870	15564	5.76%	0.869%
12	11.251	1554	1558	1568	rBV	228247	240010	88.84%	13.401%
13	11.786	1646	1649	1654	rVB3	2875	3813	1.41%	0.213%
14	12.327	1736	1741	1743	rBV2	2196	3886	1.44%	0.217%
15	12.451	1755	1762	1763	rBV6	2752	5532	2.05%	0.309%
16	12.592	1782	1786	1787	rBV3	2577	3227	1.19%	0.180%
17	12.604	1787	1788	1795	rVV8	3521	6119	2.26%	0.342%
18	12.704	1802	1805	1808	rVB4	2253	2731	1.01%	0.152%
19	12.827	1823	1826	1832	rBV	59411	53274	19.72%	2.974%
20	12.939	1844	1845	1851	rBV6	2427	3974	1.47%	0.222%
21	13.157	1878	1882	1883	rBV4	6130	7456	2.76%	0.416%
22	13.263	1898	1900	1904	rVB5	5498	7135	2.64%	0.398%
23	13.392	1920	1922	1923	rBV2	3927	2736	1.01%	0.153%
24	13.433	1927	1929	1934	rVB6	4656	5834	2.16%	0.326%
25	13.745	1980	1982	1988	rVB6	6600	9411	3.48%	0.525%
26	13.821	1993	1995	1997	rBV3	5187	3654	1.35%	0.204%
27	13.892	2004	2007	2014	rBV	208103	229098	84.80%	12.791%
28	15.327	2248	2251	2260	rVB	126651	173036	64.05%	9.661%
29	17.362	2595	2597	2599	rBV2	9672	10375	3.84%	0.579%


Sum of corrected areas: 1791049

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102919\
Data File : BF117600.D
Acq On : 29 Oct 2019 19:25
Operator : JU
Sample : K5498-01 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
189-62-(0-1)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

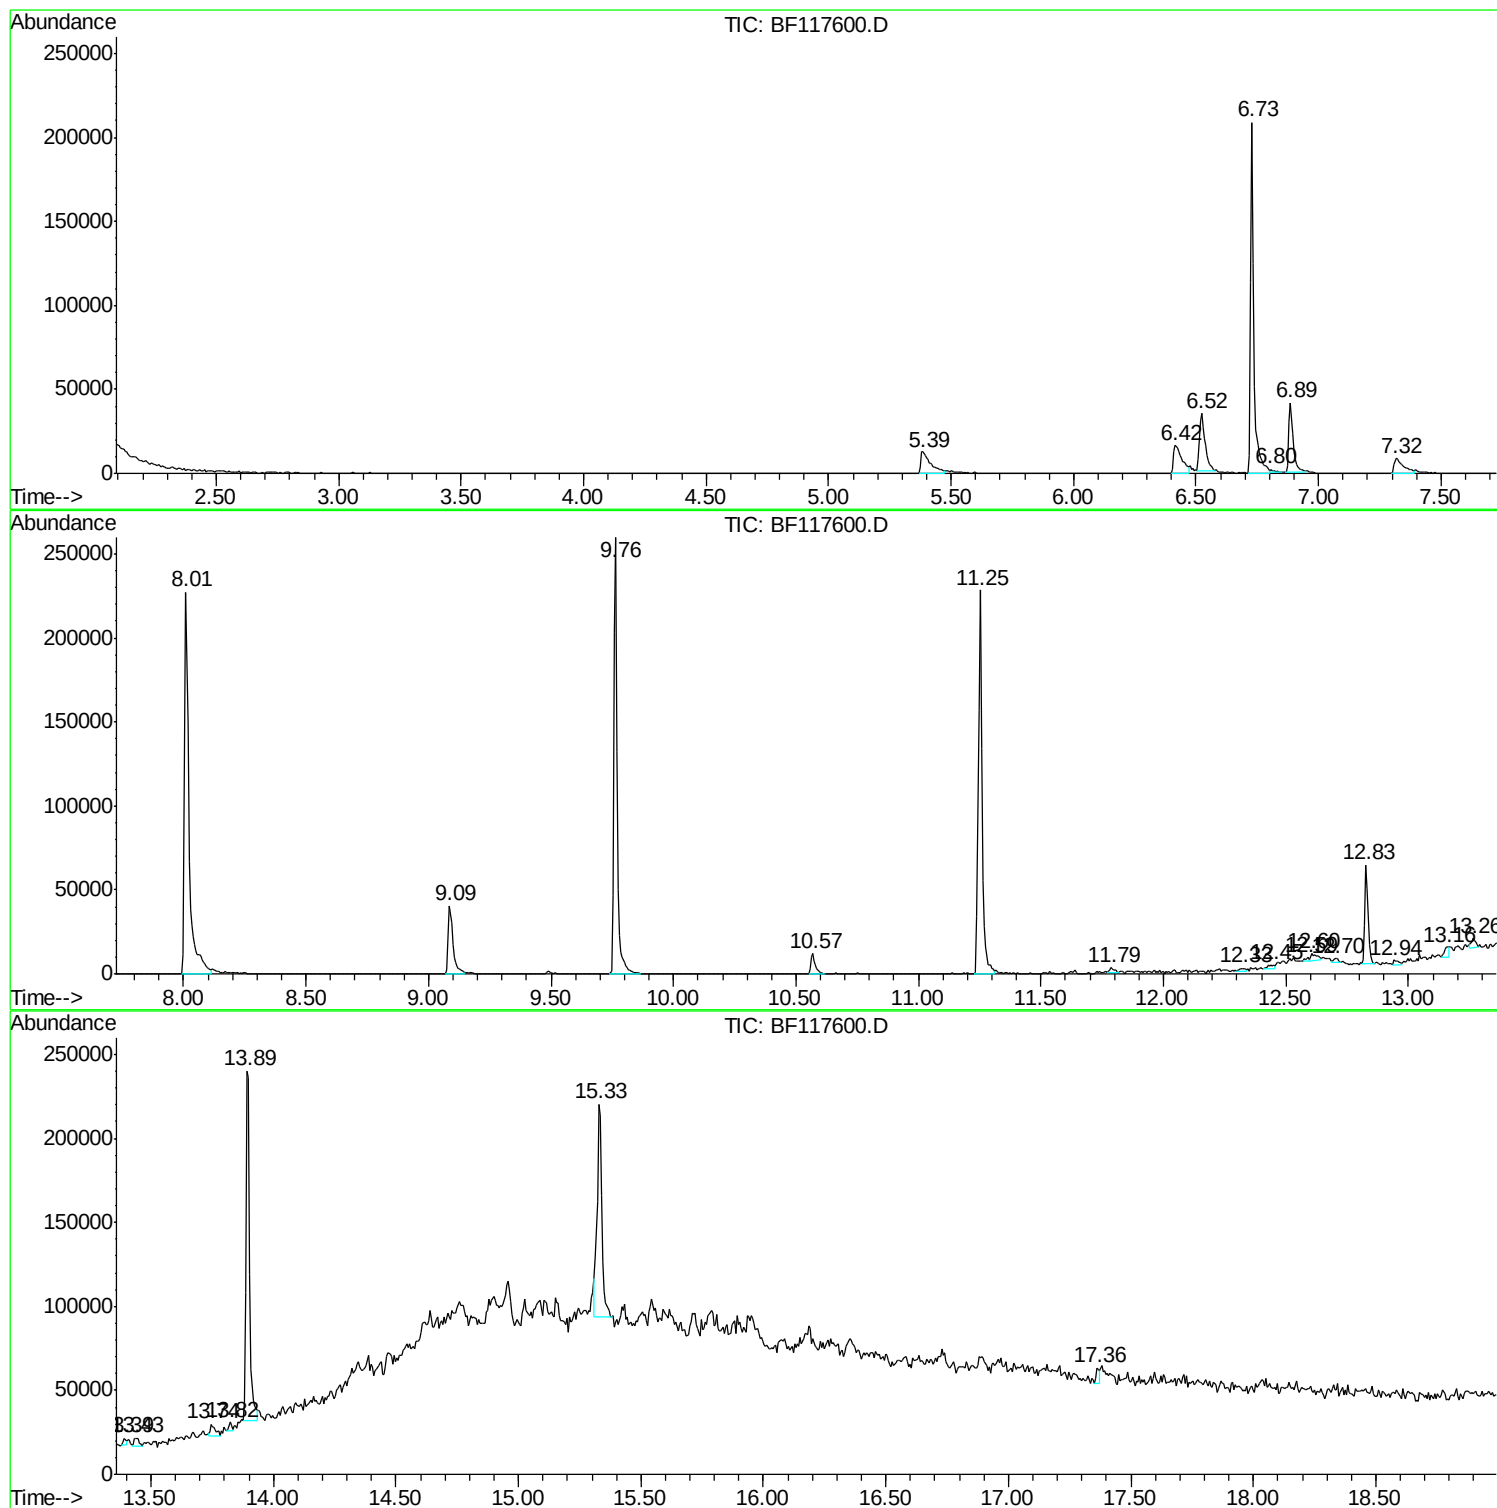

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102919\
Data File : BF117600.D
Acq On : 29 Oct 2019 19:25
Operator : JU
Sample : K5498-01 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
189-62-(0-1)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.52 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.52	5.12 ng	54210	1,4-Dichlorobenzene-d4	6.73

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	43
2			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
4			4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5			2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

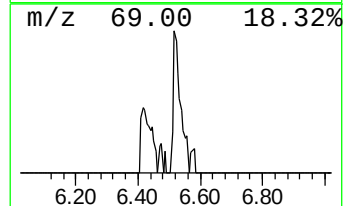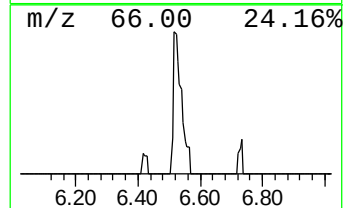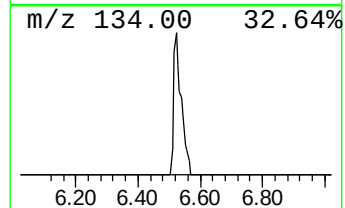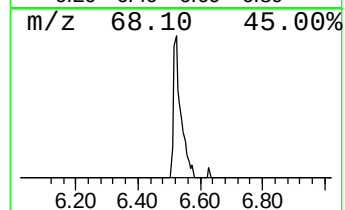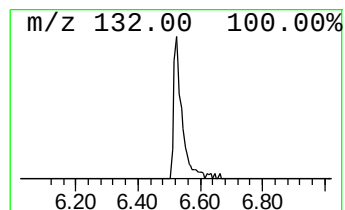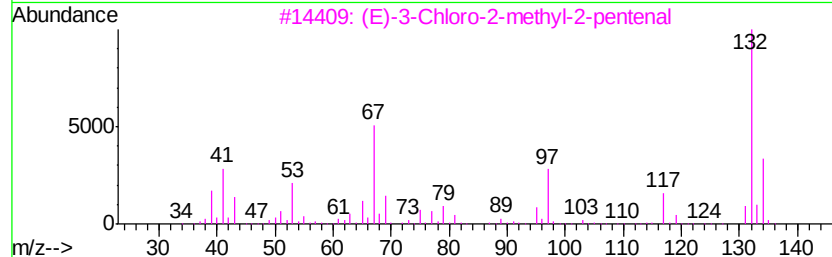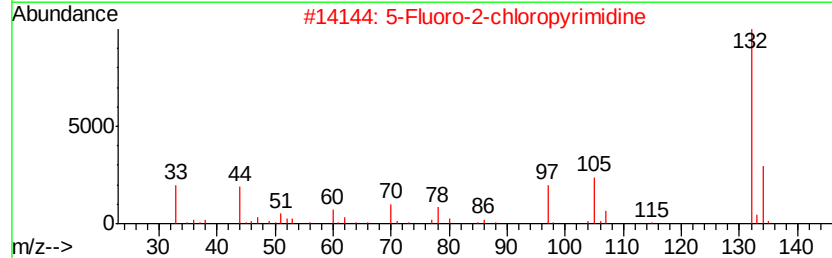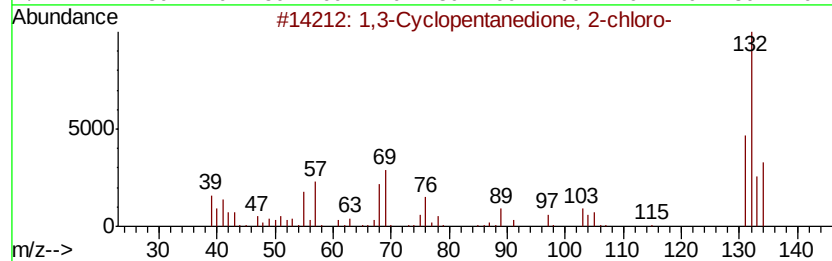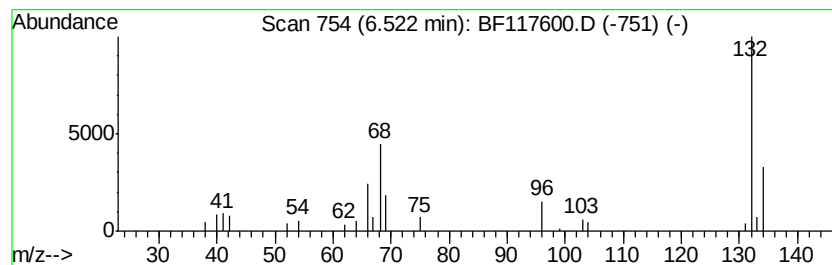

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102919\
Data File : BF117600.D
Acq On : 29 Oct 2019 19:25
Operator : JU
Sample : K5498-01 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
189-62-(0-1)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.52	6.52	5.1	ng	54210	1	6.73	211792	20.0