

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102919\
 Data File : BF117602.D
 Acq On : 29 Oct 2019 20:18
 Operator : JU
 Sample : K5497-19 2X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 189-04-(0-1.2)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.392	558	562	578	rBV2	10165	30049	10.67%	1.739%
2	6.422	733	737	751	rBV2	14758	39418	13.99%	2.281%
3	6.522	751	754	766	rVB2	30111	49880	17.71%	2.887%
4	6.728	786	789	800	rBV	201686	207660	73.71%	12.019%
5	6.886	813	816	824	rBV	33832	38552	13.68%	2.231%
6	7.328	887	891	903	rBV2	6222	17731	6.29%	1.026%
7	8.010	1004	1007	1030	rBV	220592	276566	98.17%	16.007%
8	9.086	1187	1190	1205	rBV	35600	46654	16.56%	2.700%
9	9.763	1301	1305	1323	rBB	283526	281717	100.00%	16.305%
10	10.569	1439	1442	1448	rBB2	10121	12387	4.40%	0.717%
11	11.251	1554	1558	1572	rBV	229847	245446	87.13%	14.206%
12	11.792	1645	1650	1654	rBV3	2128	3913	1.39%	0.226%
13	12.480	1763	1767	1769	rVB	3366	4398	1.56%	0.255%
14	12.698	1801	1804	1806	rBV3	4495	4240	1.51%	0.245%
15	12.827	1824	1826	1830	rBV	49697	44634	15.84%	2.583%
16	13.010	1852	1857	1858	rBV3	3364	4317	1.53%	0.250%
17	13.145	1877	1880	1881	rBV2	3548	3450	1.22%	0.200%
18	13.174	1881	1885	1888	rVV6	3339	5207	1.85%	0.301%
19	13.721	1974	1978	1980	rBV5	5870	9060	3.22%	0.524%
20	13.868	1999	2003	2004	rBV4	5966	7966	2.83%	0.461%
21	13.898	2004	2008	2013	rBV	209041	232423	82.50%	13.452%
22	15.333	2248	2252	2259	rVB	119579	162085	57.53%	9.381%


Sum of corrected areas: 1727753

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102919\
Data File : BF117602.D
Acq On : 29 Oct 2019 20:18
Operator : JU
Sample : K5497-19 2X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
189-04-(0-1.2)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

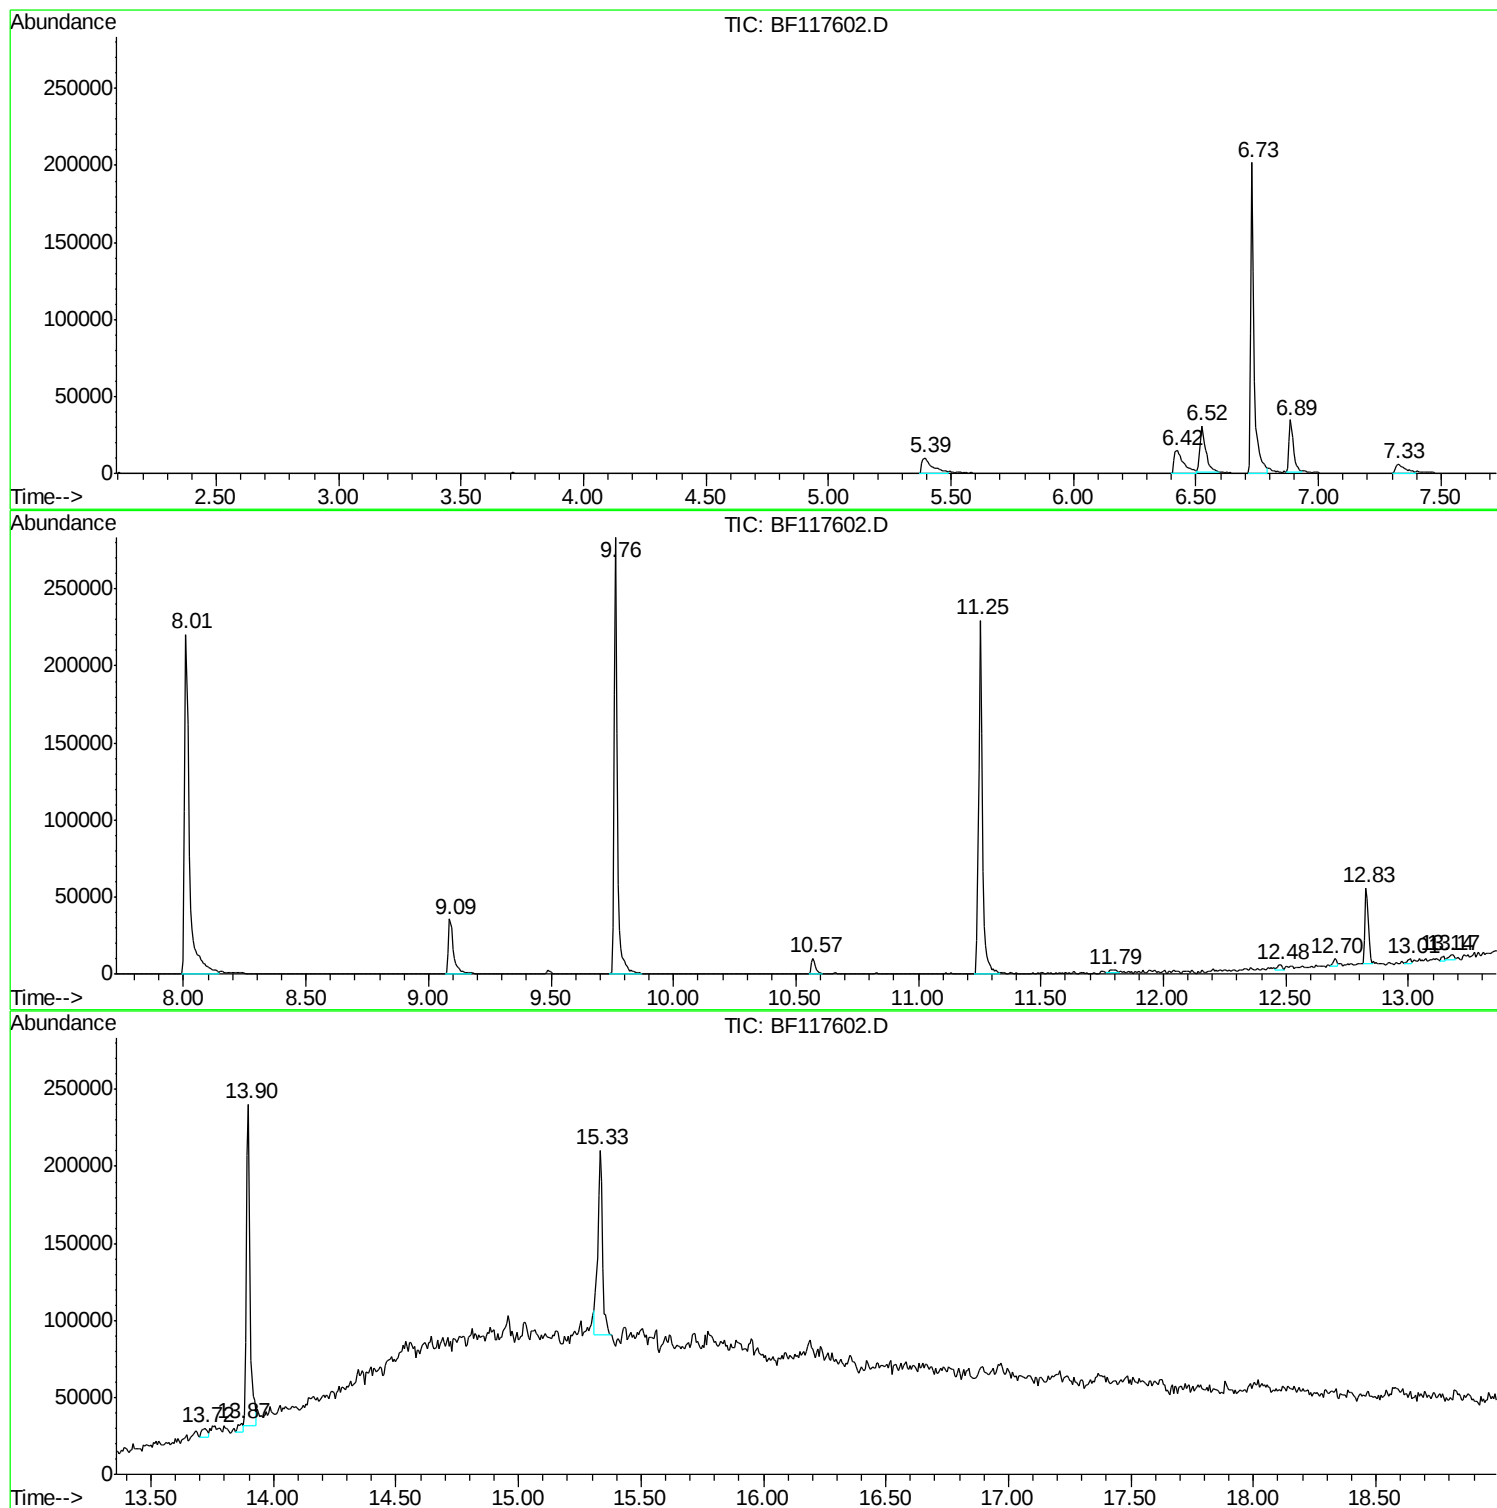

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102919\
Data File : BF117602.D
Acq On : 29 Oct 2019 20:18
Operator : JU
Sample : K5497-19 2X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
189-04-(0-1.2)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.52 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.52	4.80 ng	49880	1,4-Dichlorobenzene-d4	6.73

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	12
2			2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
3			1,2,4-Trifluorobenzene	132	C6H3F3	000367-23-7	9
4			4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

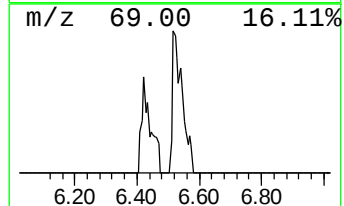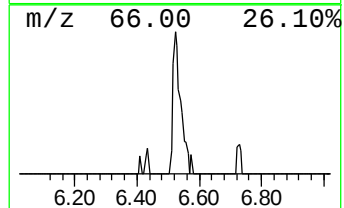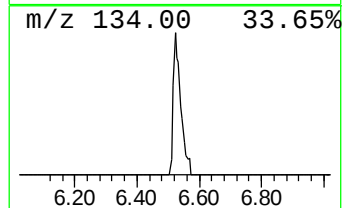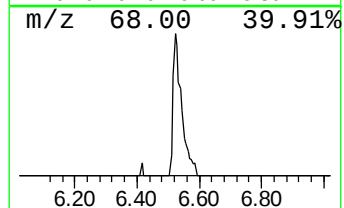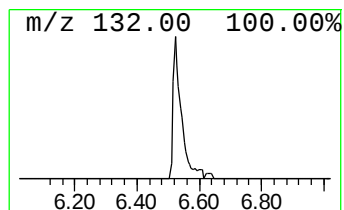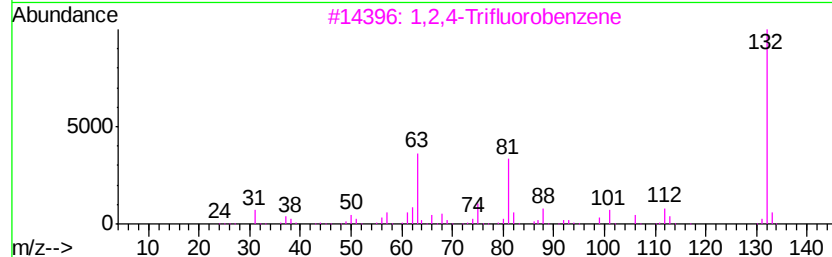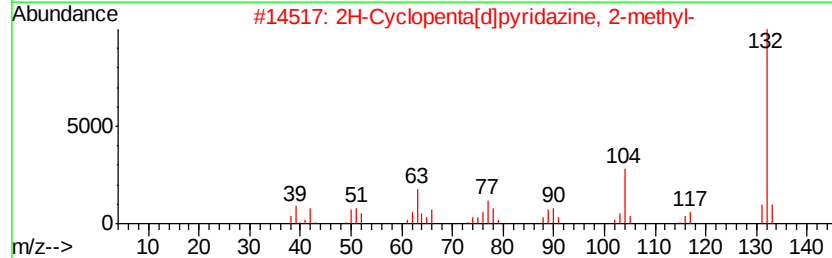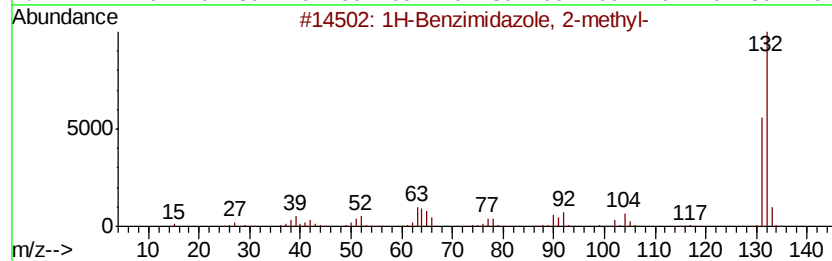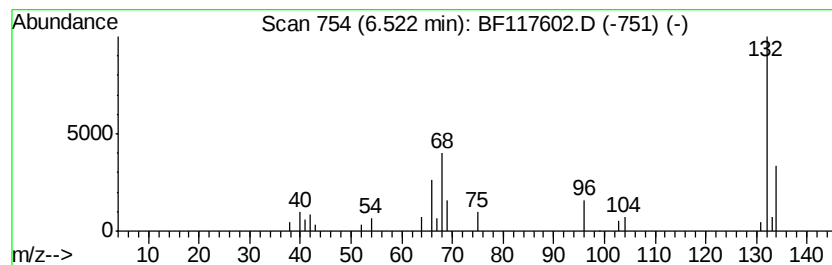

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102919\
Data File : BF117602.D
Acq On : 29 Oct 2019 20:18
Operator : JU
Sample : K5497-19 2X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
189-04-(0-1.2)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.52	6.52	4.8	ng	49880	1	6.73	207660	20.0