


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102919\
 Data File : BF117603.D
 Acq On : 29 Oct 2019 21:39
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 18 18:53:31 2019

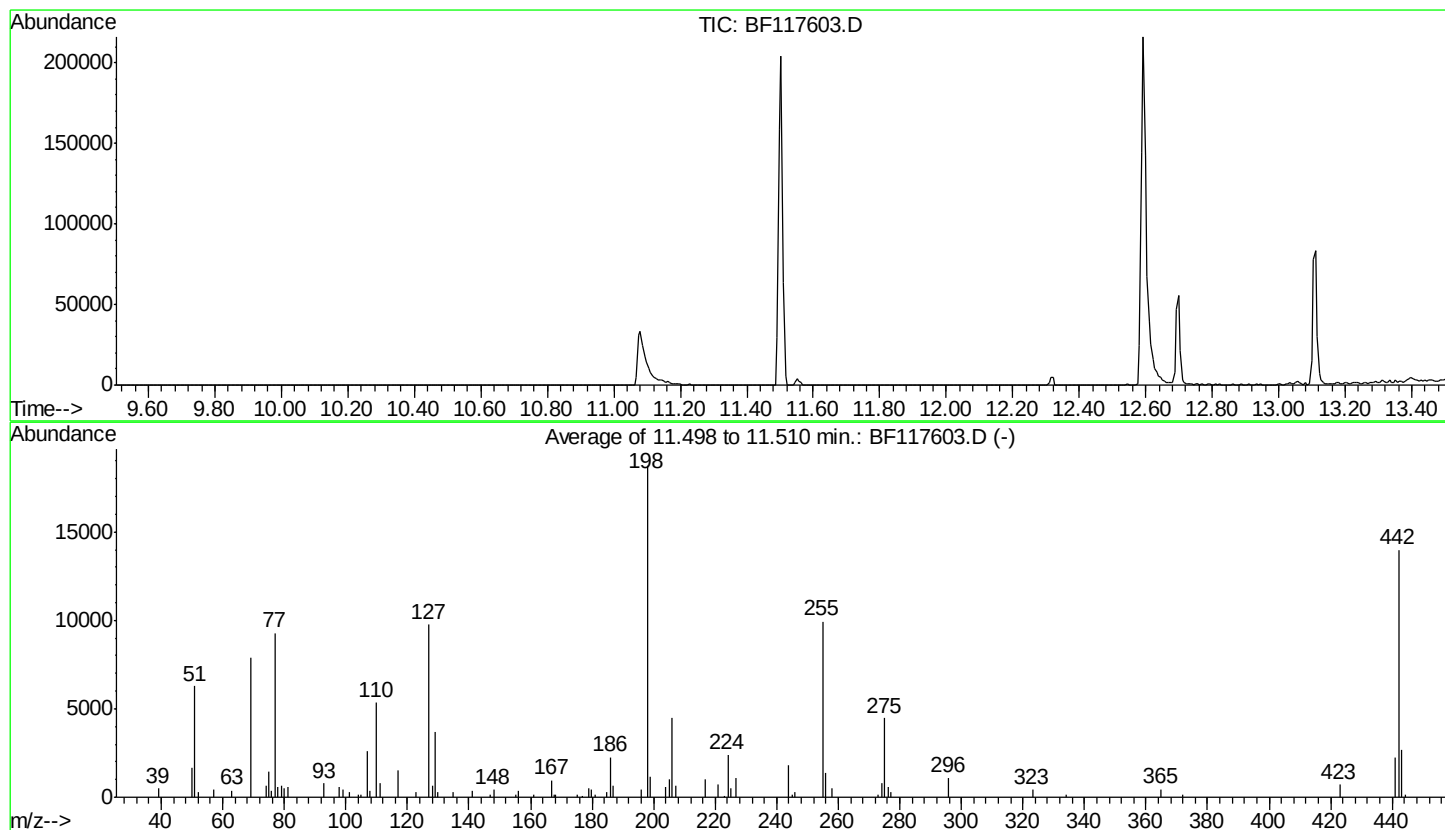

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	6282	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.0	7879	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.0	9738	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18742	PASS
199	198	5	9	6.4	1191	PASS
275	198	10	60	23.9	4484	PASS
365	198	1	100	2.4	443	PASS
441	198	0.01	100	12.1	2274	PASS
442	198	50	100	74.5	13966	PASS
443	442	15	24	19.2	2675	PASS