


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102921\
 Data File : BF126000.D
 Acq On : 29 Oct 2021 10:33
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 29 18:20:18 2021

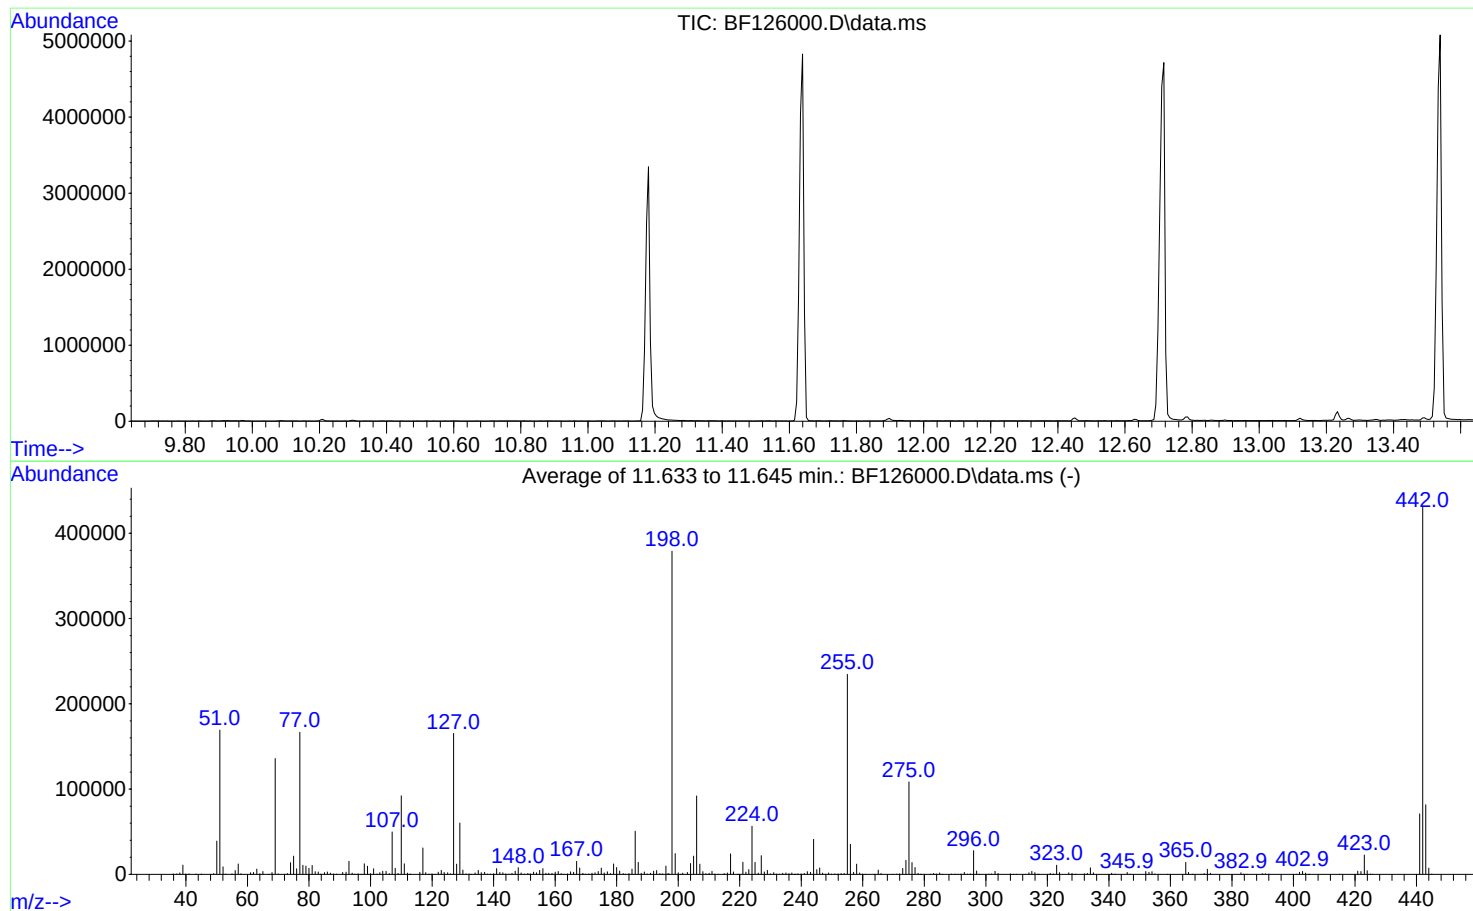




AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.6	169168	PASS
68	69	0.00	2	1.5	2073	PASS
69	198	0.00	100	35.9	135861	PASS
70	69	0.00	2	0.5	647	PASS
127	198	10	80	43.6	165280	PASS
197	198	0.00	2	0.3	1032	PASS
198	198	100	100	100.0	378944	PASS
199	198	5	9	6.5	24477	PASS
275	198	10	60	28.6	108424	PASS
365	198	1	100	3.7	14150	PASS
441	198	0.01	100	18.7	70933	PASS
442	442	50	100	100.0	431403	PASS
443	442	15	24	18.9	81587	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102921\
 Data File : BF126000.D
 Acq On : 29 Oct 2021 10:33
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 29 12:58:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 28 12:01:54 2021
 Response via : Initial Calibration

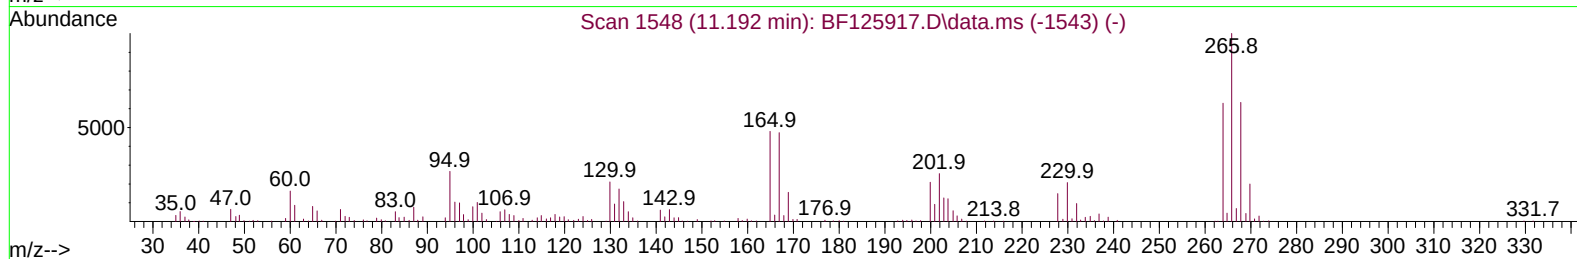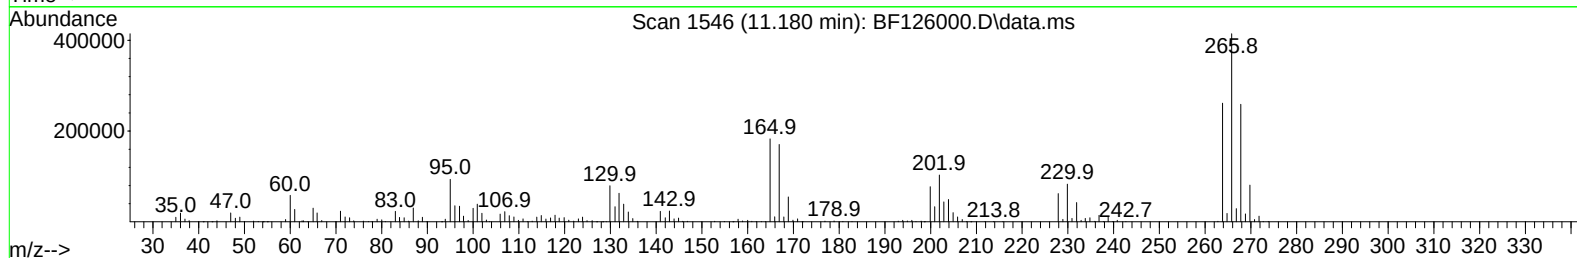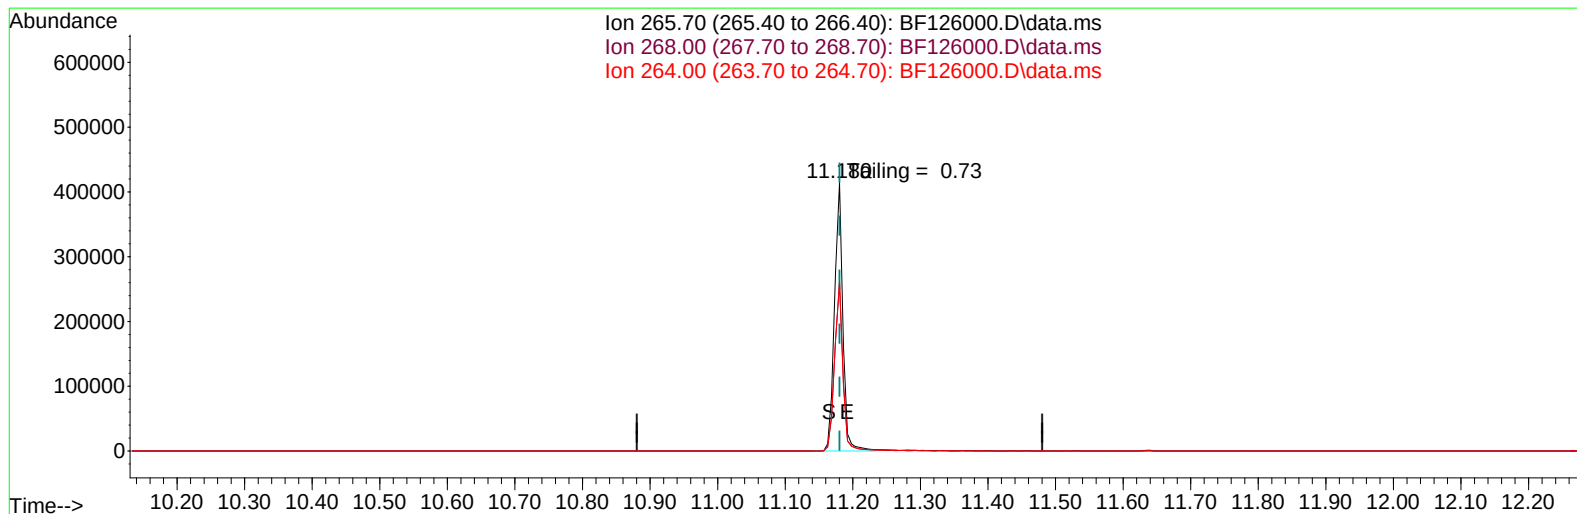

TIC: BF126000.D\data.ms

(70) Pentachlorophenol (C)

11.180min (-0.000) 33717.14 ng




response 359288

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.49
264.00	69.90	63.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102921\
Data File : BF126000.D
Acq On : 29 Oct 2021 10:33
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 29 12:58:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 28 12:01:54 2021
Response via : Initial Calibration

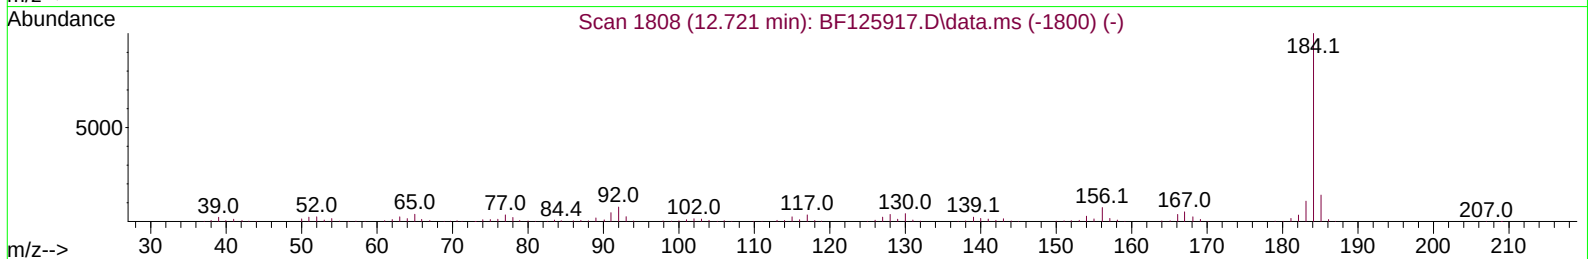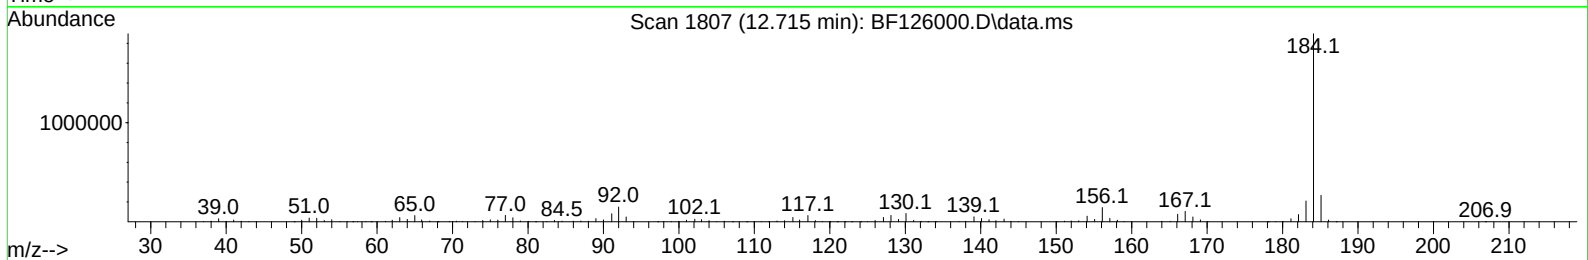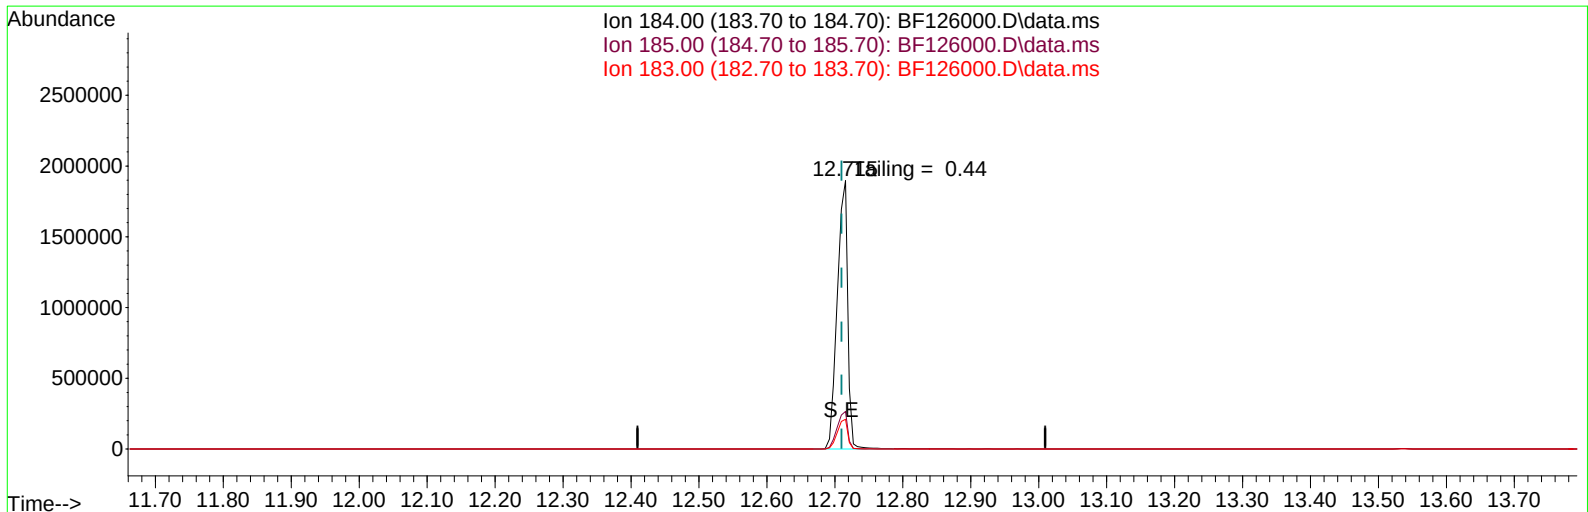

TIC: BF126000.D\data.ms

(77) Benzidine

12.715min (+ 0.006) 0.00 ng

response 2027643

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.02
183.00	10.10	11.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/29/2021	BNA_F	<u>BF126000.D</u>
Compound Name	Response	Retention Time
DDT	900056	13.53
DDD	19782	13.23
DDE	874	12.89
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20656	920712	2.24

Instrument :
BNA_F
ClientSampleId :
DFTPP