

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102925\
 Data File : BF144136.D
 Acq On : 29 Oct 2025 19:01
 Operator : RC/JU
 Sample : Q3466-07 2X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B7-1.0-2.0-20251023

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF144136.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.087	489	492	502	rVB3	4076	6458	1.16%	0.111%
2	5.493	556	561	584	rBV	328567	473219	85.33%	8.109%
3	6.498	727	732	757	rBV	348592	487834	87.97%	8.360%
4	6.875	791	796	802	rBV	308888	380563	68.62%	6.522%
5	7.434	886	891	903	rBV	209134	285451	51.47%	4.892%
6	8.157	1009	1014	1030	rBV	367834	479542	86.47%	8.218%
7	9.234	1192	1197	1207	rBV	410486	521340	94.01%	8.934%
8	9.916	1308	1313	1321	rBV	436082	541910	97.72%	9.286%
9	10.628	1430	1434	1442	rBV	36458	46940	8.46%	0.804%
10	10.704	1442	1447	1457	rVV	234557	308212	55.58%	5.282%
11	10.939	1484	1487	1495	rVB2	4639	6189	1.12%	0.106%
12	11.404	1561	1566	1573	rBV	403583	522267	94.18%	8.950%
13	11.928	1650	1655	1664	rBV5	14408	28585	5.15%	0.490%
14	12.428	1735	1740	1743	rBV5	4010	6117	1.10%	0.105%
15	12.498	1748	1752	1759	rVB9	4669	8114	1.46%	0.139%
16	12.622	1769	1773	1777	rBV	25758	31721	5.72%	0.544%
17	12.722	1785	1790	1791	rBV5	4425	6109	1.10%	0.105%
18	12.804	1799	1804	1807	rBV	13578	17858	3.22%	0.306%
19	12.851	1807	1812	1818	rVV	34614	49870	8.99%	0.855%
20	12.992	1831	1836	1844	rVB	347310	446704	80.55%	7.655%
21	13.069	1845	1849	1855	rBV6	5084	11231	2.03%	0.192%
22	13.175	1865	1867	1871	rVB3	6528	8038	1.45%	0.138%
23	13.280	1883	1885	1892	rVB6	7282	12924	2.33%	0.221%
24	13.563	1930	1933	1935	rBV5	6904	9692	1.75%	0.166%
25	14.051	2011	2016	2029	rVB	383876	554561	100.00%	9.503%
26	15.104	2191	2195	2202	rBV	32418	71152	12.83%	1.219%
27	15.539	2263	2269	2284	rVB	293323	512896	92.49%	8.789%




Sum of corrected areas: 5835497

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102925\
Data File : BF144136.D
Acq On : 29 Oct 2025 19:01
Operator : RC/JU
Sample : Q3466-07 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B7-1.0-2.0-20251023

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

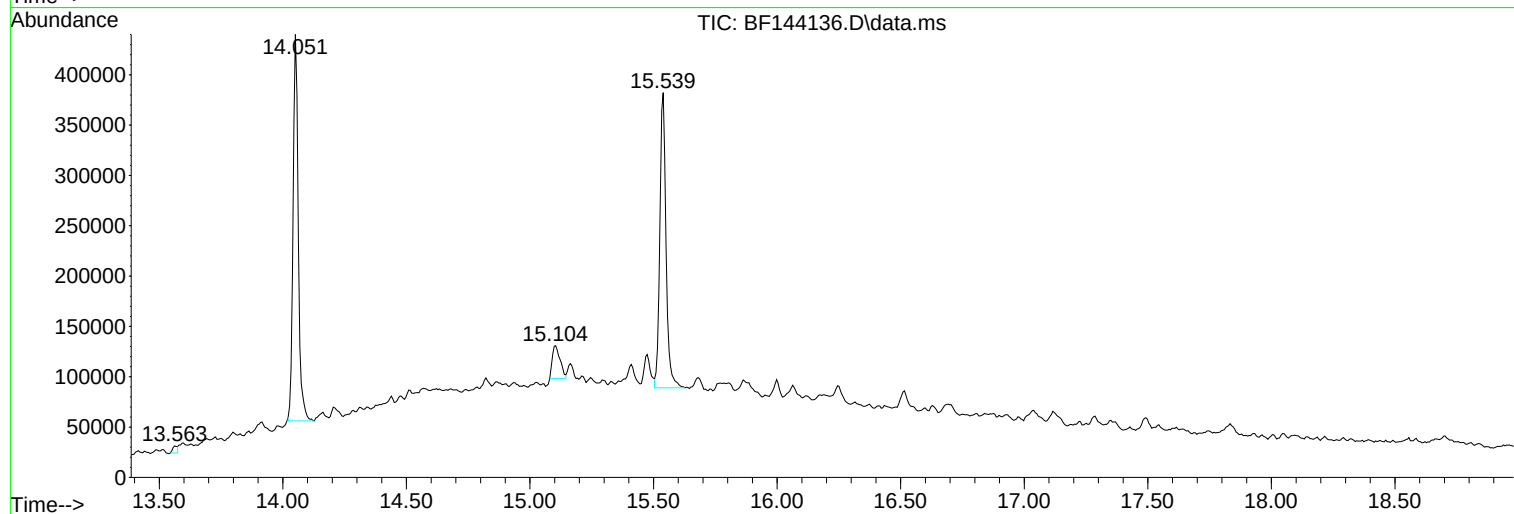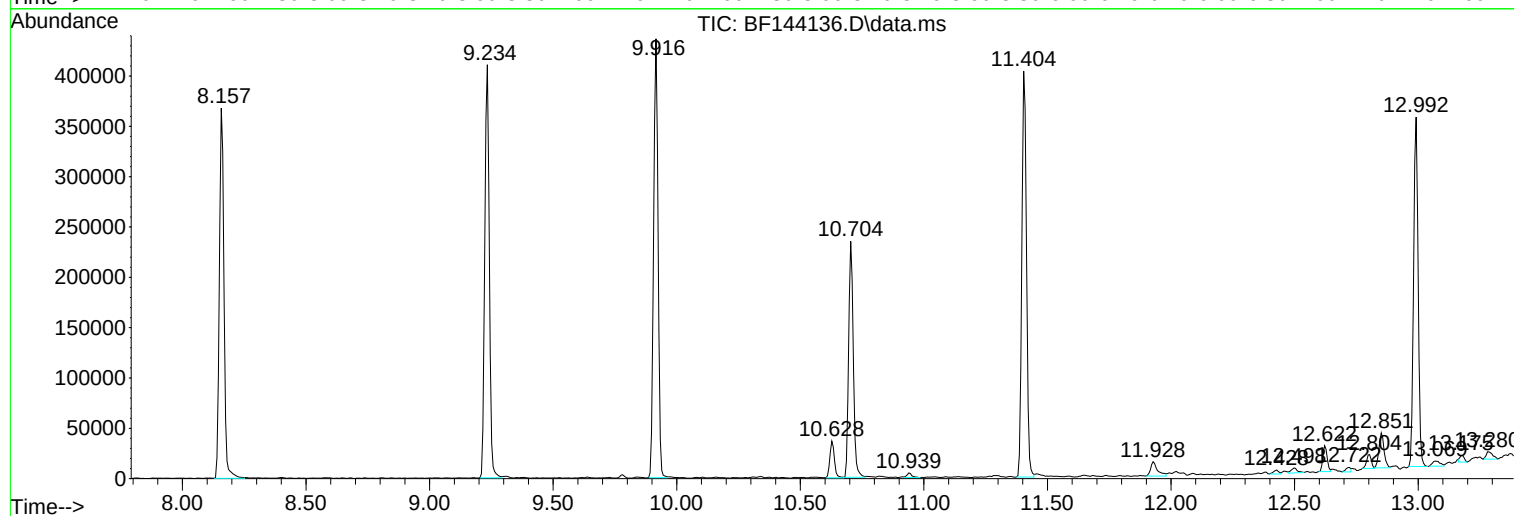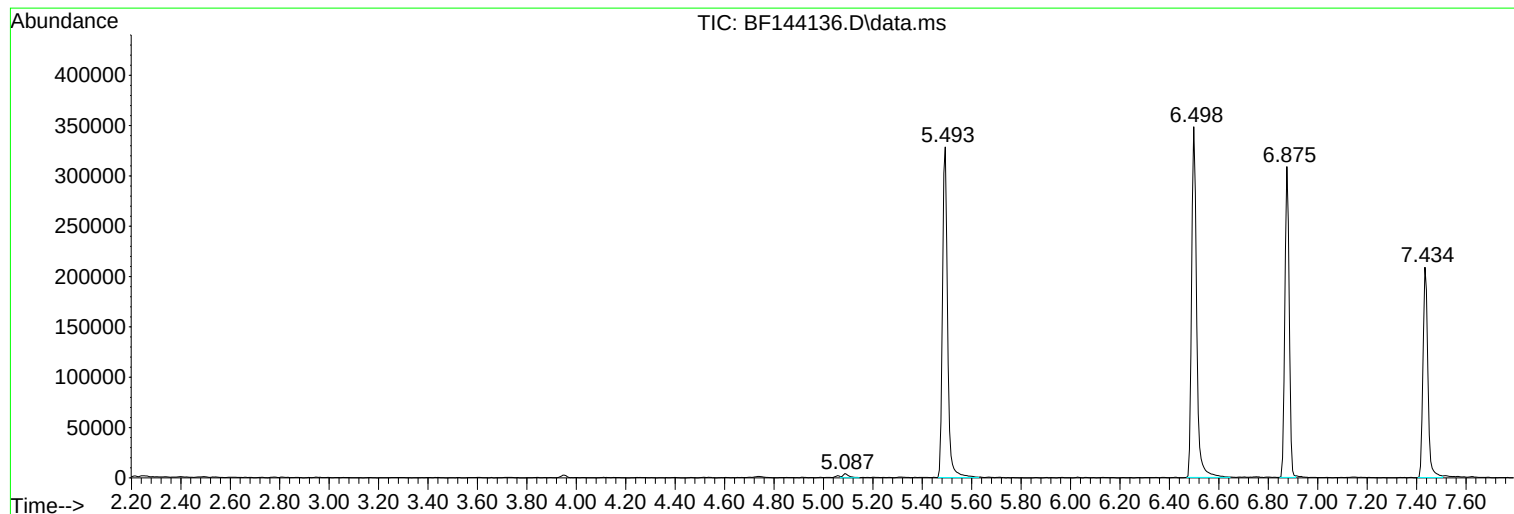

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102925\
Data File : BF144136.D
Acq On : 29 Oct 2025 19:01
Operator : RC/JU
Sample : Q3466-07 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B7-1.0-2.0-20251023

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102925\
Data File : BF144136.D
Acq On : 29 Oct 2025 19:01
Operator : RC/JU
Sample : Q3466-07 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B7-1.0-2.0-20251023

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
