
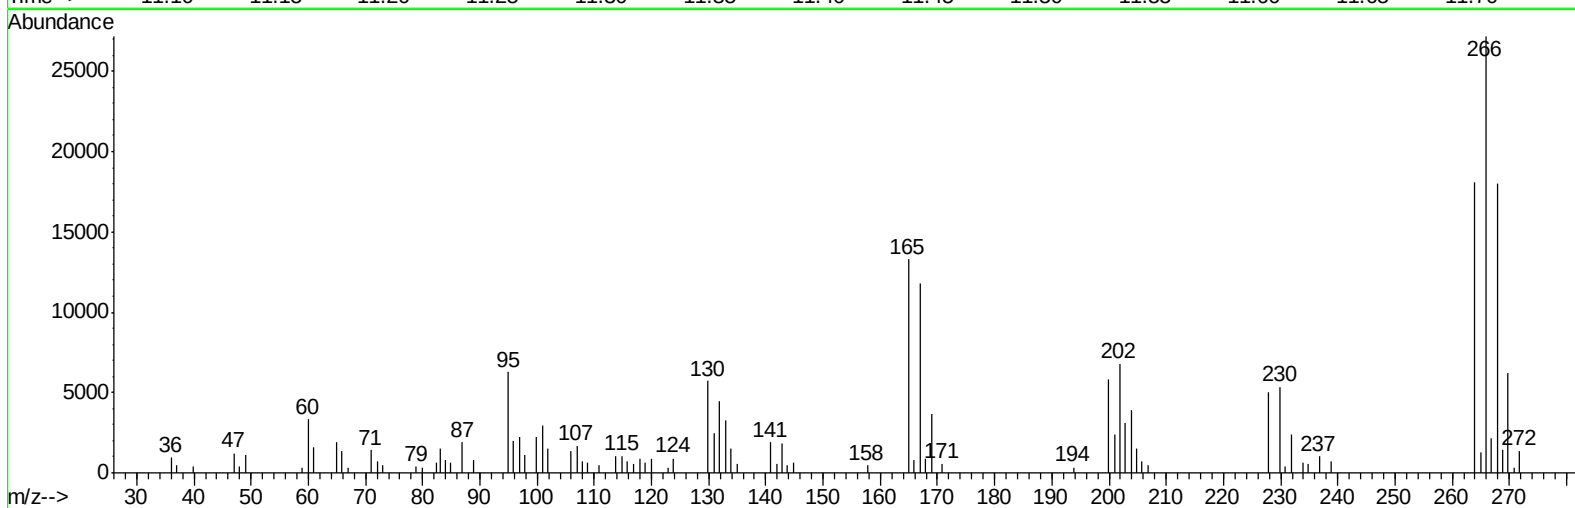


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF103018\
Data File : BF110297.D
Acq On : 30 Oct 2018 12:38
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 08:01:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 29 17:29:00 2018
Response via : Initial Calibration

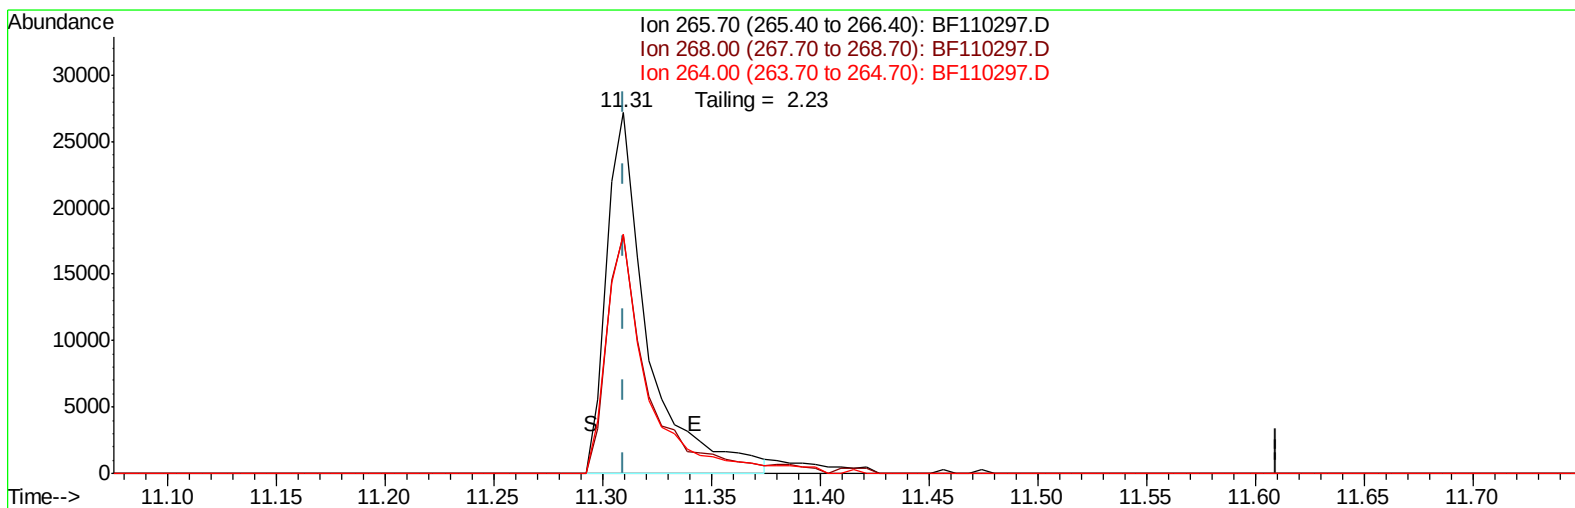

TIC: BF110297.D

(70) Pentachlorophenol (C)



11.310min (+0.000) 30139.65ng

response 37622

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	66.17
264.00	63.20	66.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF103018\
Data File : BF110297.D
Acq On : 30 Oct 2018 12:38
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 08:01:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 29 17:29:00 2018
Response via : Initial Calibration

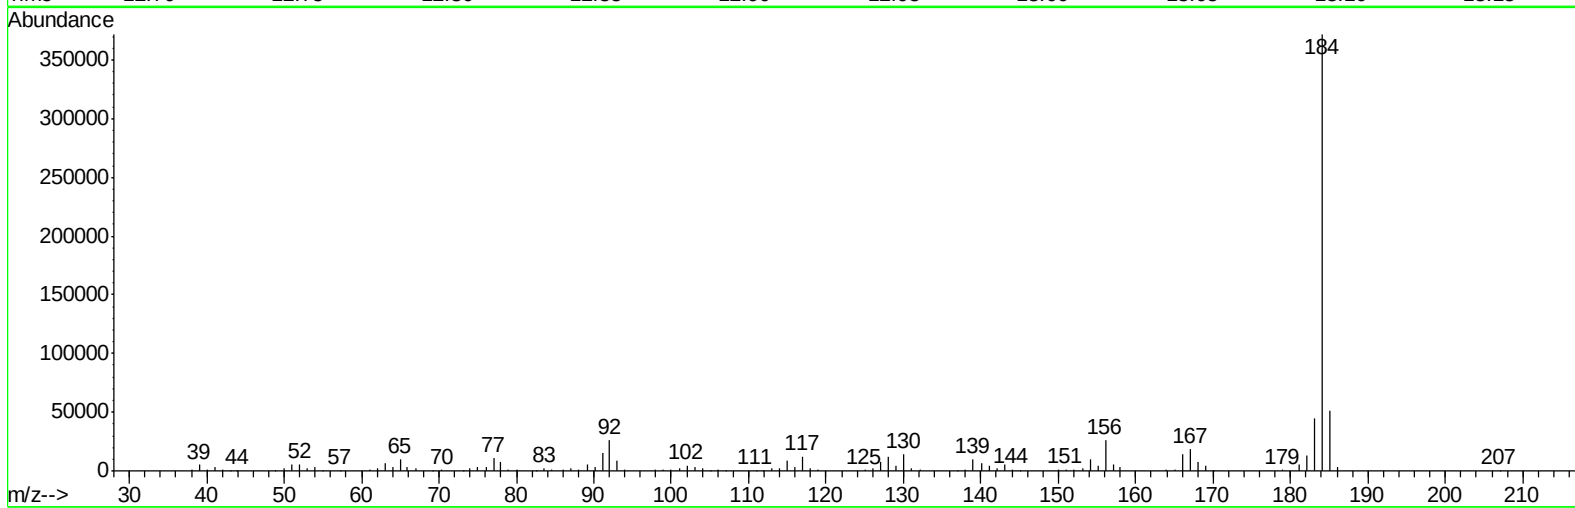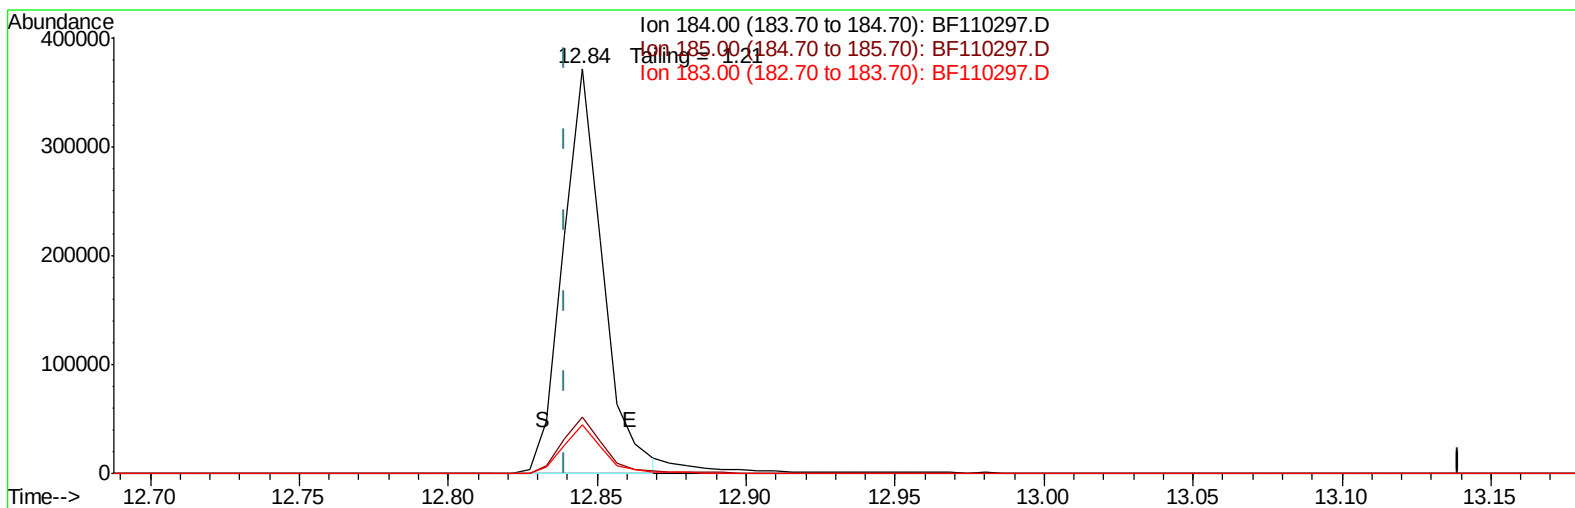

TIC: BF110297.D

(77) Benzidine

12.845min (+0.006) 0.00ng

response 355377

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	13.85
183.00	11.80	12.13
0.00	0.00	0.00