

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF103018\
 Data File : BF110307.D
 Acq On : 30 Oct 2018 17:08
 Operator : JU/SJ
 Sample : J5722-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 102618-TIPC-F-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.316	33	39	55	rVB	1339716	1808016	61.24%	9.156%
2	5.198	526	529	538	rBV	27106	34011	1.15%	0.172%
3	5.587	591	595	615	rBV	750477	722483	24.47%	3.659%
4	6.581	761	764	776	rBV2	510724	589956	19.98%	2.988%
5	6.734	786	790	797	rBV	1700765	1477832	50.06%	7.484%
6	6.969	826	830	836	rBV	775350	631263	21.38%	3.197%
7	7.128	852	857	860	rBV	2246057	2066928	70.01%	10.467%
8	7.533	921	926	929	rBV	1793706	1707823	57.85%	8.648%
9	8.251	1044	1048	1053	rBV	866135	765983	25.94%	3.879%
10	9.327	1226	1231	1234	rBV	3480893	2952380	100.00%	14.951%
11	9.716	1294	1297	1303	rBV	34673	37164	1.26%	0.188%
12	10.010	1344	1347	1359	rVB	859434	840832	28.48%	4.258%
13	10.804	1478	1482	1494	rBV	1135727	1035745	35.08%	5.245%
14	11.504	1598	1601	1610	rBV	765959	719296	24.36%	3.643%
15	13.092	1866	1871	1874	rBV	2518925	2148844	72.78%	10.882%
16	13.974	2017	2021	2025	rBV	43510	55250	1.87%	0.280%
17	14.157	2048	2052	2059	rBV	571125	533317	18.06%	2.701%
18	14.286	2071	2074	2080	rBV	40094	43507	1.47%	0.220%
19	14.592	2123	2126	2131	rBV	89936	83302	2.82%	0.422%
20	14.915	2177	2181	2185	rVB	122983	129120	4.37%	0.654%
21	15.268	2236	2241	2246	rBV	164908	205557	6.96%	1.041%
22	15.686	2305	2312	2322	rBV2	344269	700368	23.72%	3.547%
23	16.133	2383	2388	2395	rVB	150827	239744	8.12%	1.214%
24	16.674	2474	2480	2487	rBV	87615	151536	5.13%	0.767%
25	17.303	2581	2587	2595	rBV3	29770	66907	2.27%	0.339%


Sum of corrected areas: 19747164

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF103018\
Data File : BF110307.D
Acq On : 30 Oct 2018 17:08
Operator : JU/SJ
Sample : J5722-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
102618-TIPC-F-U-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

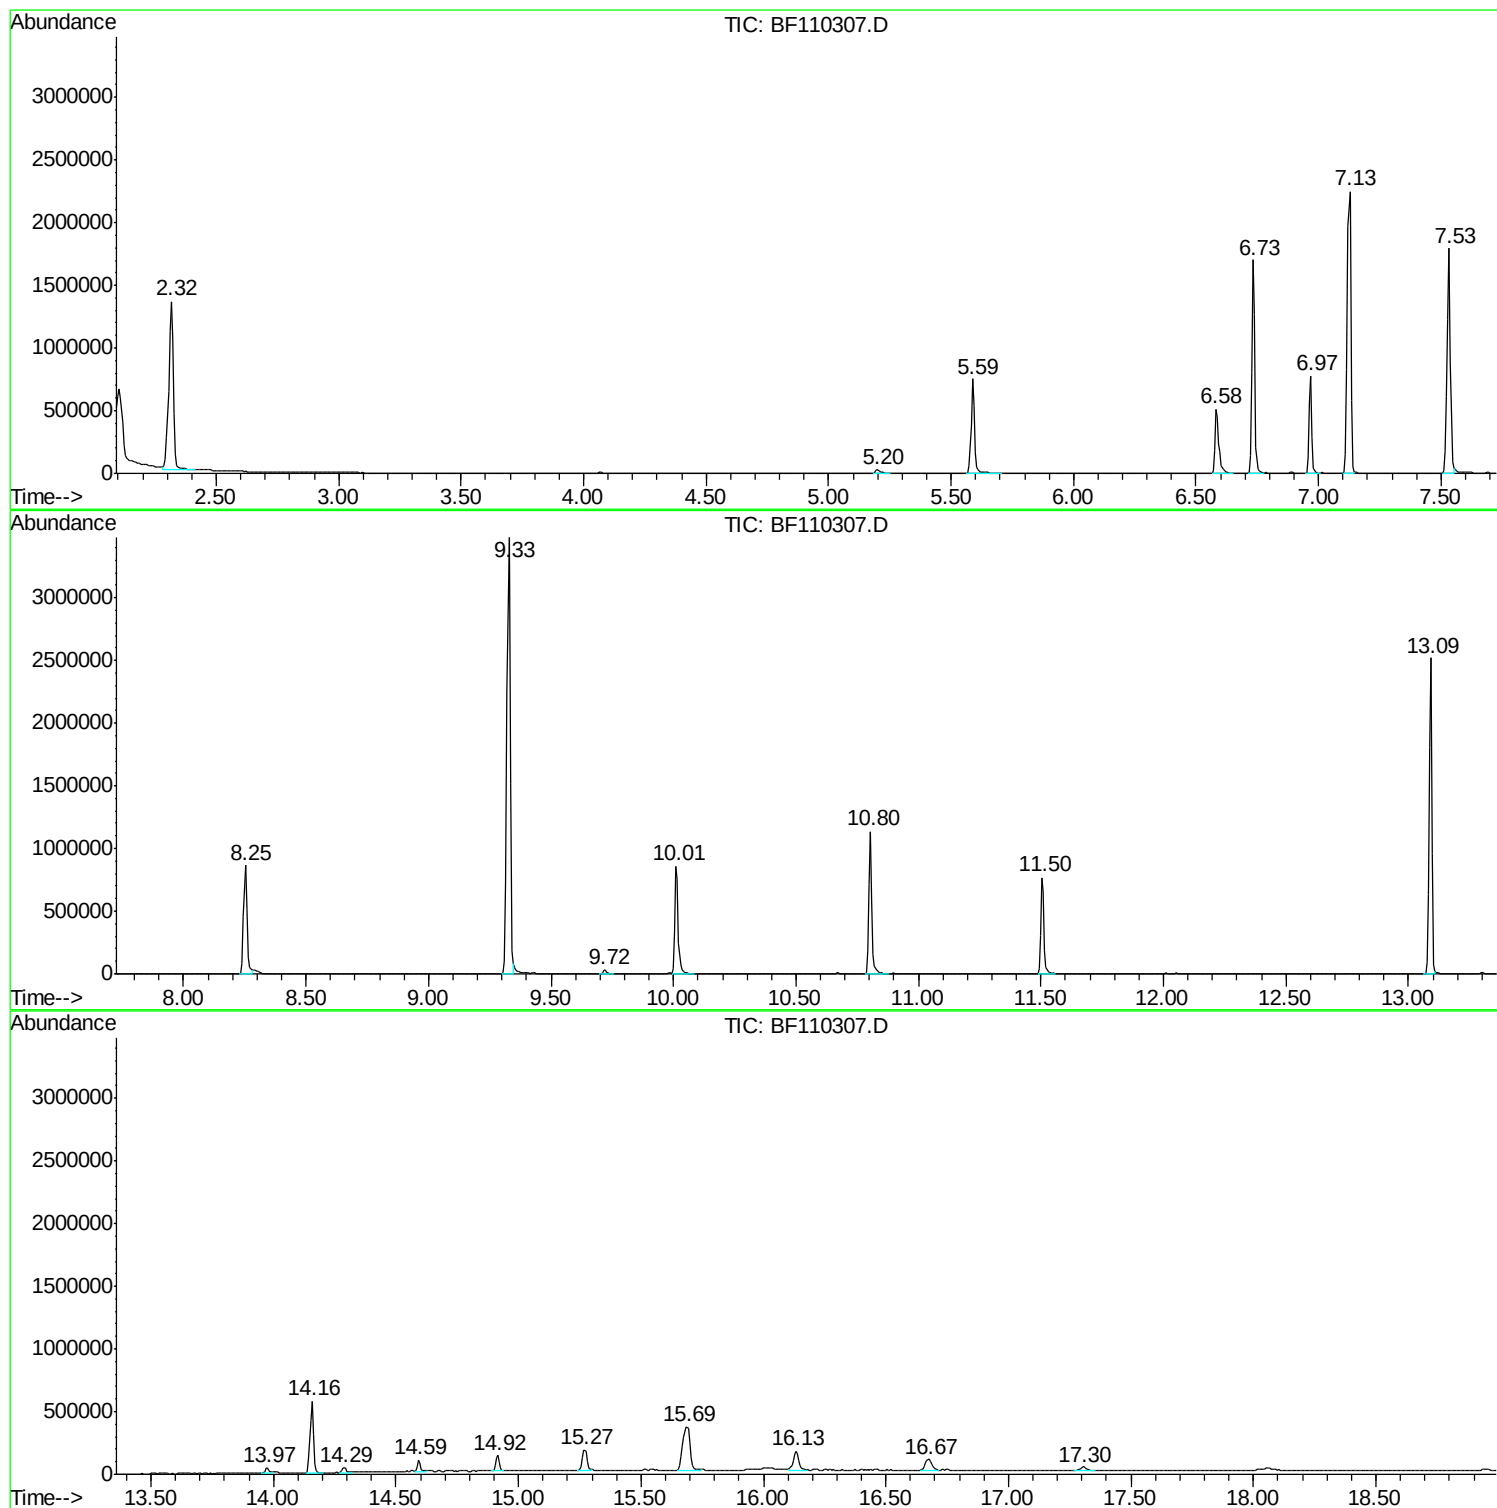

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF103018\
Data_File : BF110307.D
Acq_On : 30-Oct-2018 17:088
Operator : JU/SJJ
Sample : J5722-099
Misc :
ALS_Vial : 11 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
102618-TIPC-F-U-B

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
