


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103018\
 Data File : BF110297.D
 Acq On : 30 Oct 2018 12:38
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 29 17:29:00 2018

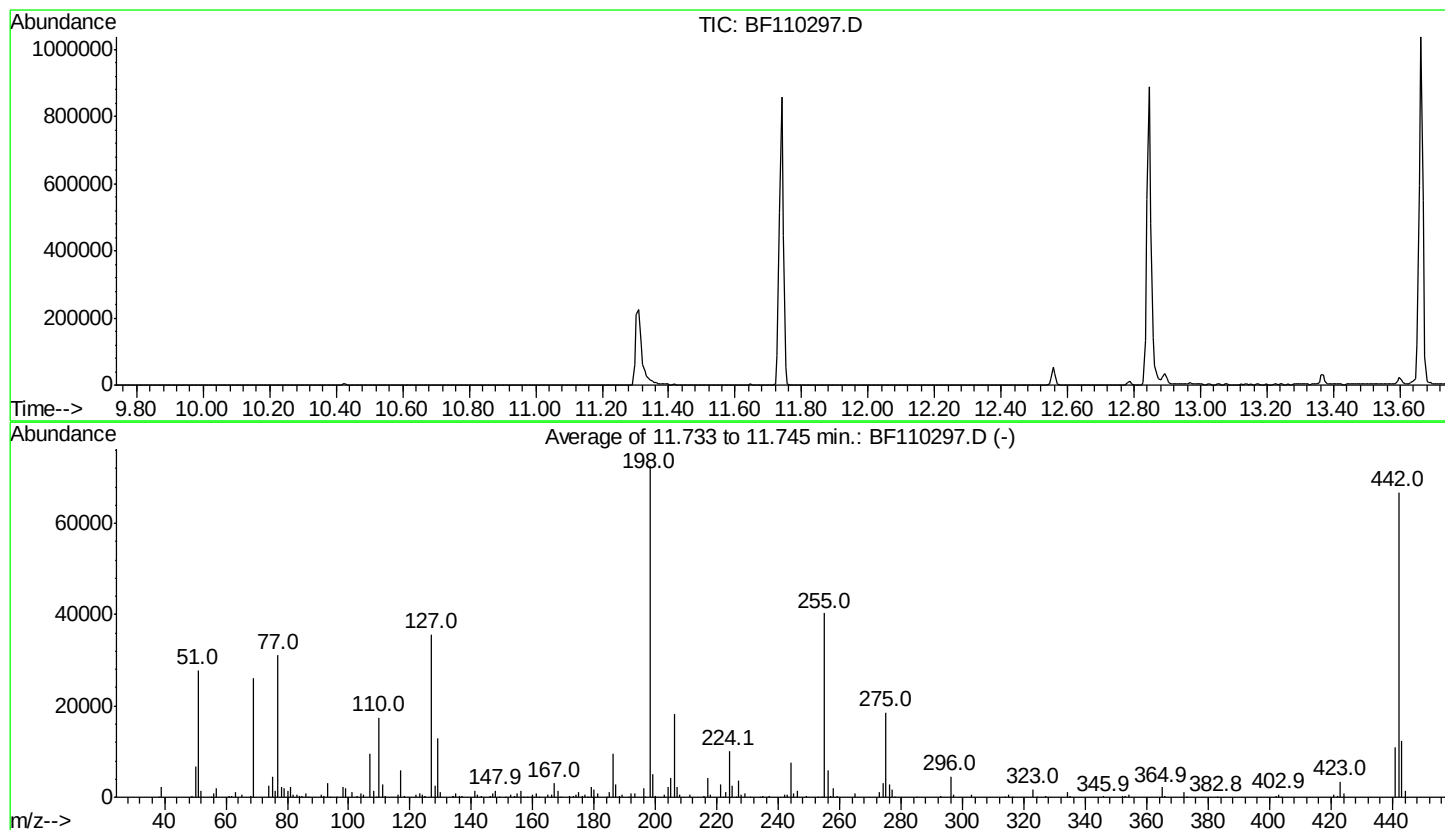

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	27876	PASS
68	69	0.00	2	1.5	403	PASS
69	198	0.00	100	36.0	26201	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.1	35693	PASS
197	198	0.00	2	0.2	133	PASS
198	198	100	100	100.0	72680	PASS
199	198	5	9	6.9	5002	PASS
275	198	10	60	25.7	18656	PASS
365	198	1	100	3.0	2179	PASS
441	198	0.01	100	14.9	10843	PASS
442	198	50	100	92.1	66904	PASS
443	442	15	24	18.4	12321	PASS