
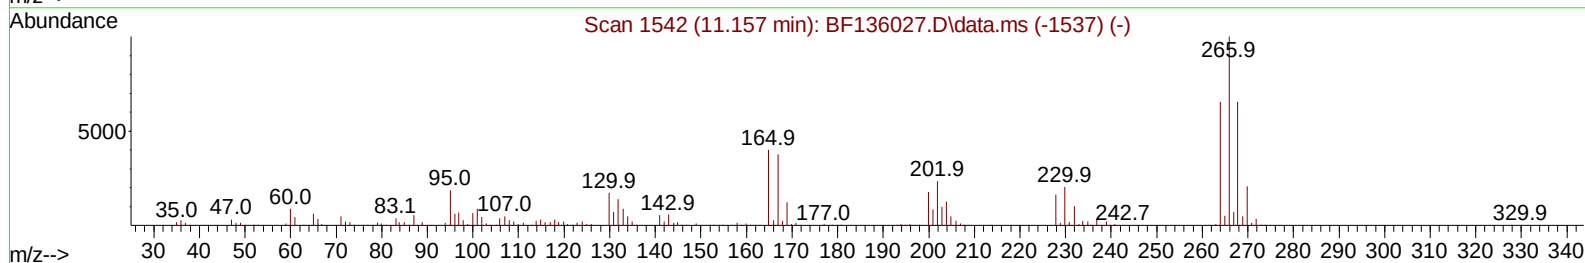
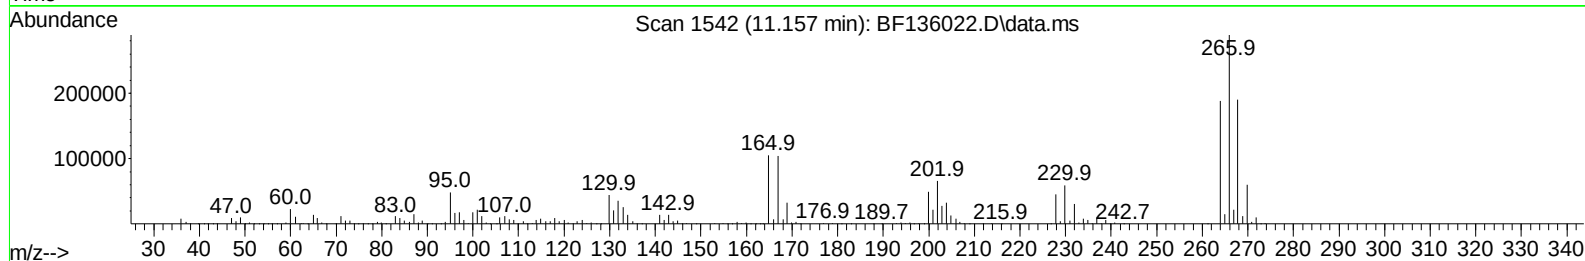


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103023\
Data File : BF136022.D
Acq On : 30 Oct 2023 11:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 01:19:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 01:13:02 2023
Response via : Initial Calibration

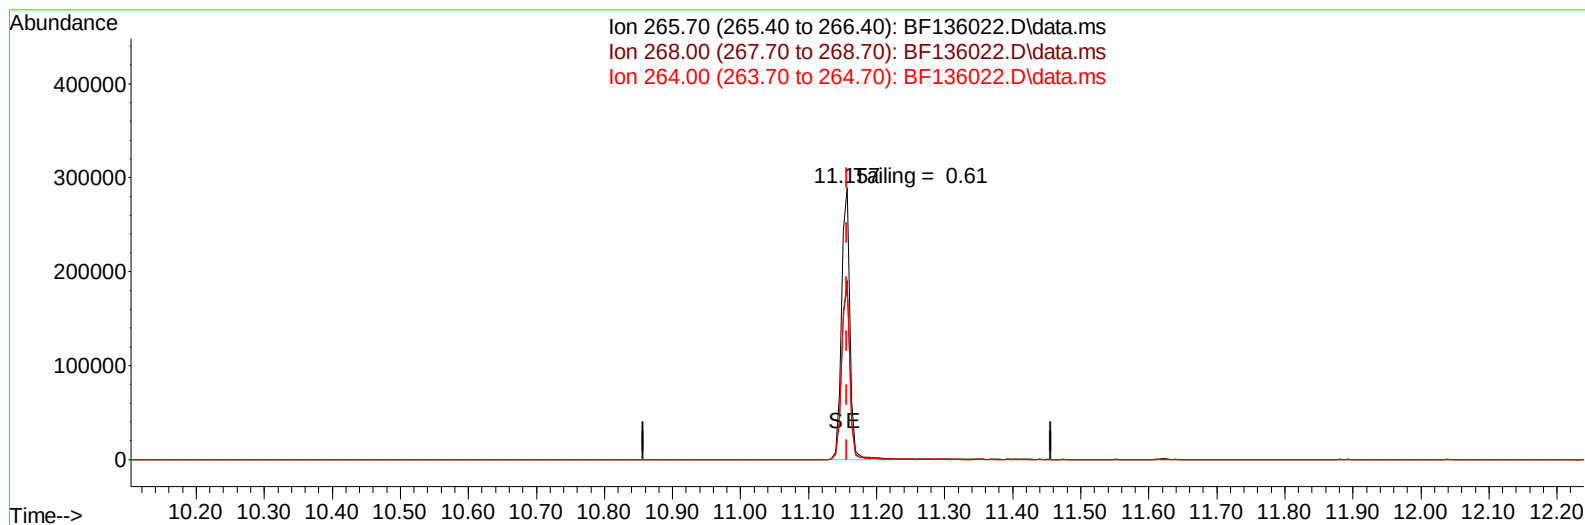

TIC: BF136022.D\data.ms

(70) Pentachlorophenol (C)




11.157min (+ 0.000) 31322.27 ng

response 247319

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	65.83
264.00	65.30	65.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103023\
Data File : BF136022.D
Acq On : 30 Oct 2023 11:02
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 01:19:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 01:13:02 2023
Response via : Initial Calibration

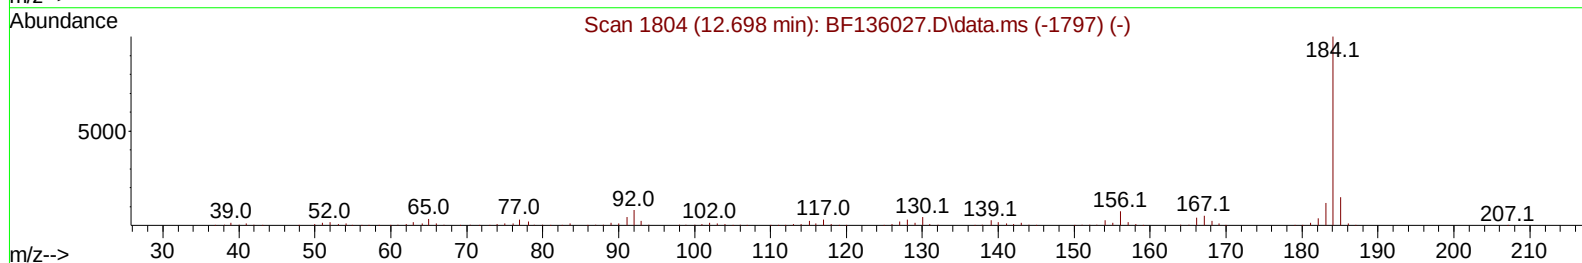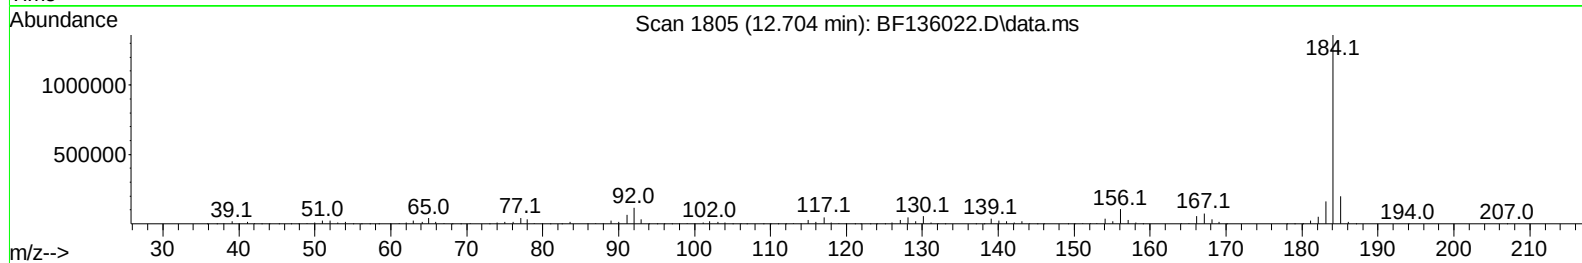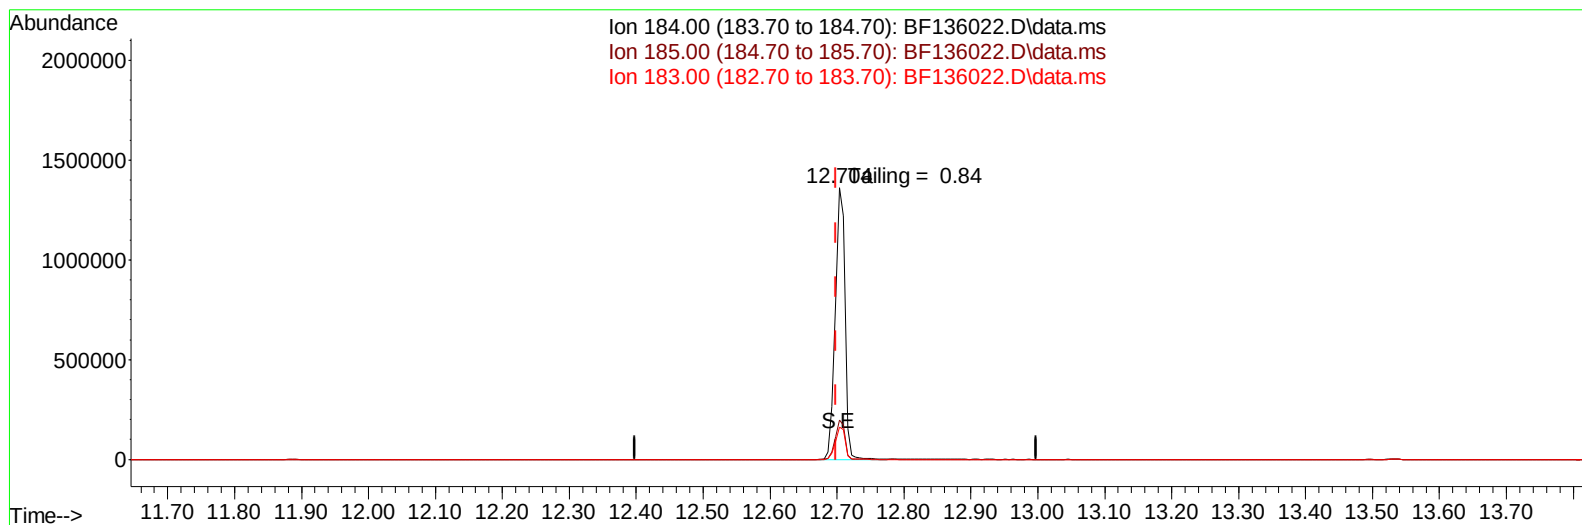

TIC: BF136022.D\data.ms

(77) Benzidine

12.704min (+ 0.006) 70133.47 ng

response 1380629

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.44
183.00	11.90	12.00
0.00	0.00	0.00