

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103023\
 Data File : BF136033.D
 Acq On : 30 Oct 2023 17:56
 Operator : CG\JU
 Sample : PB156392BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB156392BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.157	8	12	21	rVB	89859	123503	2.14%	0.364%
2	5.069	501	507	518	rVB	403897	551801	9.56%	1.625%
3	5.463	568	574	577	rBV	4009926	4432109	76.80%	13.052%
4	6.457	736	743	746	rBV	3875969	4361292	75.57%	12.844%
5	6.822	801	805	808	rBV	1239589	944498	16.37%	2.781%
6	7.387	895	901	904	rBV	2990238	2862717	49.60%	8.430%
7	8.098	1018	1022	1026	rBV	1547780	1250243	21.66%	3.682%
8	9.186	1200	1207	1210	rBV	5458368	5216129	90.38%	15.361%
9	9.857	1317	1321	1325	rBV	1766885	1423137	24.66%	4.191%
10	10.651	1452	1456	1459	rBV	3583701	3302308	57.22%	9.725%
11	11.351	1571	1575	1578	rBV	1828365	1472570	25.52%	4.337%
12	12.957	1843	1848	1851	rBV	5787253	5771060	100.00%	16.995%
13	14.004	2022	2026	2030	rBV	1458631	1242143	21.52%	3.658%
14	15.492	2273	2279	2287	rBV	821069	1003634	17.39%	2.956%




Sum of corrected areas: 33957144

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103023\
Data File : BF136033.D
Acq On : 30 Oct 2023 17:56
Operator : CG\JU
Sample : PB156392BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156392BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

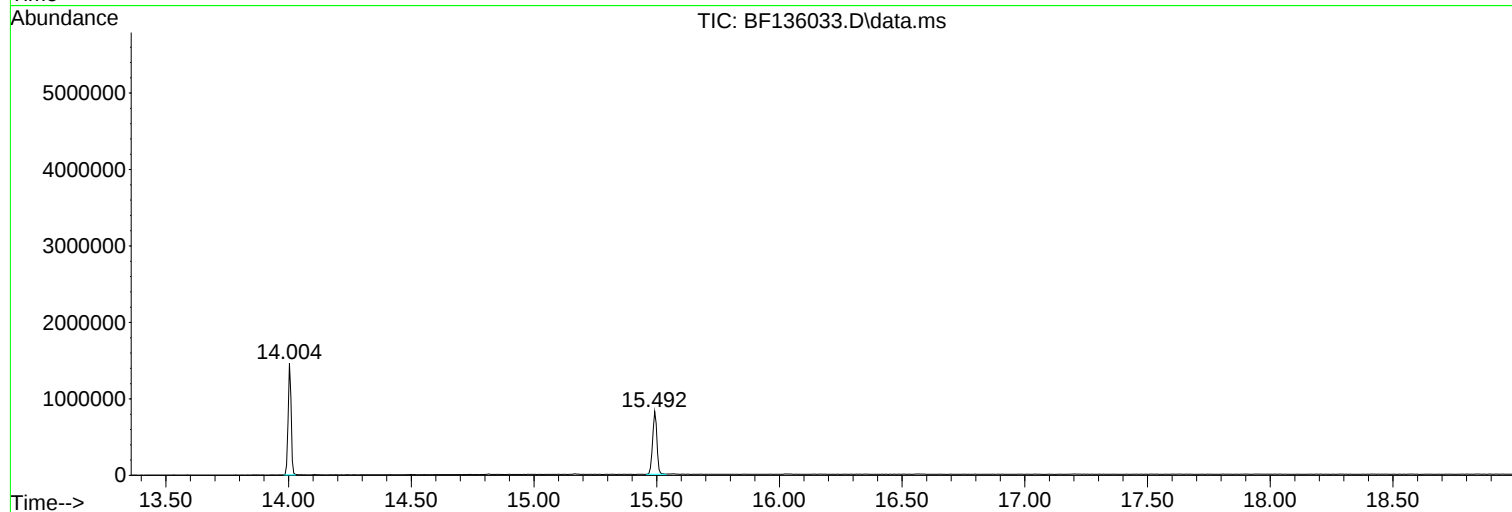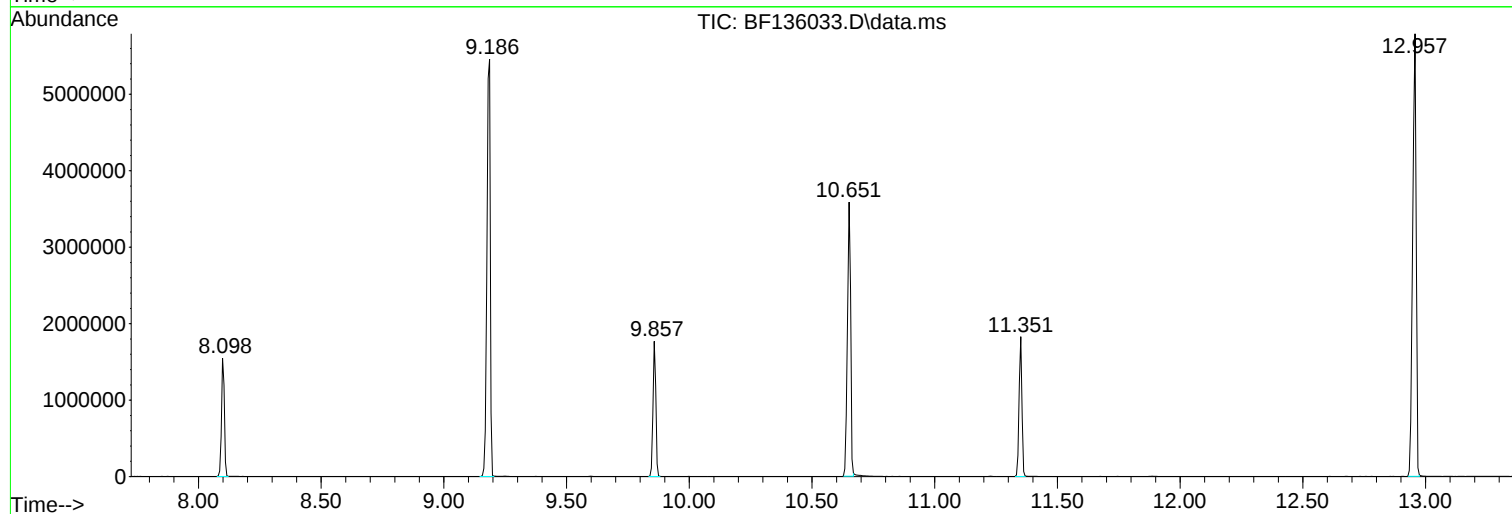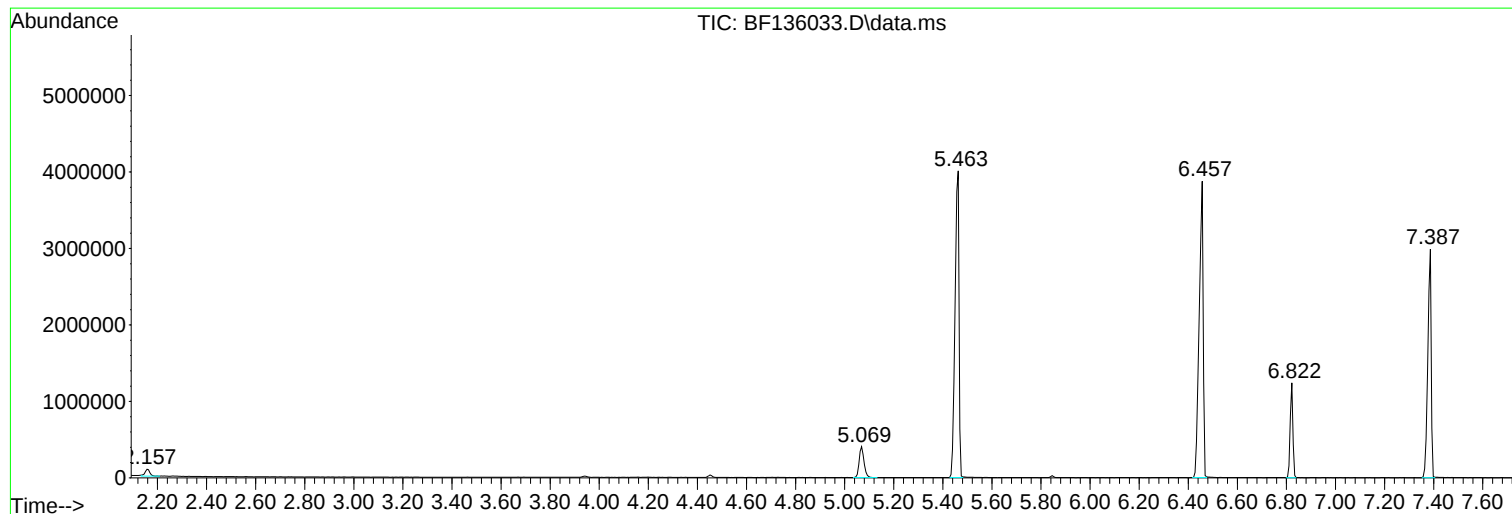

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103023\
Data File : BF136033.D
Acq On : 30 Oct 2023 17:56
Operator : CG\JU
Sample : PB156392BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156392BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.157	2.62 ng	123503	1,4-Dichlorobenzene-d4	6.822

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Silane, tetramethyl-	88	C4H12Si	000075-76-3	32
4			1,3-Dioxolane, 2-propyl-	116	C6H12O2	003390-13-4	23
5			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12

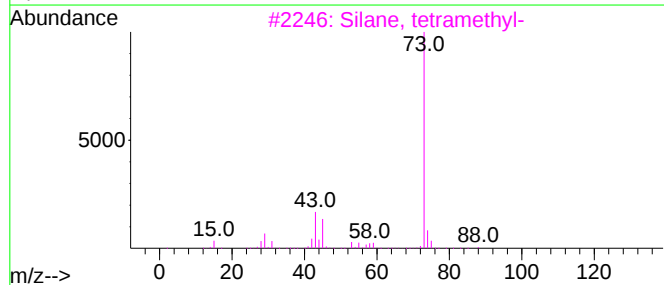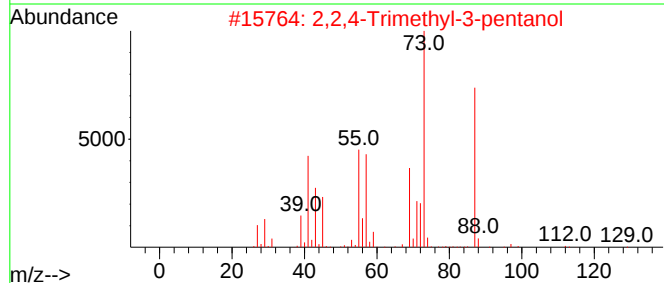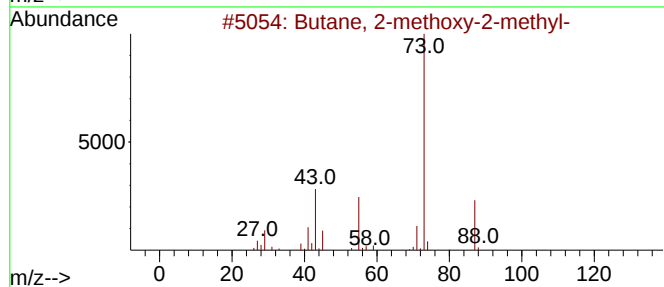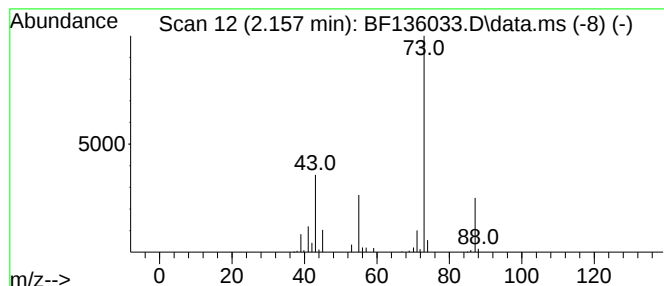

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103023\
Data File : BF136033.D
Acq On : 30 Oct 2023 17:56
Operator : CG\JU
Sample : PB156392BL
Misc :
ALS Vial : 12 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB156392BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
5.069	11.68 ng	551801	1,4-Dichlorobenzene-d4			6.822
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	59
2	Acetic acid, cyano-, 1,1-dimethy...		141	C7H11NO2	001116-98-9	23
3	1-Propen-2-ol, acetate		100	C5H8O2	000108-22-5	16
4	Acetone		58	C3H6O	000067-64-1	9
5	2,3-Butanedione, monooxime		101	C4H7NO2	000057-71-6	9

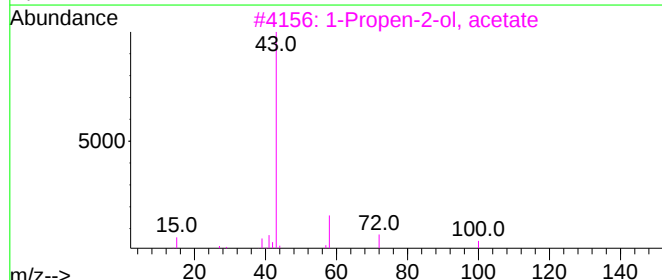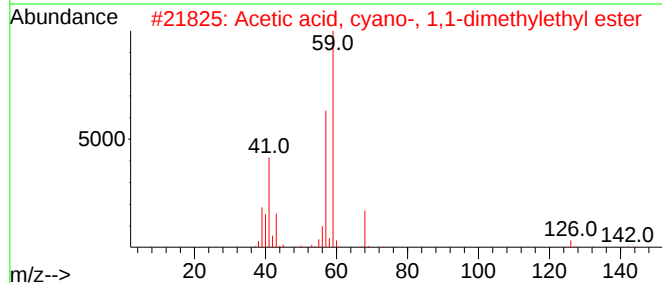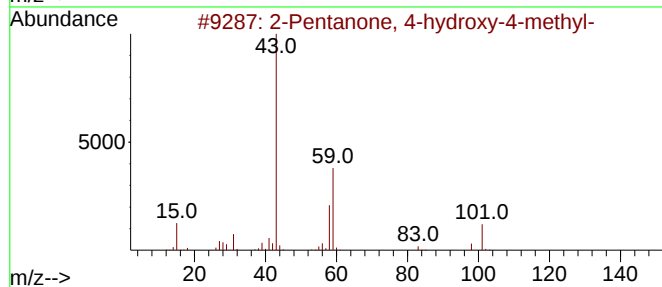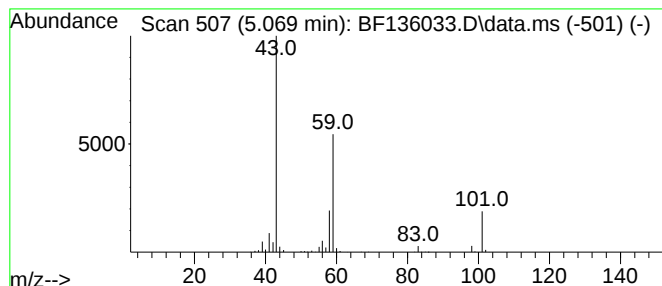

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103023\
Data File : BF136033.D
Acq On : 30 Oct 2023 17:56
Operator : CG\JU
Sample : PB156392BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156392BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.157	2.6	ng	123503	1	6.822	944498	20.0
2-Pentanone, 4-...	5.069	11.7	ng	551801	1	6.822	944498	20.0