
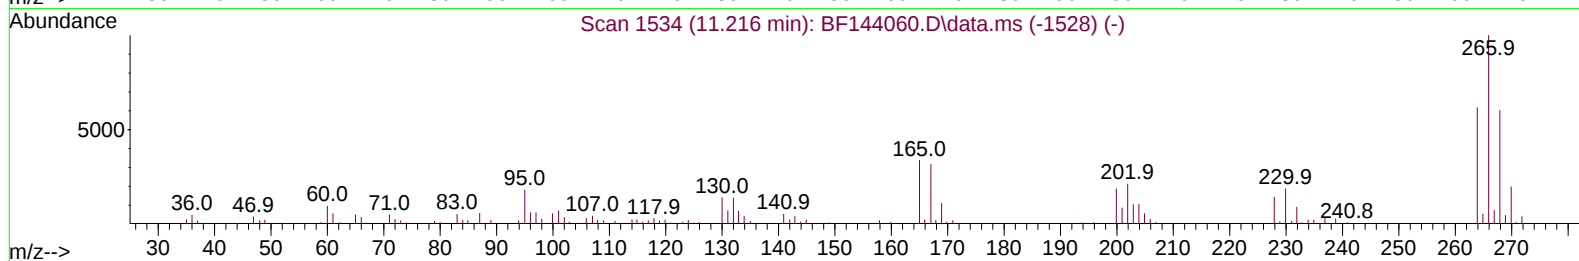
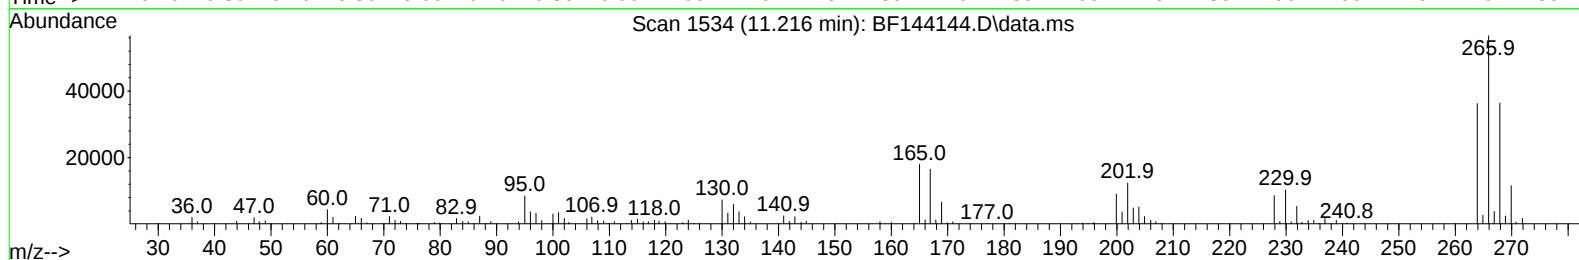


Quant Time: Oct 30 17:47:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 17:30:25 2025
Response via : Initial Calibration

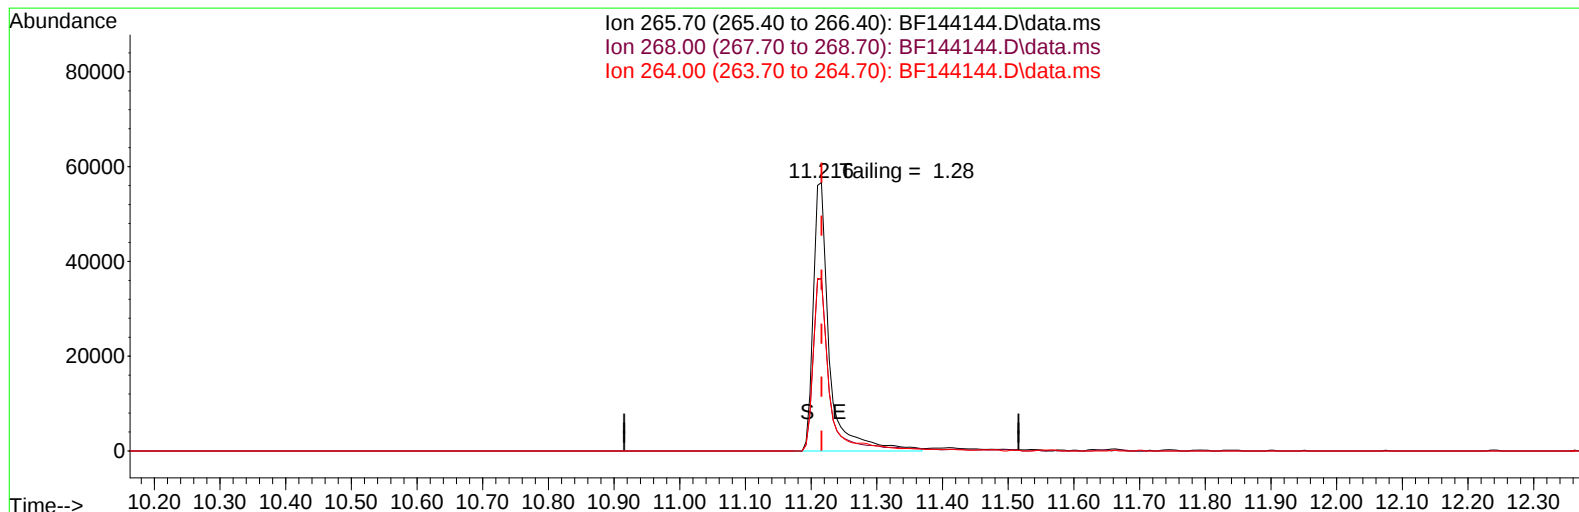

TIC: BF144144.D\data.ms

(70) Pentachlorophenol (C)




11.216min (+ 0.000) 41450.58 ng

response **96951**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.30	64.22
264.00	61.70	64.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103025\
Data File : BF144144.D
Acq On : 30 Oct 2025 16:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 17:47:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 17:30:25 2025
Response via : Initial Calibration

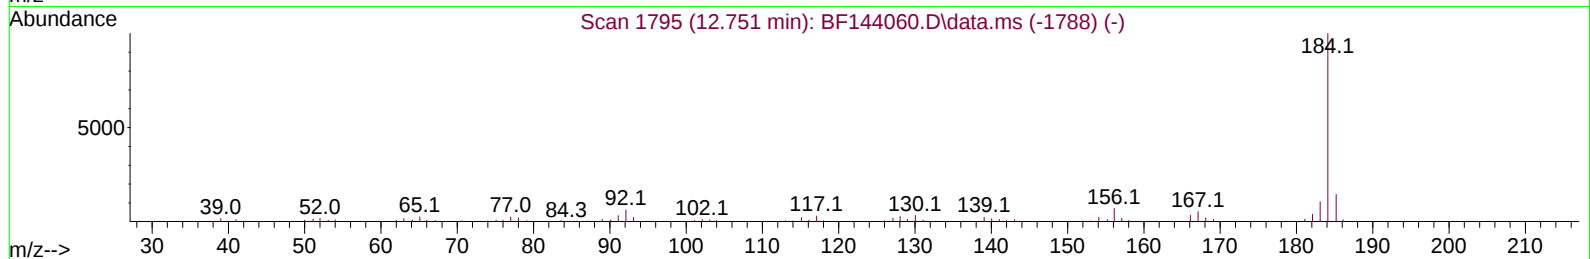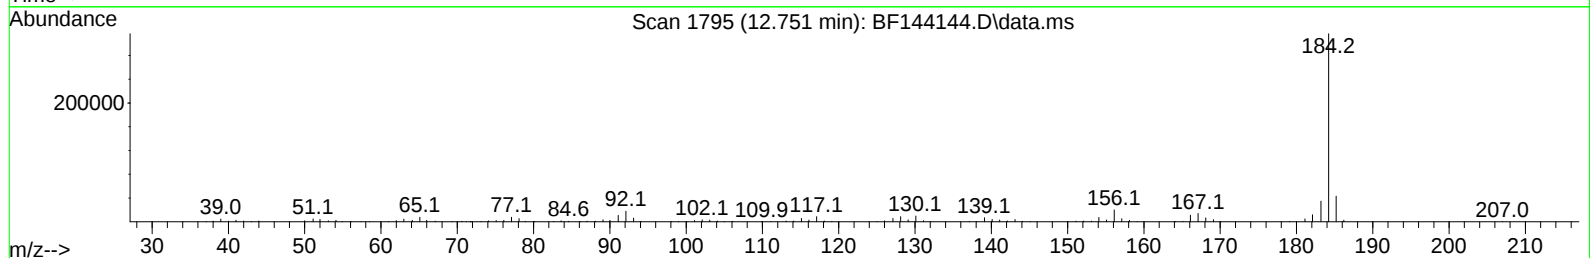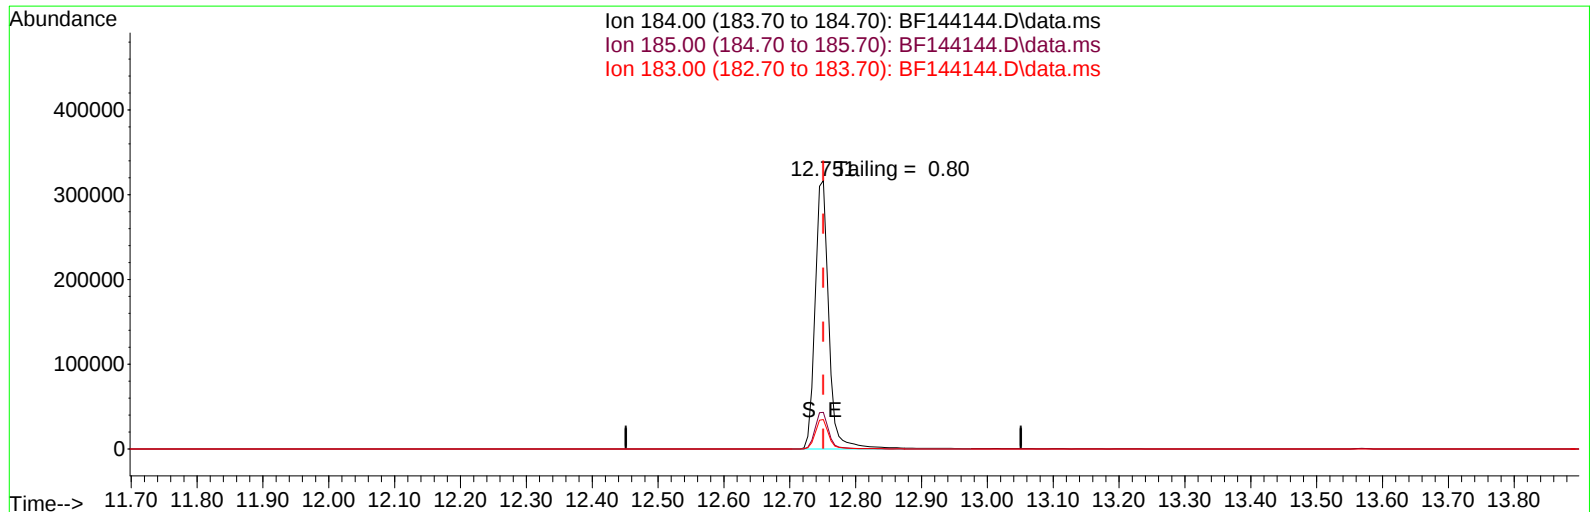

TIC: BF144144.D\data.ms

(77) Benzidine

12.751min (+ 0.000) 0.00 ng

response 461703

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.63
183.00	10.60	10.95
0.00	0.00	0.00