


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103025\
Data File : BF144144.D
Acq On : 30 Oct 2025 16:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 24 17:30:25 2025

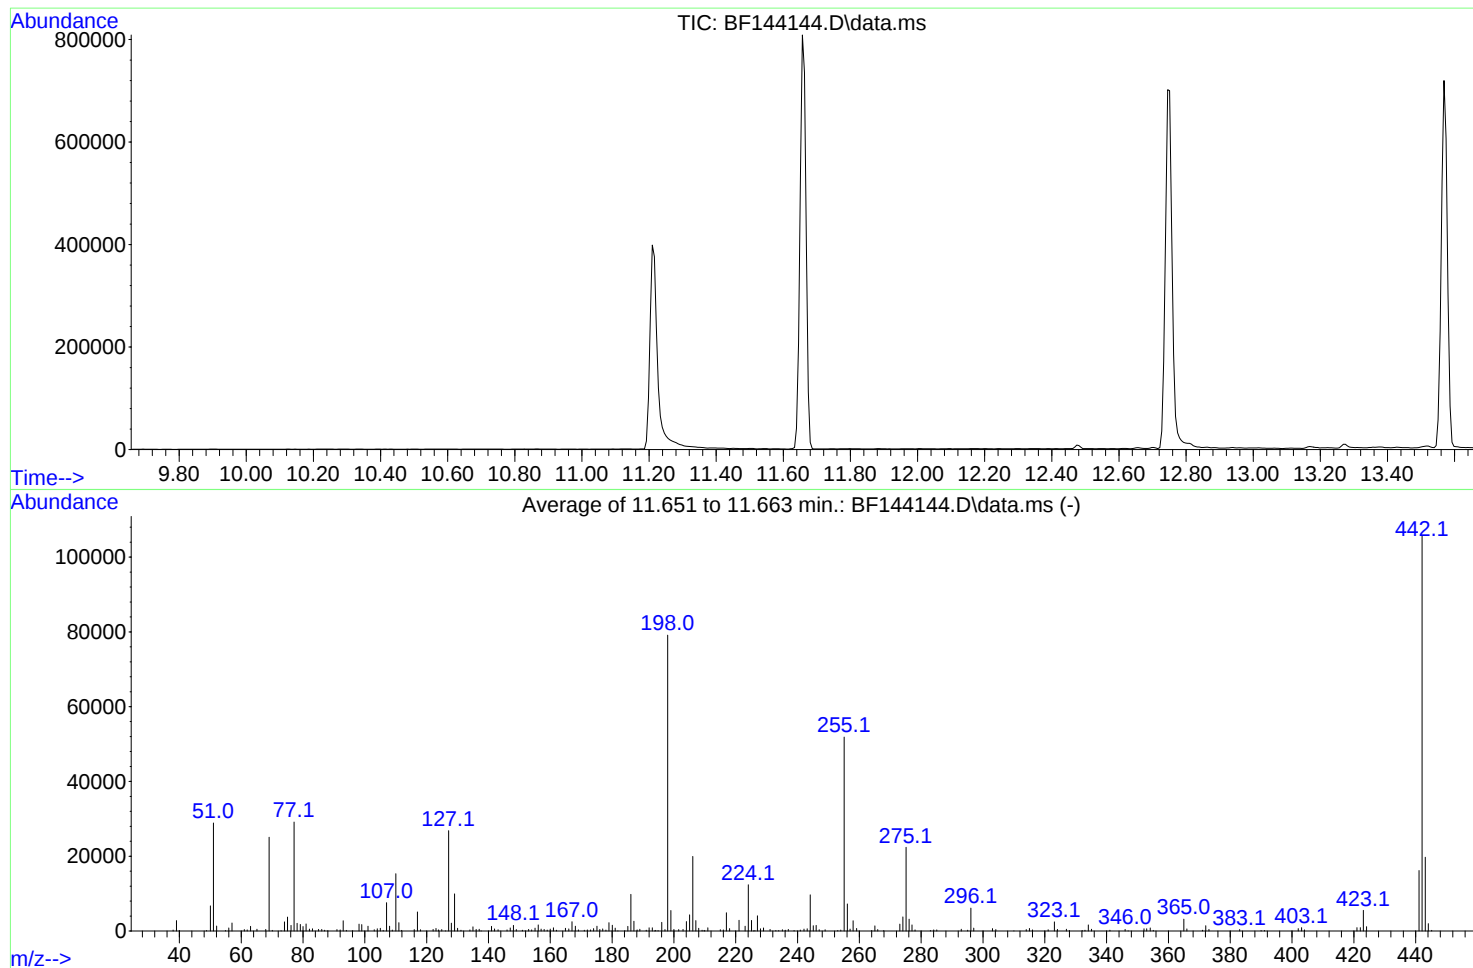

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	424	PASS
69	69	100	100	100.0	25101	PASS
70	69	0.00	2	0.7	168	PASS
197	198	0.00	2	0.5	401	PASS
198	198	100	100	100.0	79112	PASS
199	198	5	9	6.9	5472	PASS
365	198	1	100	4.0	3157	PASS
441	443	0.01	150	81.9	16185	PASS
442	442	100	100	100.0	105603	PASS
443	442	15	24	18.7	19750	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/30/2025	BNA_F	<u>BF144144.D</u>
Compound Name	Response	Retention Time
DDT	195826	13.569
DDD	4248	13.269
DDE	126	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4374	200200	2.18

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103025\
Data File : BF144144.D
Acq On : 30 Oct 2025 16:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 30 17:47:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 17:30:25 2025
Response via : Initial Calibration

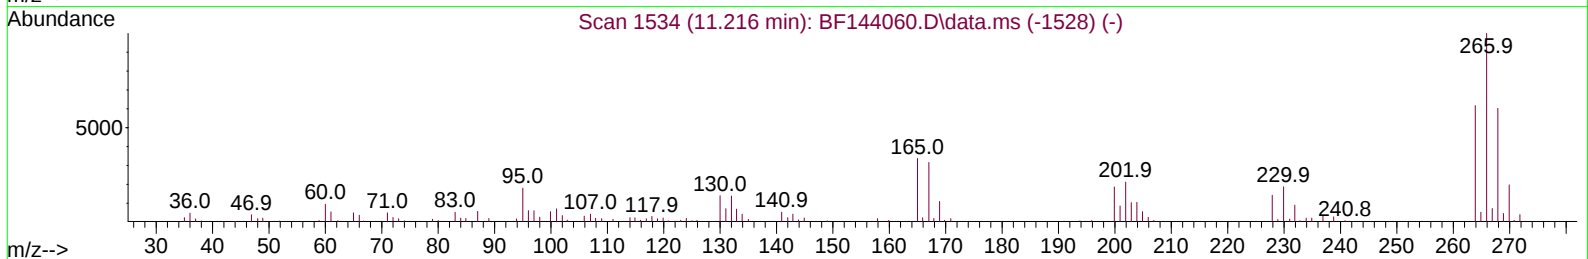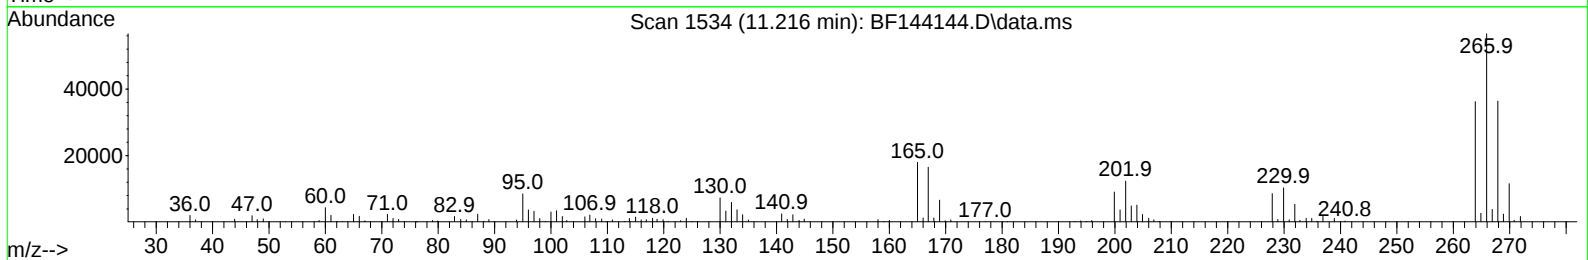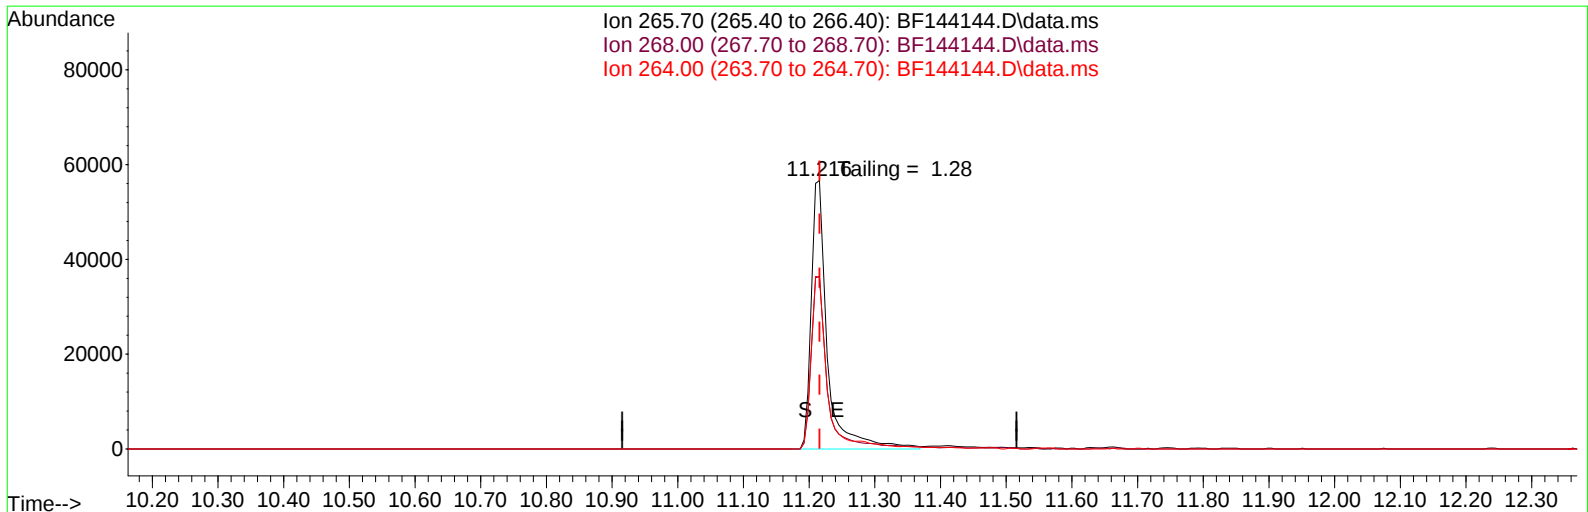

TIC: BF144144.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.000) 41450.58 ng




response 96951

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.30	64.22
264.00	61.70	64.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103025\
Data File : BF144144.D
Acq On : 30 Oct 2025 16:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 30 17:47:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 24 17:30:25 2025
Response via : Initial Calibration

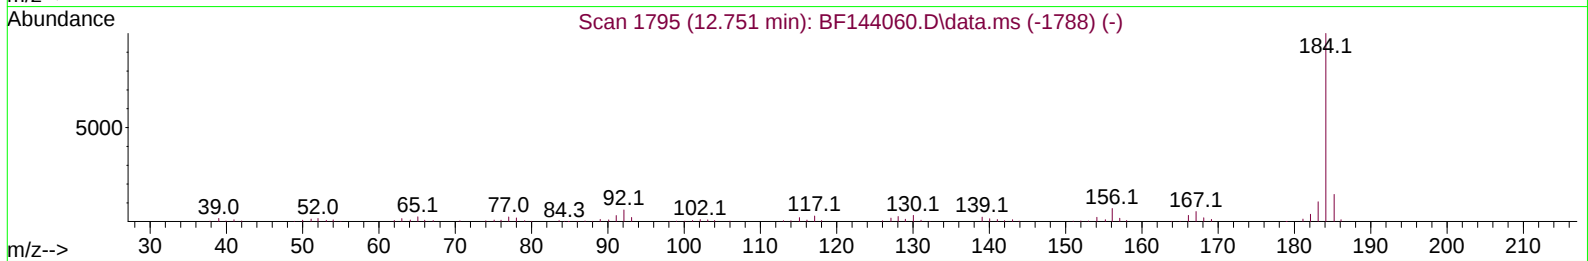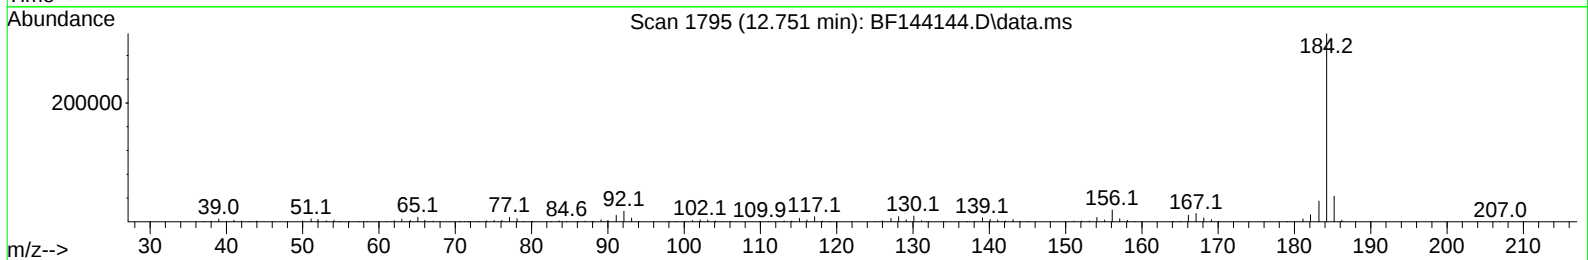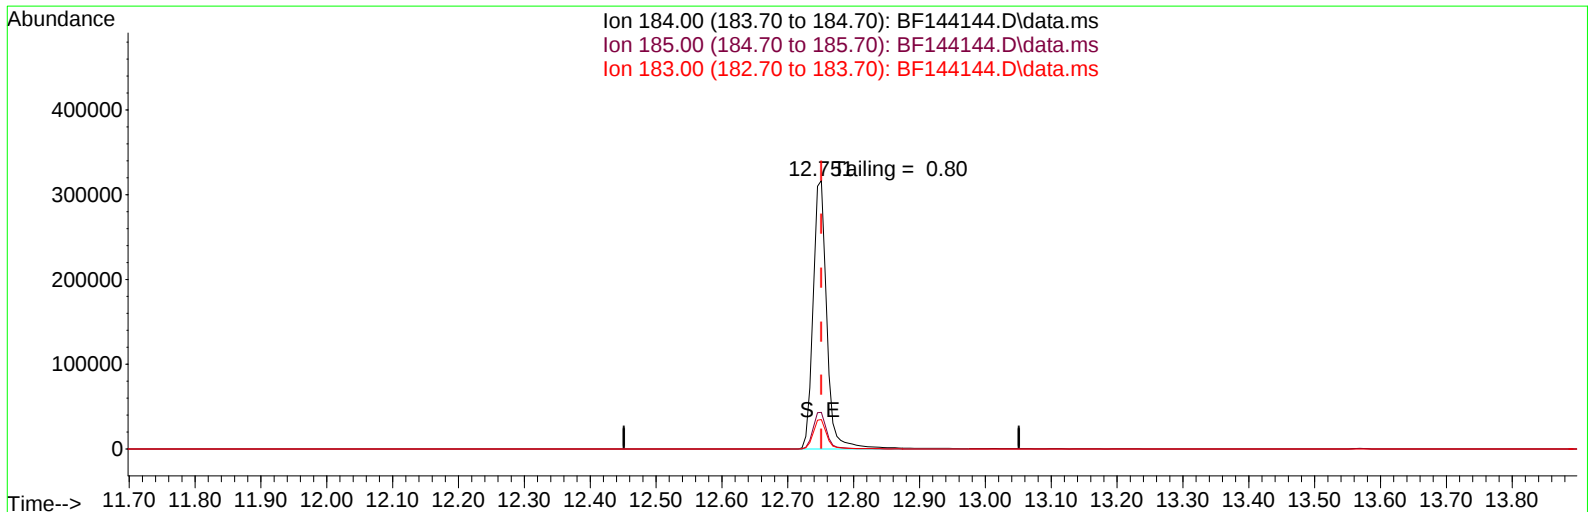

TIC: BF144144.D\data.ms

(77) Benzidine

12.751min (+ 0.000) 0.00 ng

response 461703

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.63
183.00	10.60	10.95
0.00	0.00	0.00