
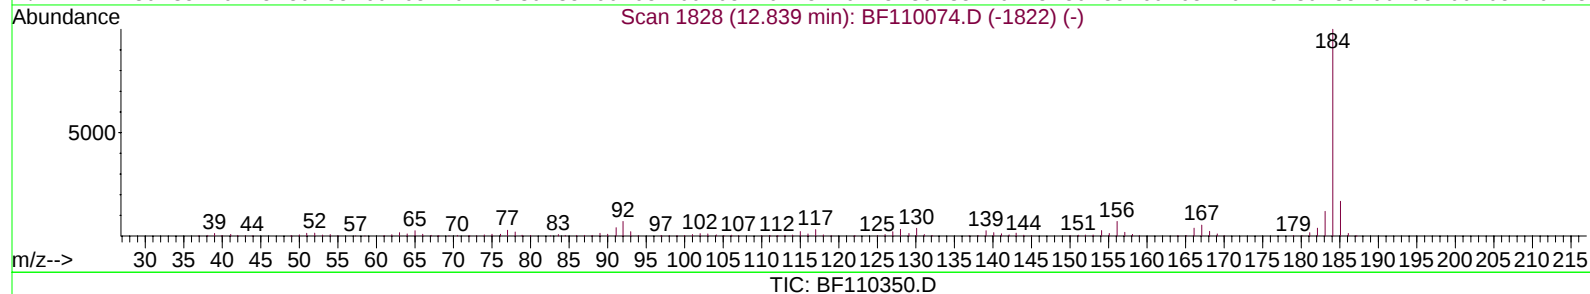
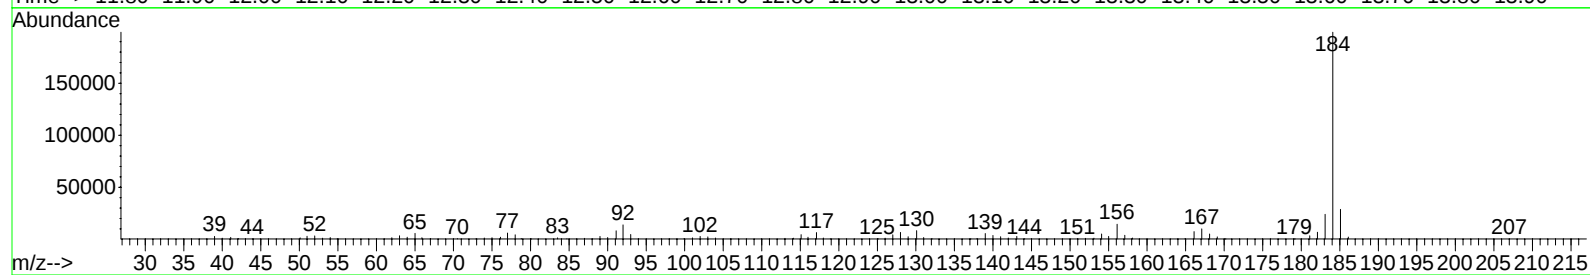


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF103118\  
Data File : BF110350.D  
Acq On : 1 Nov 2018 00:07  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 11:08:04 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 31 14:18:16 2018  
Response via : Initial Calibration

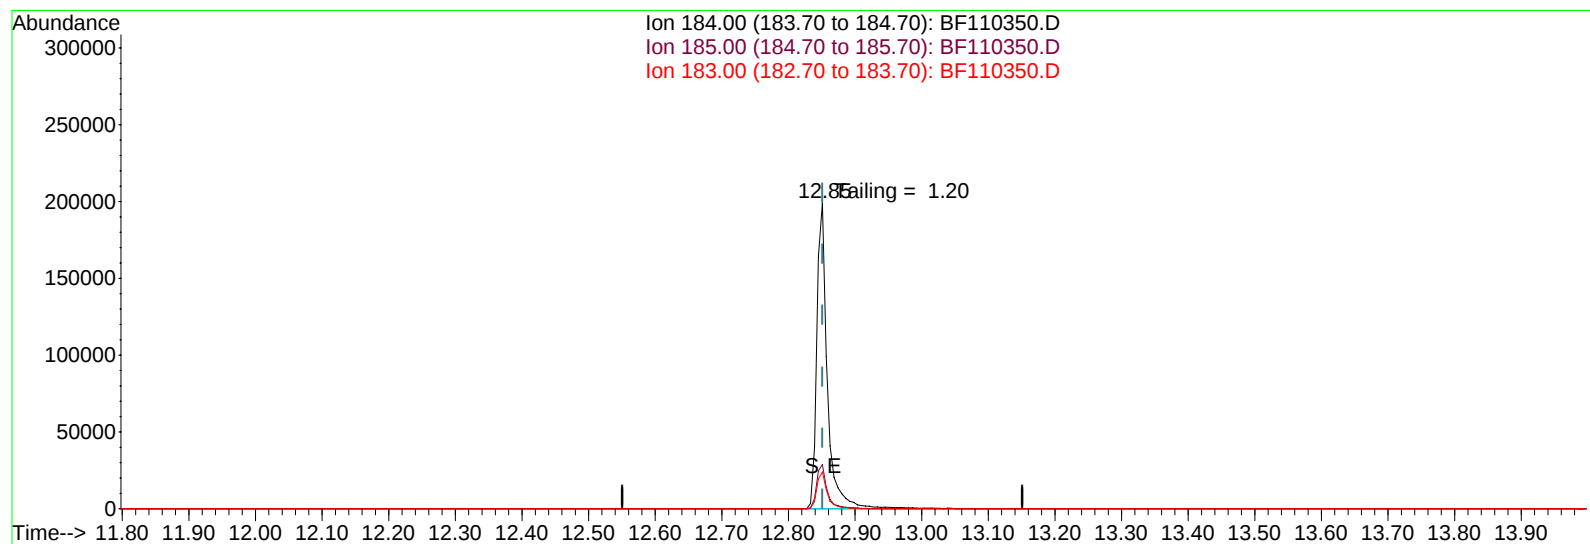

(77) Benzidine




12.851min (+0.000) 0.00ng

response 220174

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.80 | 14.49 |
| 183.00 | 11.80 | 12.03 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF103118\  
Data File : BF110350.D  
Acq On : 1 Nov 2018 00:07  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 11:08:04 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 31 14:18:16 2018  
Response via : Initial Calibration

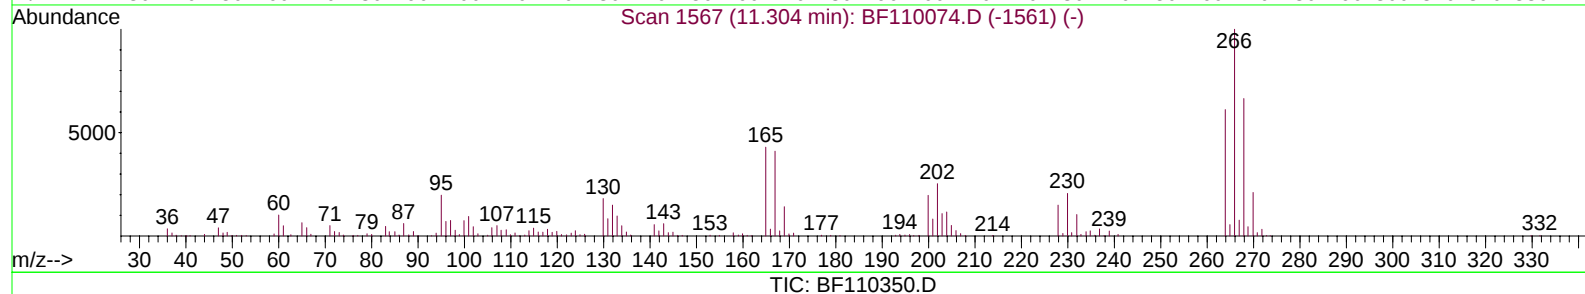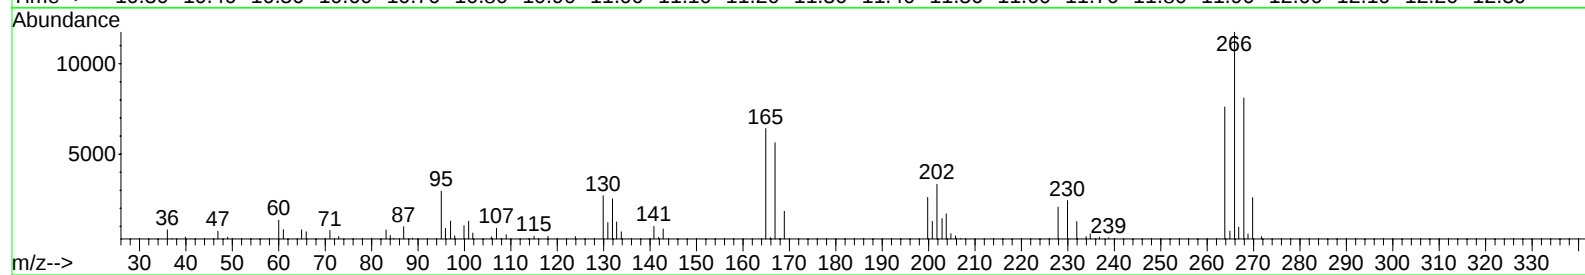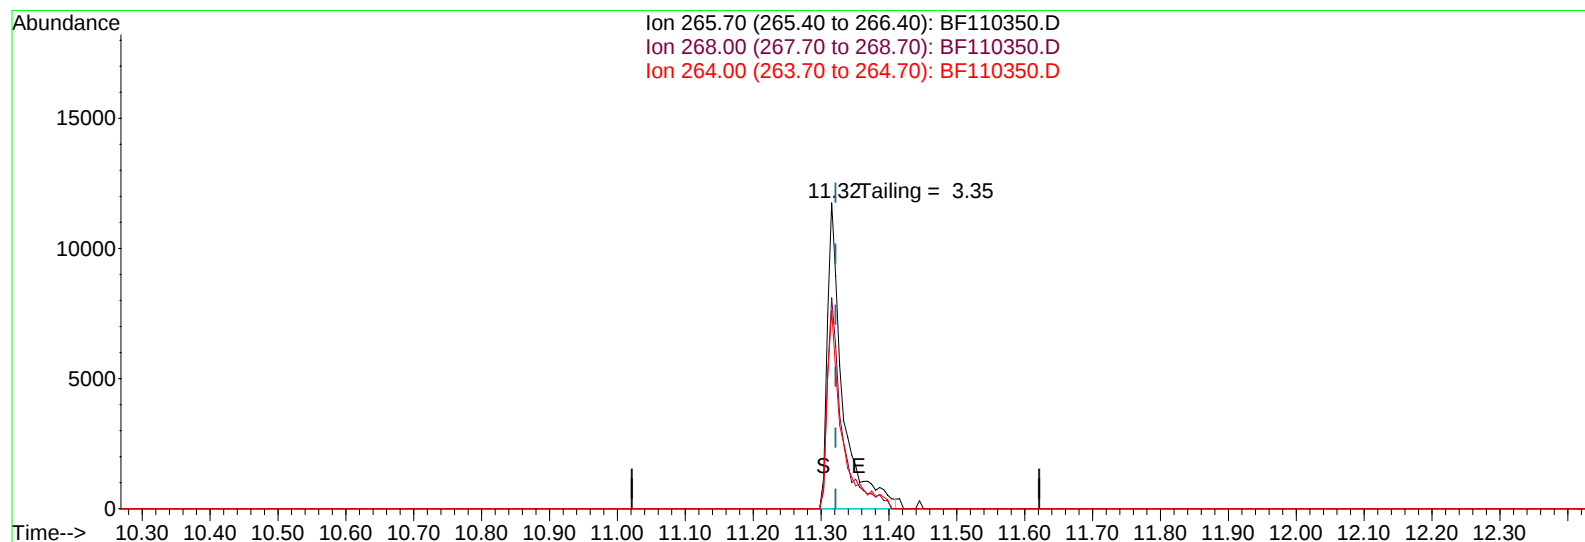

(70) Pentachlorophenol (C)

11.316min (-0.006) 0.00ng

response 18576

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.20 | 68.99 |
| 264.00 | 63.20 | 64.80 |
| 0.00   | 0.00  | 0.00  |