

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF103118\
 Data File : BF110327.D
 Acq On : 31 Oct 2018 12:45
 Operator : JU/SJ
 Sample : J5377-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RBR-200036

Manual Integrations
 APPROVED

Sohil
 11/1/2018 10:45:54 AM

Quant Time: Oct 31 14:29:22 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 29 17:29:00 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	84115	20.00	ng	0.00
21) Naphthalene-d8	8.26	136	338475	20.00	ng	0.00
39) Acenaphthene-d10	10.02	164	161082	20.00	ng	0.00
64) Phenanthrene-d10	11.51	188	294027	20.00	ng	0.00
76) Chrysene-d12	14.16	240	185085	20.00	ng	0.00
87) Perylene-d12	15.70	264	177554	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	613933	118.86	ng	0.01
7) Phenol-d6	6.60	99	778861	117.89	ng	0.00
23) Nitrobenzene-d5	7.53	82	490218	85.90	ng	0.00
42) 2,4,6-Tribromophenol	10.81	330	185783	116.43	ng	0.00
45) 2-Fluorobiphenyl	9.33	172	874787	85.28	ng	0.00
79) Terphenyl-d14	13.10	244	768099	86.31	ng	0.00
Target Compounds						
10) Phenol	6.61	94	52377	7.416	ng	Qvalue # 65
31) Naphthalene	8.27	128	263296	16.878	ng	99
37) 2-Methylnaphthalene	8.97	142	247372	23.967	ng	99
38) 1-Methylnaphthalene	9.07	142	131189	13.153	ng	99
46) 1,1'-Biphenyl	9.43	154	94905	6.515	ng	97
50) Dimethylphthalate	9.72	163	127451	10.719	ng	98
52) Acenaphthene	10.05	154	305324	29.906	ng	98
55) Dibenzofuran	10.22	168	305964	21.405	ng	96
58) Fluorene	10.57	166	268425	25.231	ng	99
71) Phenanthrene	11.54	178	974699	63.354	ng	100
72) Anthracene	11.59	178	83888	5.440	ng	98
73) Carbazole	11.74	167	59811	3.972	ng	98
75) Fluoranthene	12.73	202	555685	35.589	ng	99
78) Pyrene	12.96	202	397366	29.947	ng	98
81) Benzo(a)anthracene	14.15	228	81414	7.418	ng	98
83) Chrysene	14.19	228	52039	4.992	ng	98
84) Bis(2-ethylhexyl)phthalate	14.11	149	18959	2.435	ng	97
88) Benzo(b)fluoranthene	15.24	252	43001m	4.194	ng	
90) Benzo(a)pyrene	15.63	252	24962	2.646	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF103118\
Data File : BF110327.D
Acq On : 31 Oct 2018 12:45
Operator : JU/SJ
Sample : J5377-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RBR-200036

Manual Integrations
APPROVED

Sohil
11/1/2018 10:45:54 AM

Quant Time: Oct 31 14:29:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 29 17:29:00 2018
Response via : Initial Calibration

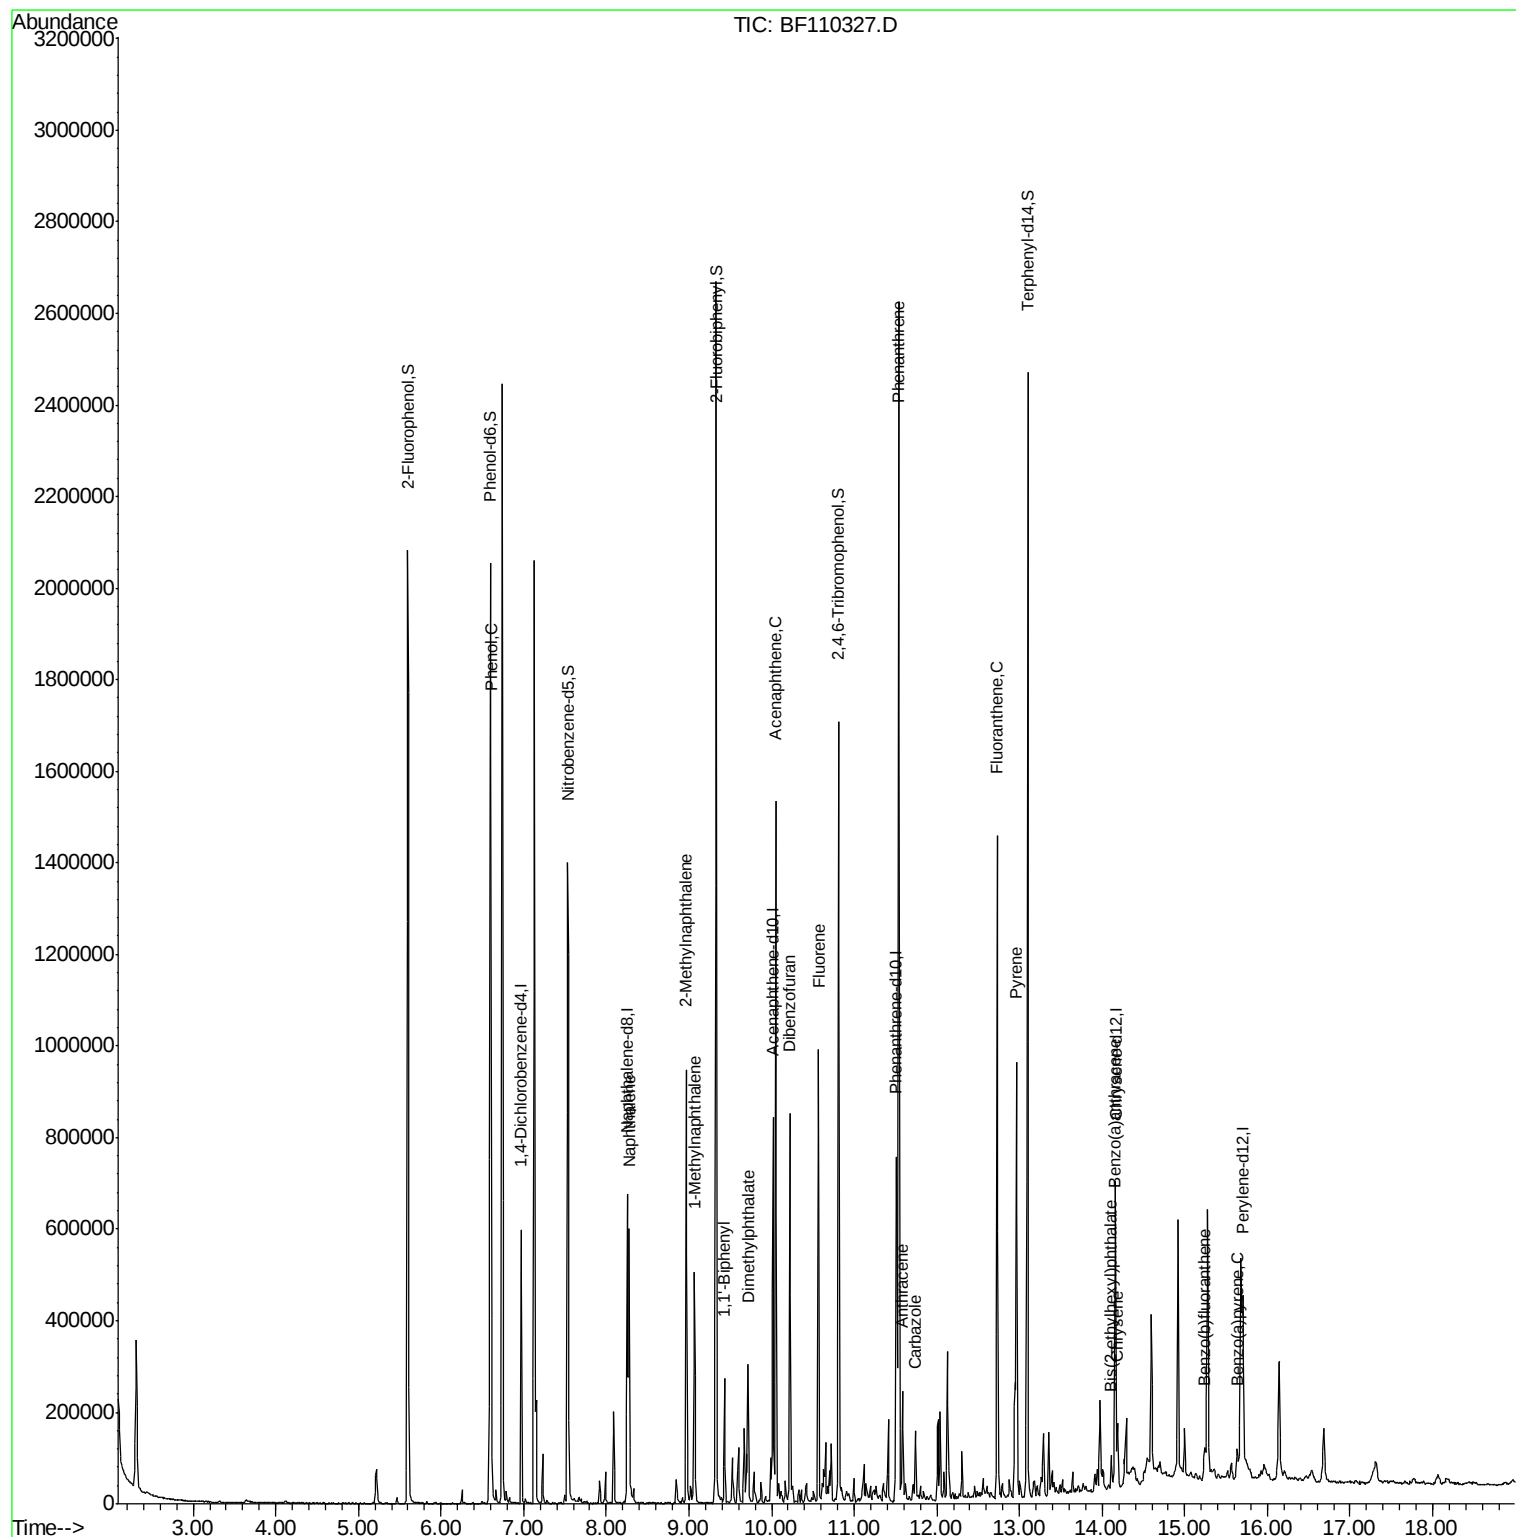



#1


1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 830
Delta R.T. -0.00 min
Lab File: BF110327.D
Acq: 31 Oct 2018 12:45

Instrument :
BNA_F
ClientSampleId :
RBR-200036

Tot Ion	Ratio	Lower	Upper
152	100		
150	157.8	122.7	184.1
115	64.3	49.1	73.7

Manual Integrations
APPROVED

Sohil
11/1/2018 10:45:54 AM





Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E


Time-->

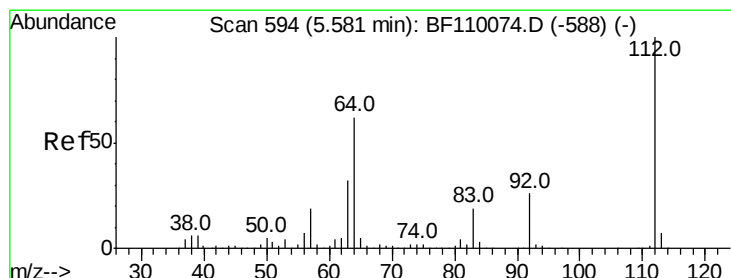

#5

2-Fluorophenol
Concen: 118.856 ng
RT: 5.60 min Scan# 597
Delta R.T. 0.01 min
Lab File: BF110327.D
Acq: 31 Oct 2018 12:45

Tgt Ion	Ratio	Lower	Upper
112	100		
64	60.9	44.1	66.1
63	33.1	23.7	35.5




Abundance


Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

Time-->



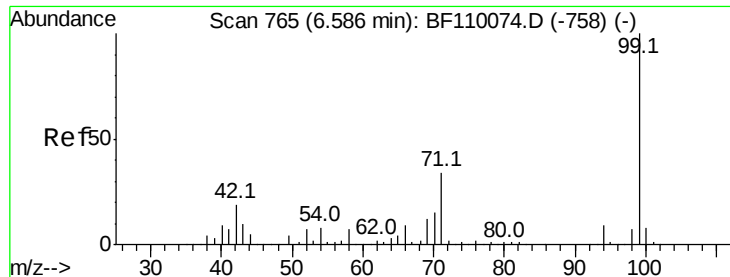

#7

Phenol-d6

Concen: 117.887 ng

RT: 6.60 min Scan# 767

Delta R.T. 0.01 min

Lab File: BF110327.D

Acq: 31 Oct 2018 12:45

Instrument :

BNA_F


ClientSampleId :

RBR-200036




Tot Ion:	99	Resp:	778861
Ion	Ratio	Lower	Upper
99	100		
42	20.4	15.8	23.6
71	36.6	28.0	42.0

Manual Integrations
APPROVED

Sohil
11/1/2018 10:45:54 AM

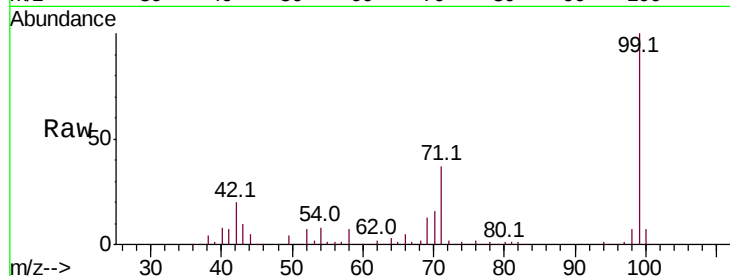

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

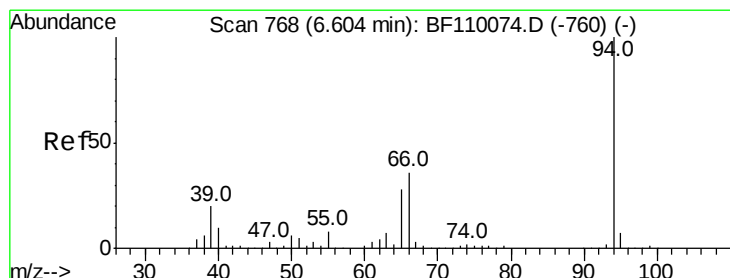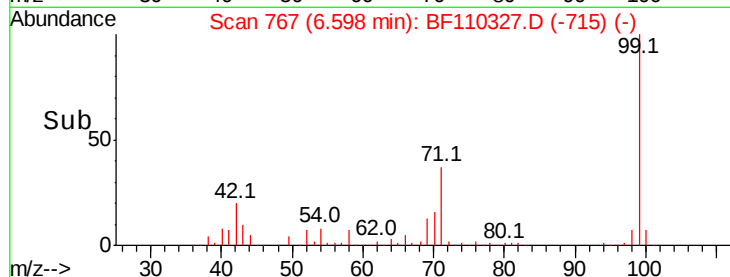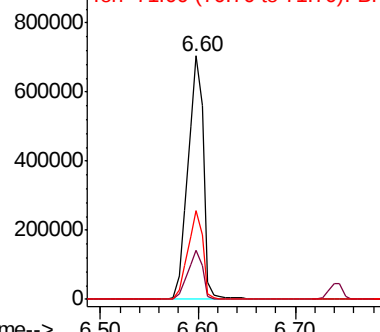

#10

Phenol

Concen: 7.416 ng


RT: 6.61 min Scan# 769

Delta R.T. 0.01 min



Lab File: BF110327.D

Acq: 31 Oct 2018 12:45

Tgt Ion:	94	Resp:	52377
Ion	Ratio	Lower	Upper
94	100		
65	29.4	25.3	65.3
66	39.9	54.5	94.5#

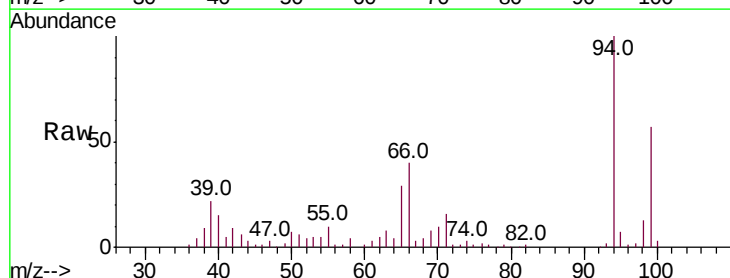

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

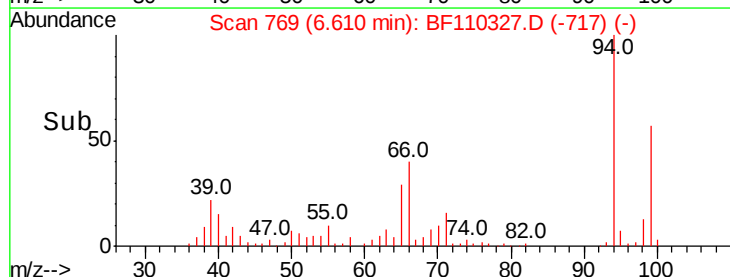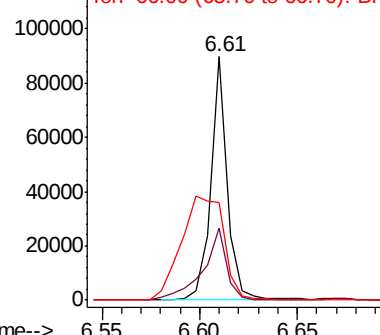




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.26 min Scan# 1049
Delta R.T. 0.01 min
Lab File: BF110327.D
Acq: 31 Oct 2018 12:45

Instrument :
BNA_F
ClientSampleId :
RBR-200036

Tot Ion	Ratio	Resp	Lower	Upper
136	100			
137	10.8	8.8	13.2	
54	6.9	5.4	8.2	
68	4.7	4.2	6.2	

Manual Integrations
APPROVED

Sohil
11/1/2018 10:45:54 AM






Abundance

Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E


Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

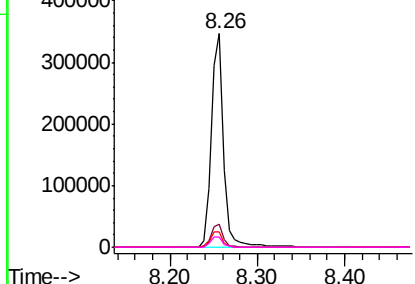

#23
Nitrobenzene-d5
Concen: 85.904 ng
RT: 7.53 min Scan# 926
Delta R.T. -0.00 min
Lab File: BF110327.D
Acq: 31 Oct 2018 12:45

Tgt Ion	Ratio	Resp	Lower	Upper
82	100			
128	44.0	34.2	51.2	
54	54.0	38.6	58.0	






Abundance

Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

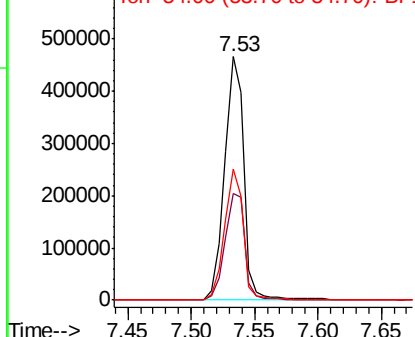




#31
Naphthalene
Concen: 16.878 ng
RT: 8.27 min Scan# 1052
Delta R.T. -0.00 min
Lab File: BF110327.D
Acq: 31 Oct 2018 12:45

Instrument :
BNA_F
ClientSampleId :
RBR-200036

Tot Ion	Ratio	Resp	Lower	Upper
128	100	263296		
129	11.1		8.8	13.2
127	12.9		10.8	16.2

Manual Integrations
APPROVED

Sohil
11/1/2018 10:45:54 AM






Abundance

Ion 128.00 (127.70 to 128.70): E


Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

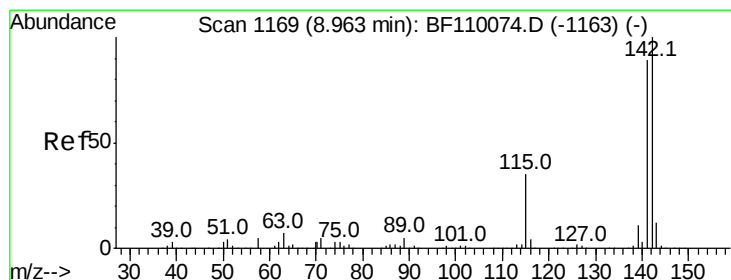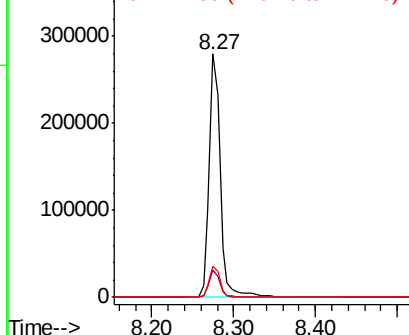

#37
2-Methylnaphthalene
Concen: 23.967 ng
RT: 8.97 min Scan# 1170
Delta R.T. -0.00 min
Lab File: BF110327.D
Acq: 31 Oct 2018 12:45

Tgt Ion	Ratio	Resp	Lower	Upper
142	100	247372		
141	88.0		71.4	107.2
115	35.1		28.7	43.1






Abundance

Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

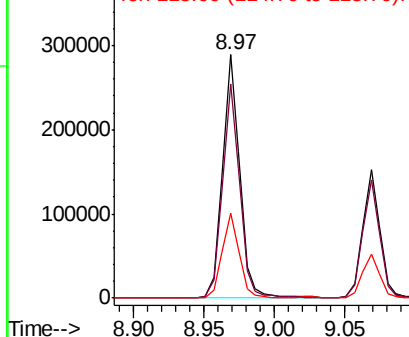







#38
1-Methylnaphthalene
Concen: 13.153 ng
RT: 9.07 min Scan# 1187
Delta R.T. -0.00 min
Lab File: BF110327.D
Acq: 31 Oct 2018 12:45

Instrument :
BNA_F
ClientSampleId :
RBR-200036

Tot Ion	Ratio	Resp	Lower	Upper
142	100	131189		
141	91.6	74.2	111.4	
116	3.7	2.6	4.0	




Manual Integrations
APPROVED


Sohil
11/1/2018 10:45:54 AM

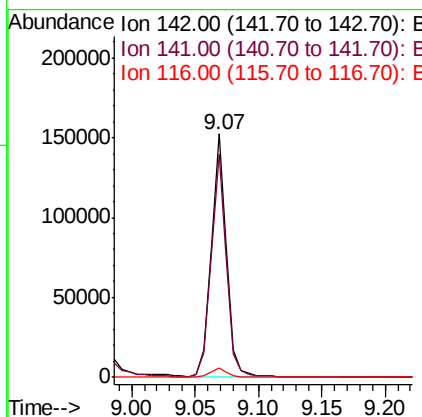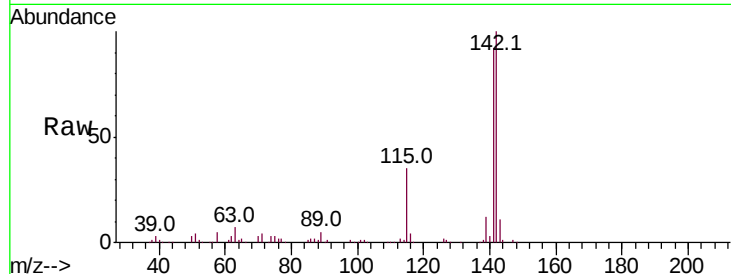

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.02 min Scan# 1348
Delta R.T. -0.00 min
Lab File: BF110327.D
Acq: 31 Oct 2018 12:45

Tgt Ion	Ratio	Resp	Lower	Upper
164	100	161082		
162	106.8	83.0	124.6	
160	45.4	37.0	55.6	

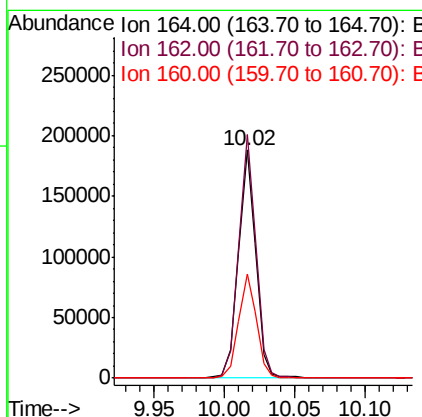




#42
 2,4,6-Tribromophenol
 Concen: 116.433 ng
 RT: 10.81 min Scan# 1483
 Delta R.T. -0.00 min
 Lab File: BF110327.D
 Acq: 31 Oct 2018 12:45

Instrument :
 BNA_F
 ClientSampled :
 RBR-200036

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.5	77.1	115.7
141	38.1	27.0	40.4

Manual Integrations
 APPROVED

Sohil
 11/1/2018 10:45:54 AM






Abundance

Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

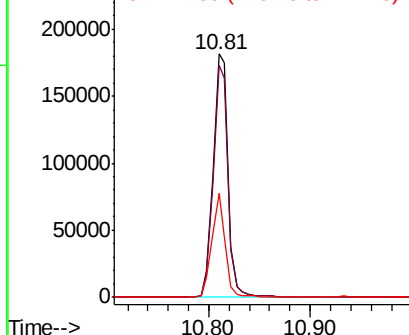

#45
 2-Fluorobiphenyl
 Concen: 85.276 ng
 RT: 9.33 min Scan# 1231
 Delta R.T. -0.00 min
 Lab File: BF110327.D
 Acq: 31 Oct 2018 12:45




Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.8	28.6	43.0
170	23.6	19.7	29.5


Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

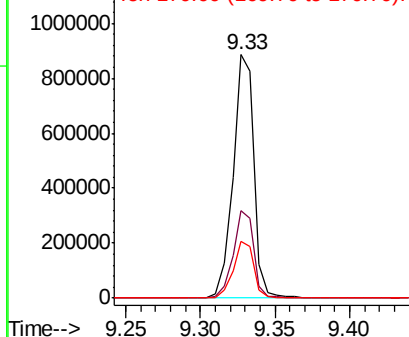




#46
1,1'-Biphenyl
Concen: 6.515 ng
RT: 9.43 min Scan# 1249
Delta R.T. -0.00 min
Lab File: BF110327.D
Acq: 31 Oct 2018 12:45

Instrument :
BNA_F
ClientSampled :
RBR-200036




Tot Ion	Ratio	Resp	Lower	Upper
154	100			
153	39.1	20.4	60.4	
76	9.5	0.0	31.9	

Manual Integrations
APPROVED

Sohil
11/1/2018 10:45:54 AM




Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 76.00 (75.70 to 76.70): BF1

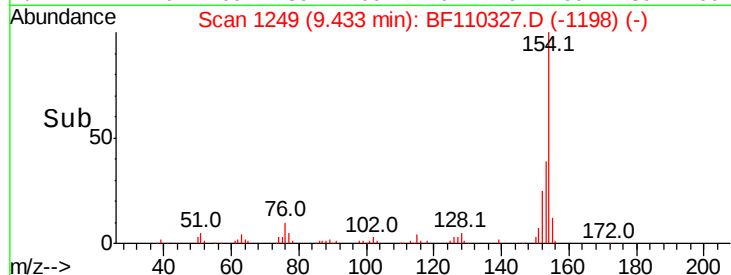
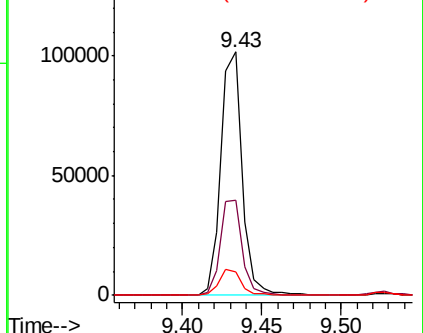



#50
Dimethylphthalate
Concen: 10.719 ng
RT: 9.72 min Scan# 1298
Delta R.T. -0.01 min
Lab File: BF110327.D
Acq: 31 Oct 2018 12:45

Tgt Ion	Ratio	Resp	Lower	Upper
163	100			
194	4.3	3.2	4.8	
164	9.2	8.1	12.1	



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

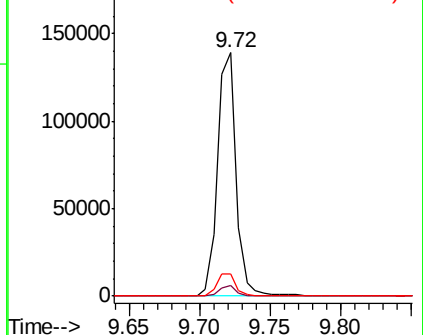



#52

Acenaphthene

Concen: 29.906 ng

RT: 10.05 min Scan# 1354

Delta R.T. -0.00 min

Lab File: BF110327.D

Acq: 31 Oct 2018 12:45

Instrument :

BNA_F


ClientSampleId :

RBR-200036




Tot Ion:	154	Resp:	305324
Ion Ratio	Lower	Upper	
154	100		
153	113.7	90.1	135.1
152	51.2	43.4	65.2

Manual Integrations
APPROVED

Sohil
11/1/2018 10:45:54 AM



Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E

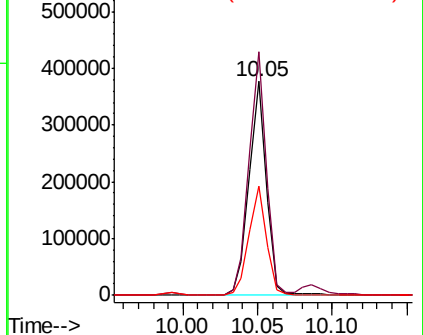

#55

Dibenzofuran

Concen: 21.405 ng

RT: 10.22 min Scan# 1383




Delta R.T. -0.00 min


Lab File: BF110327.D

Acq: 31 Oct 2018 12:45

Tgt Ion:	168	Resp:	305964
Ion Ratio	Lower	Upper	
168	100		
139	38.4	33.0	49.6
169	12.9	11.3	16.9

Abundance Ion 168.00 (167.70 to 168.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 169.00 (168.70 to 169.70): E

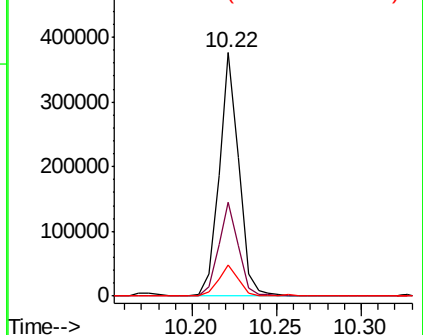



#58

Fluorene

Concen: 25.231 ng

RT: 10.57 min Scan# 1442

Delta R.T. 0.01 min

Lab File: BF110327.D

Acq: 31 Oct 2018 12:45

Instrument :

BNA_F





ClientSampleId :

RBR-200036

Tot Ion:	166	Resp:	268425
Ion Ratio	Lower	Upper	
166	100		
165	99.3	78.6	117.8
167	13.4	10.8	16.2

Manual Integrations
APPROVED

Sohil
11/1/2018 10:45:54 AM

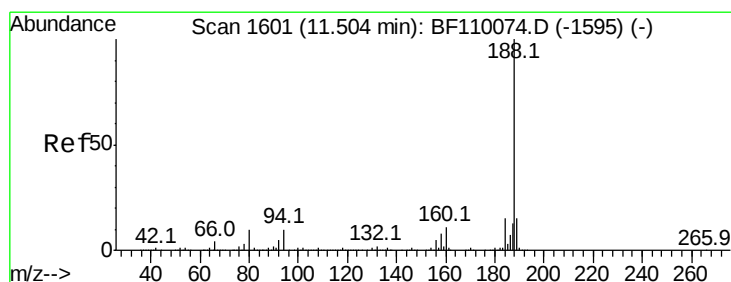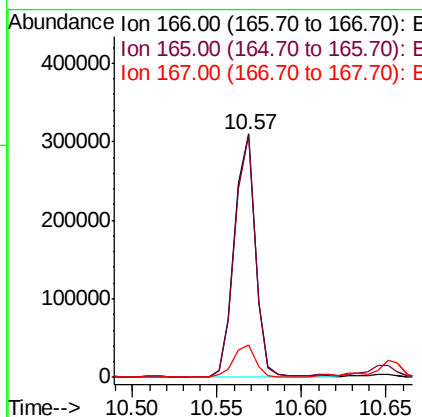

#64

Phenanthrene-d10

Concen: 20.000 ng




RT: 11.51 min Scan# 1602


Delta R.T. -0.00 min

Lab File: BF110327.D

Acq: 31 Oct 2018 12:45

Tgt Ion:	188	Resp:	294027
Ion Ratio	Lower	Upper	
188	100		
94	9.3	7.2	10.8
80	10.2	7.9	11.9

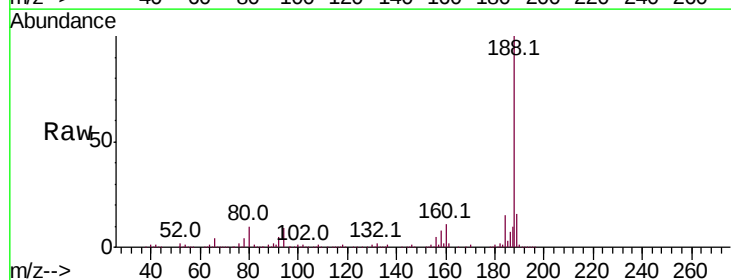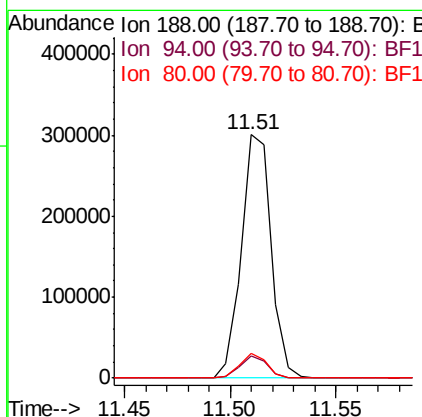



#71

Phenanthrene

Concen: 63.354 ng

RT: 11.54 min Scan# 1607

Delta R.T. 0.01 min

Lab File: BF110327.D

Acq: 31 Oct 2018 12:45

Instrument :

BNA_F

ClientSampleId :

RBR-200036

Tot Ion:178 Resp: 974699

Ion Ratio Lower Upper

178 100


176 19.6 15.5 23.3

179 15.5 12.5 18.7




Manual Integrations
APPROVED

Sohil

11/1/2018 10:45:54 AM



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

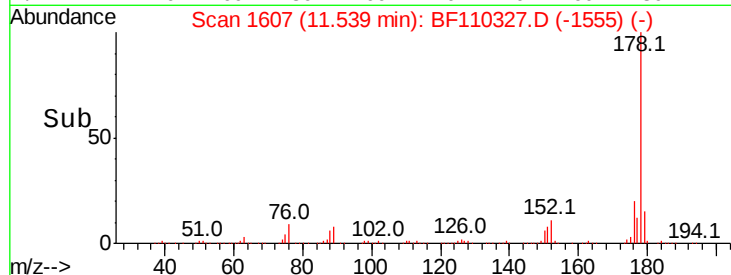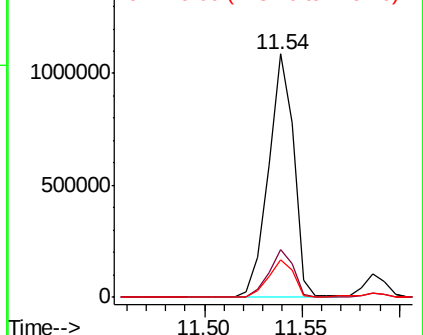

#72

Anthracene

Concen: 5.440 ng

RT: 11.59 min Scan# 1615

Delta R.T. -0.00 min

Lab File: BF110327.D

Acq: 31 Oct 2018 12:45


Tgt Ion:178 Resp: 83888

Ion Ratio Lower Upper



178 100


176 17.8 15.4 23.2

179 15.9 12.6 18.8



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

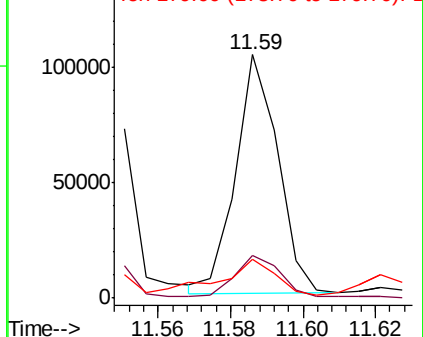







#73
 Carbazole
 Concen: 3.972 ng
 RT: 11.74 min Scan# 1641
 Delta R.T. -0.00 min
 Lab File: BF110327.D
 Acq: 31 Oct 2018 12:45

Instrument :
 BNA_F
 ClientSampleId :
 RBR-200036

Tot Ion	Ratio	Lower	Upper
167	100		
166	20.4	17.4	26.0
139	13.9	10.9	16.3




Manual Integrations
 APPROVED


Sohil
 11/1/2018 10:45:54 AM

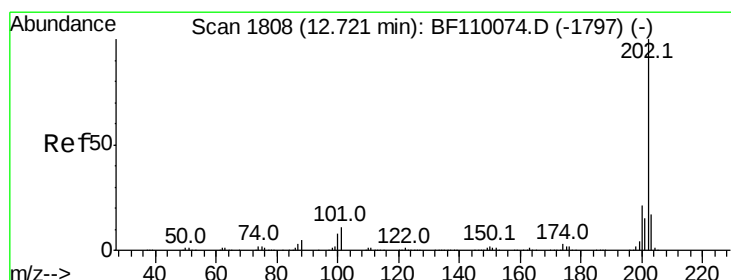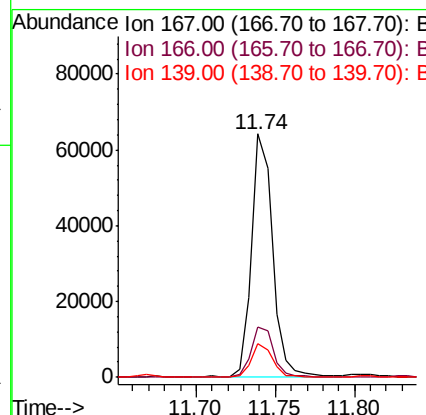

#75
 Fluoranthene
 Concen: 35.589 ng
 RT: 12.73 min Scan# 1810
 Delta R.T. 0.01 min
 Lab File: BF110327.D
 Acq: 31 Oct 2018 12:45

Tgt Ion	Ratio	Lower	Upper
202	100		
101	10.6	0.0	31.4
203	17.5	0.0	37.7

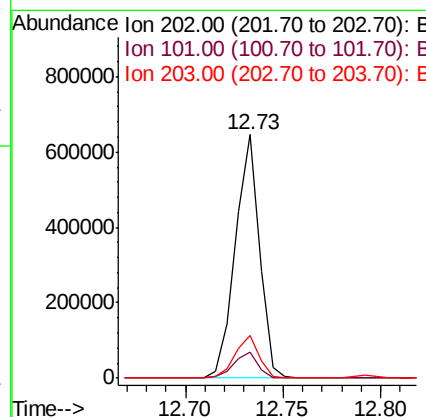







#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 14.16 min Scan# 2053
 Delta R.T. 0.01 min
 Lab File: BF110327.D
 Acq: 31 Oct 2018 12:45

Instrument :
 BNA_F
 ClientSampleId :
 RBR-200036

Tot Ion	Ratio	Resp Lower	Upper
240	100		
120	10.2	8.3	12.5
236	25.2	21.2	31.8




Manual Integrations
 APPROVED


Sohil
 11/1/2018 10:45:54 AM

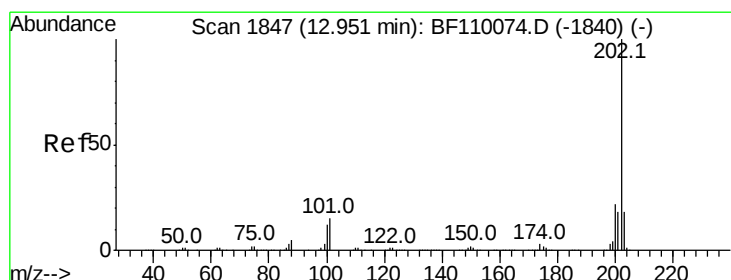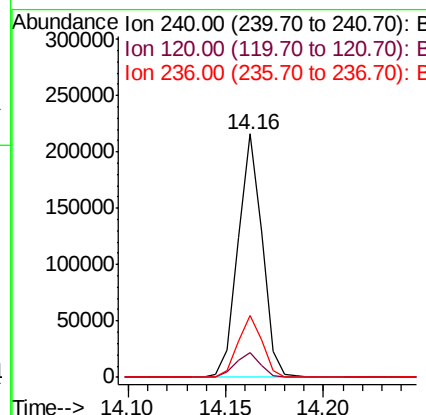

#78
 Pyrene
 Concen: 29.947 ng
 RT: 12.96 min Scan# 1849
 Delta R.T. 0.01 min
 Lab File: BF110327.D
 Acq: 31 Oct 2018 12:45

Tgt Ion	Ratio	Resp Lower	Upper
202	100		
200	20.9	17.8	26.6
203	17.3	14.2	21.4

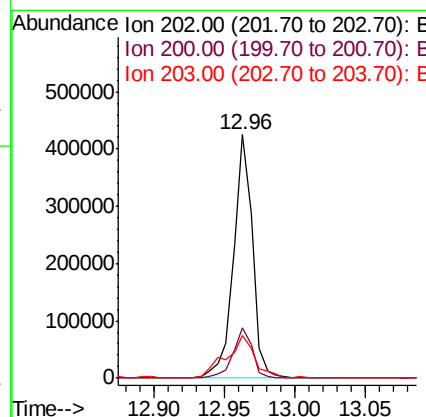

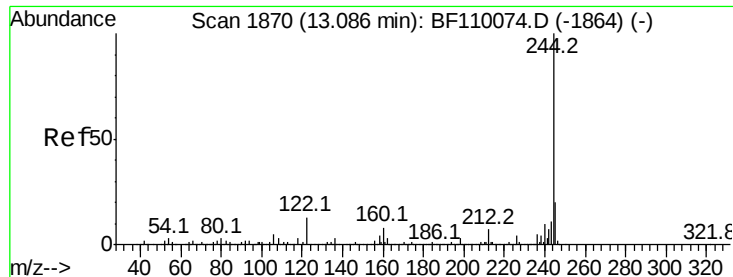

#79

Terphenyl-d14

Concen: 86.308 ng

RT: 13.10 min Scan# 1872

Delta R.T. 0.01 min

Lab File: BF110327.D

Acq: 31 Oct 2018 12:45

Instrument :

BNA_F





ClientSampled :

RBR-200036

Tot Ion:	244	Resp:	768099
Ion Ratio	Lower	Upper	
244	100		
212	6.8	5.8	8.8
122	12.4	8.7	13.1

Manual Integrations
APPROVED

Sohil
11/1/2018 10:45:54 AM

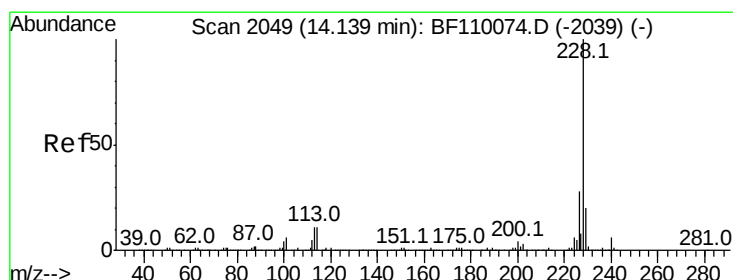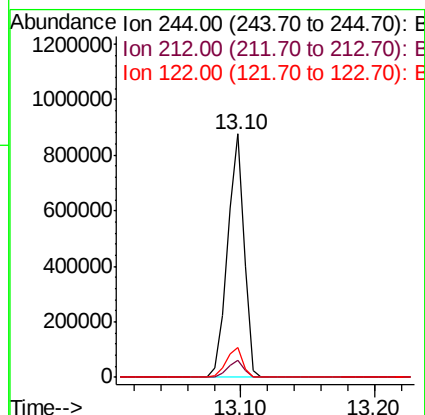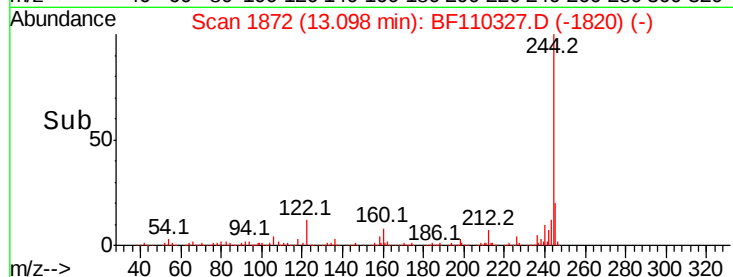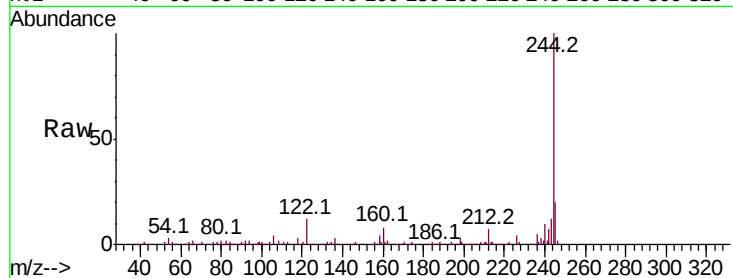

#81

Benzo(a)anthracene

Concen: 7.418 ng




RT: 14.15 min Scan# 2051


Delta R.T. 0.01 min

Lab File: BF110327.D

Acq: 31 Oct 2018 12:45

Tgt Ion:	228	Resp:	81414
Ion Ratio	Lower	Upper	
228	100		
226	28.2	22.1	33.1
229	20.8	15.6	23.4

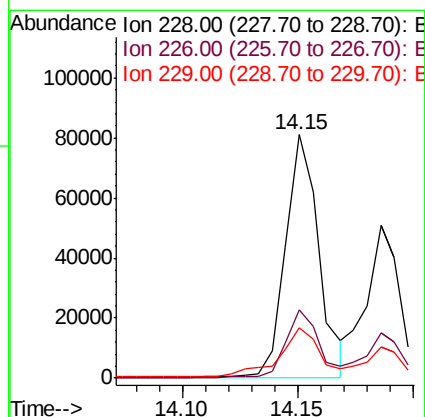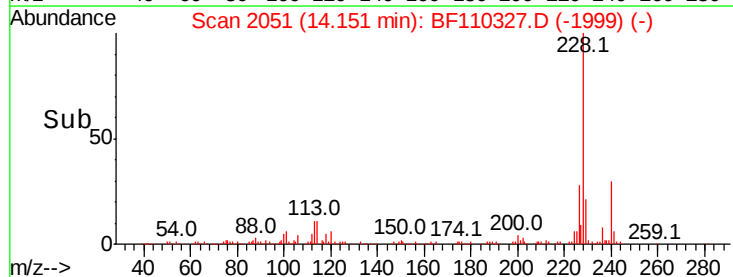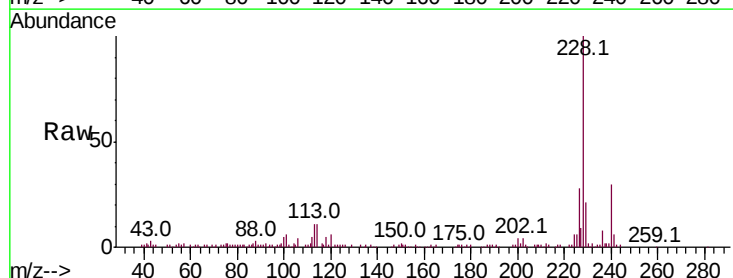

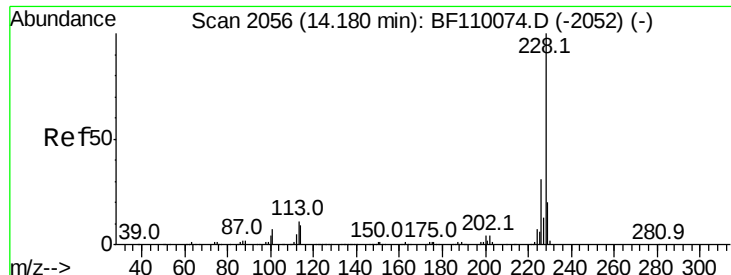





#83
 Chrysene
 Concen: 4.992 ng
 RT: 14.19 min Scan# 2057
 Delta R.T. -0.00 min
 Lab File: BF110327.D
 Acq: 31 Oct 2018 12:45

Instrument :
 BNA_F
 ClientSampleID :
 RBR-200036

Tot Ion	Ratio	Lower	Upper
228	100		
226	29.9	24.7	37.1
229	20.4	15.9	23.9




Manual Integrations
 APPROVED


Sohil
 11/1/2018 10:45:54 AM

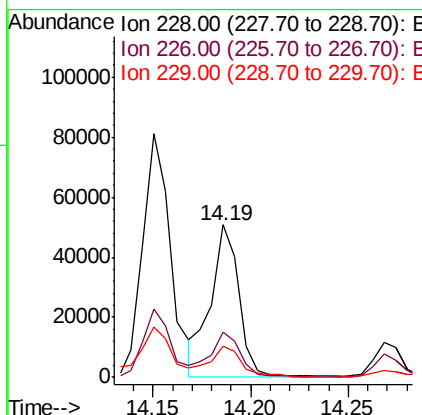

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 2.435 ng
 RT: 14.11 min Scan# 2044
 Delta R.T. -0.00 min
 Lab File: BF110327.D
 Acq: 31 Oct 2018 12:45

Tgt Ion	Ratio	Lower	Upper
149	100		
167	26.6	19.8	29.8
279	3.5	2.7	4.1

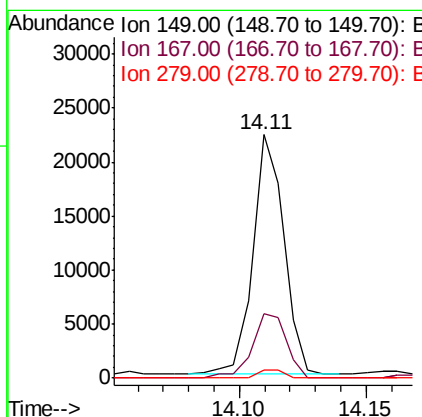



#87

Pervlene-d12

Concen: 20.000 ng

RT: 15.70 min Scan# 2315

Delta R.T. 0.02 min

Lab File: BF110327.D

Acq: 31 Oct 2018 12:45

Instrument :

BNA_F


ClientSampleId :

RBR-200036




Tot Ion:	264	Resp:	177554
Ion Ratio		Lower	Upper
264	100		
260	23.5	18.7	28.1
265	20.8	16.7	25.1

Manual Integrations
APPROVED

Sohil
11/1/2018 10:45:54 AM



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

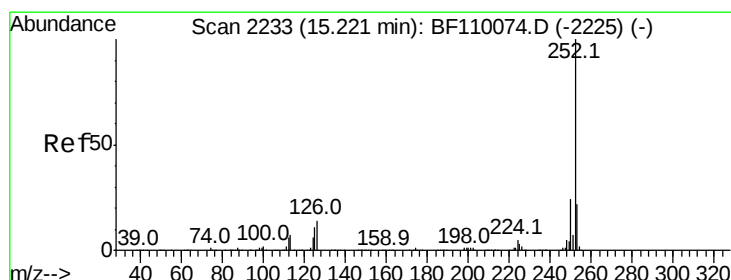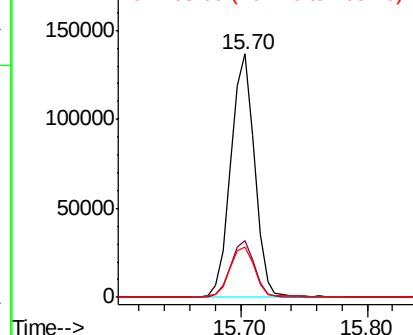

#88

Benzo(b)fluoranthene

Concen: 4.194 ng m

RT: 15.24 min Scan# 2236




Delta R.T. 0.01 min


Lab File: BF110327.D

Acq: 31 Oct 2018 12:45

Tgt Ion:	252	Resp:	43001
Ion Ratio		Lower	Upper
252	100		
253	22.2	17.2	25.8
125	12.6	8.2	12.4#

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

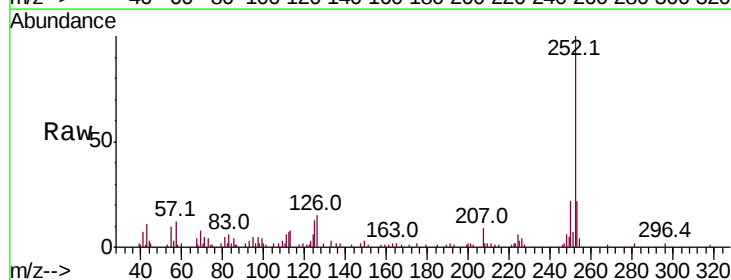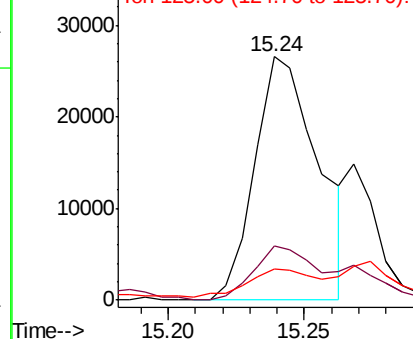

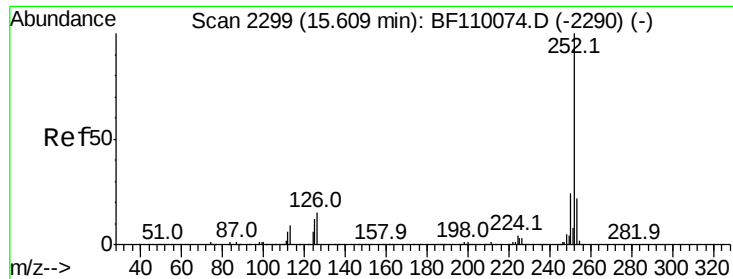

#90

Benzo(a)pyrene

Concen: 2.646 ng

RT: 15.63 min Scan# 2303

Delta R.T. 0.01 min

Lab File: BF110327.D

Acq: 31 Oct 2018 12:45

Instrument :

BNA_F

ClientSampleId :

RBR-200036

Tot Ion:	252	Resp:	24962
Ion Ratio	Lower	Upper	
252	100		
253	21.9	18.2	27.4
125	11.4	9.0	13.6

Manual Integrations
APPROVED

Sohil
11/1/2018 10:45:54 AM

