

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF103118\
 Data File : BF110339.D
 Acq On : 31 Oct 2018 18:09
 Operator : JU/SJ
 Sample : J5730-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 102918-TIPC-E-D-M

Quant Time: Nov 01 04:23:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 31 14:18:16 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	90654	20.00	ng	0.00
21) Naphthalene-d8	8.26	136	365717	20.00	ng	0.00
39) Acenaphthene-d10	10.02	164	167895	20.00	ng	0.00
64) Phenanthrene-d10	11.52	188	292688	20.00	ng	0.00
76) Chrysene-d12	14.17	240	170745	20.00	ng	0.00
87) Perylene-d12	15.71	264	148337	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	209638	37.66	ng	0.00
7) Phenol-d6	6.59	99	162254	22.79	ng	-0.01
23) Nitrobenzene-d5	7.54	82	543169	88.09	ng	0.00
42) 2,4,6-Tribromophenol	10.82	330	131158	78.86	ng	0.00
45) 2-Fluorobiphenyl	9.33	172	999957	93.52	ng	0.00
79) Terphenyl-d14	13.10	244	751413	91.52	ng	0.00
Target Compounds						
10) Phenol	6.60	94	21073	2.769	ng	Qvalue # 70

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF103118\
Data File : BF110339.D
Acq On : 31 Oct 2018 18:09
Operator : JU/SJ
Sample : J5730-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
102918-TIPC-E-D-M

Quant Time: Nov 01 04:23:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 31 14:18:16 2018
Response via : Initial Calibration

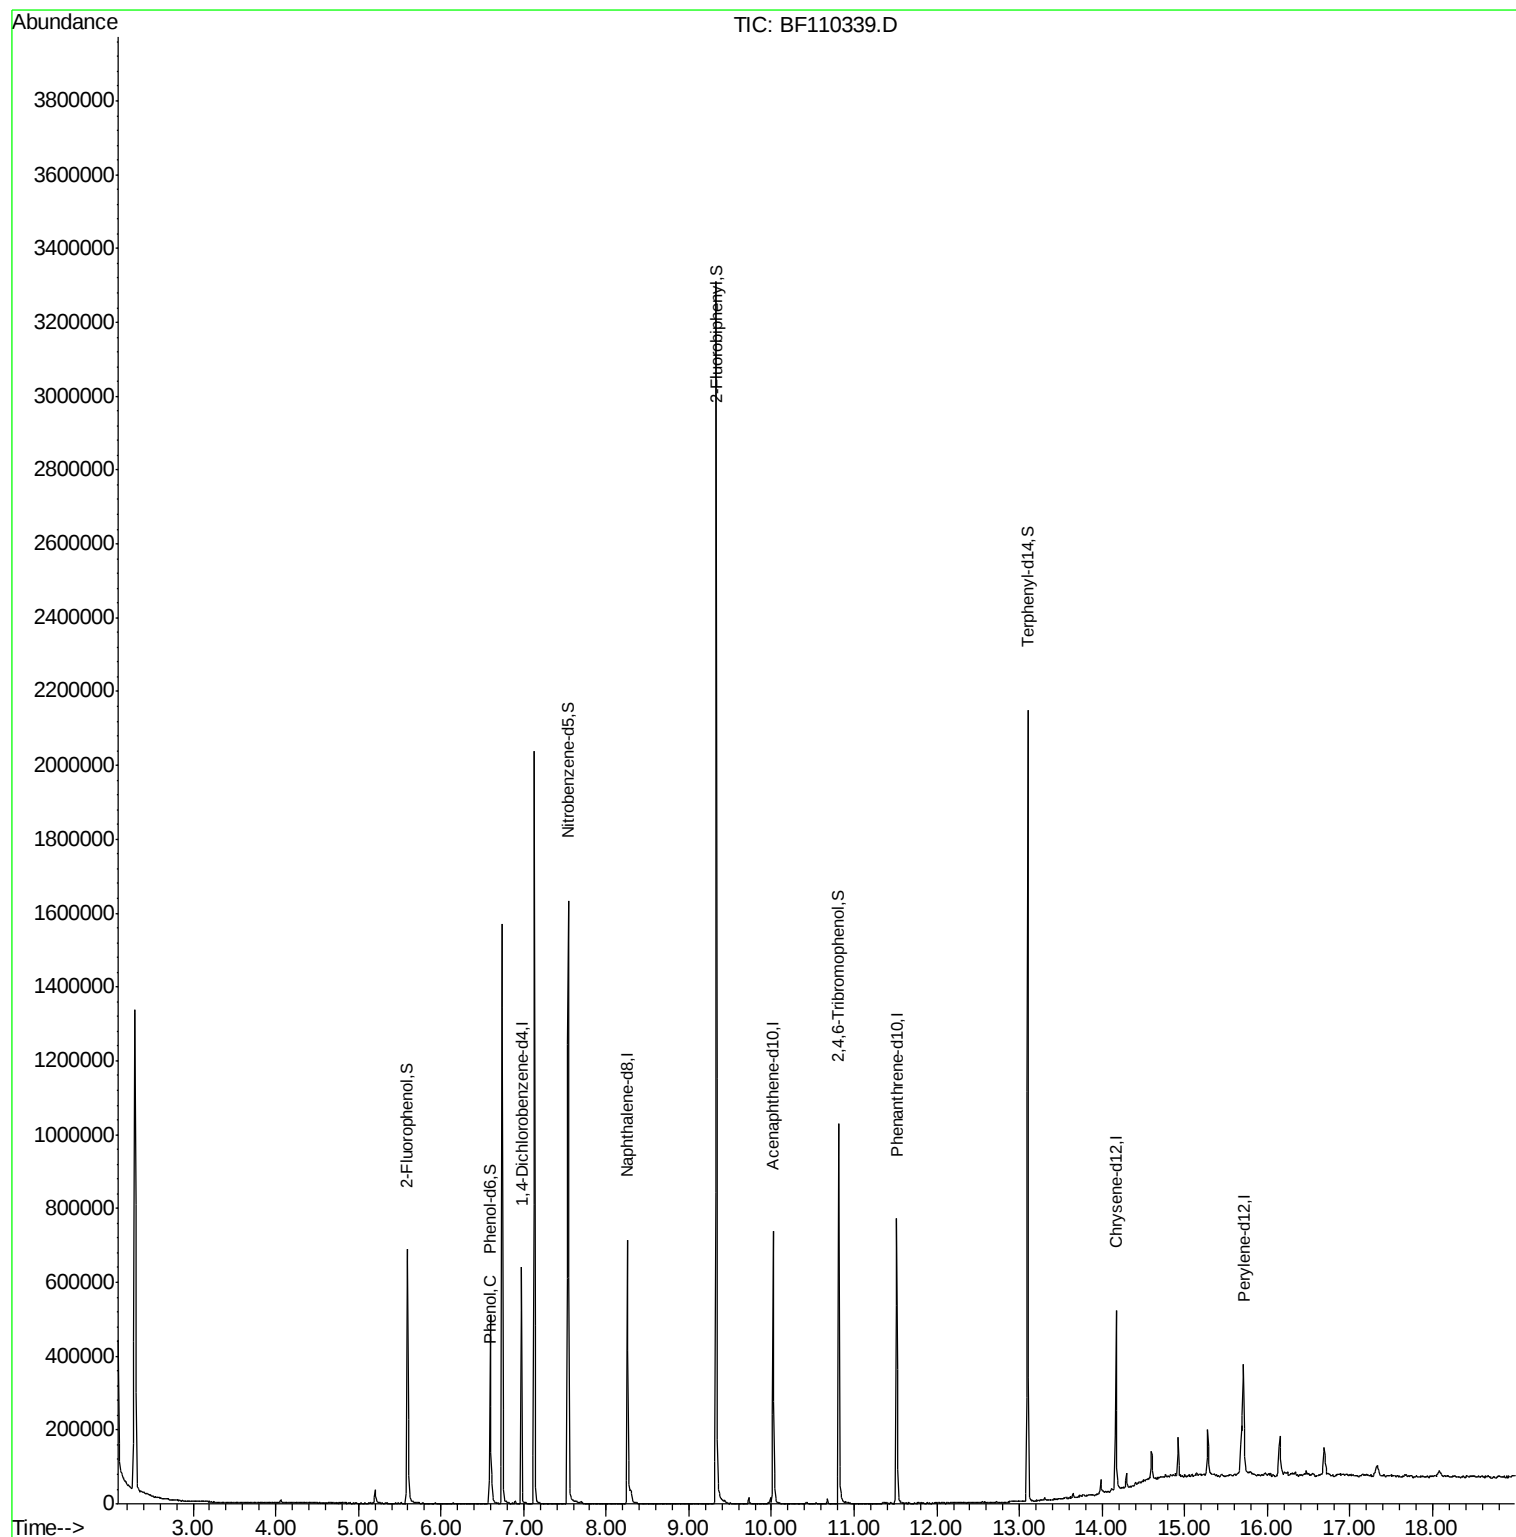




#1


1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 831
Delta R.T. 0.00 min
Lab File: BF110339.D
Acq: 31 Oct 2018 18:09

Instrument :
BNA_F
ClientSampleId :
102918-TIPC-E-D-M



Tot Ion:152 Resp: 90654
Ion Ratio Lower Upper
152 100
150 158.8 122.7 184.1
115 60.5 49.1 73.7

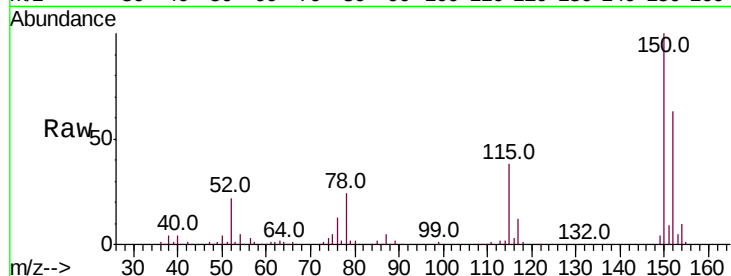

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

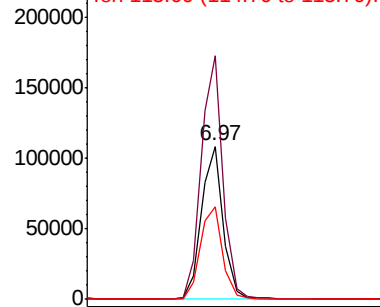


Time-->

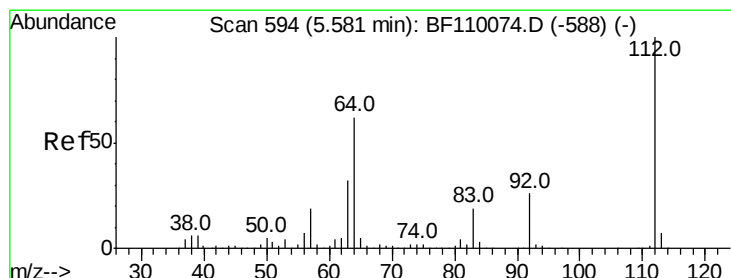


#5

2-Fluorophenol
Concen: 37.658 ng
RT: 5.60 min Scan# 597
Delta R.T. 0.01 min
Lab File: BF110339.D
Acq: 31 Oct 2018 18:09


Tgt Ion:112 Resp: 209638
Ion Ratio Lower Upper
112 100
64 56.1 44.1 66.1
63 30.1 23.7 35.5

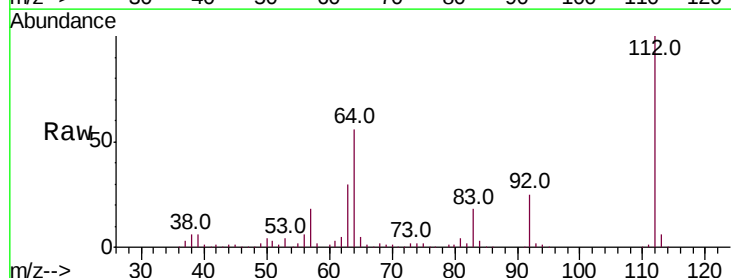


Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

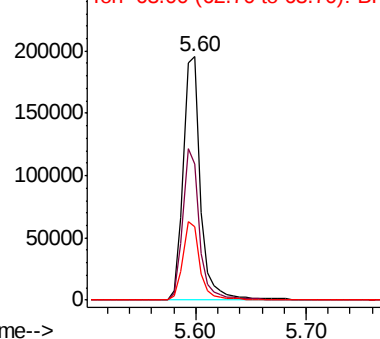

Time-->



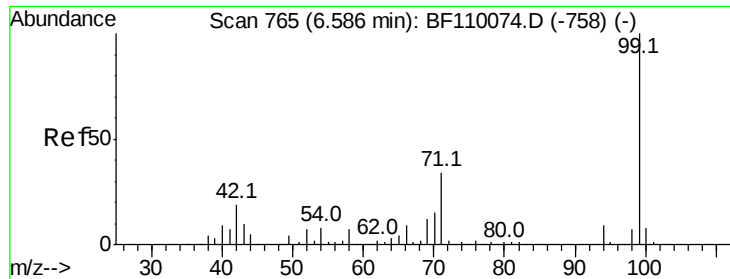

#7

Phenol-d6

Concen: 22.787 ng

RT: 6.59 min Scan# 766

Delta R.T. -0.01 min

Lab File: BF110339.D

Acq: 31 Oct 2018 18:09

Instrument :

BNA_F

ClientSampleId :

102918-TIPC-E-D-M


Tot Ion: 99 Resp: 162254

Ion Ratio Lower Upper




99 100

42 19.0 15.8 23.6

71 34.9 28.0 42.0

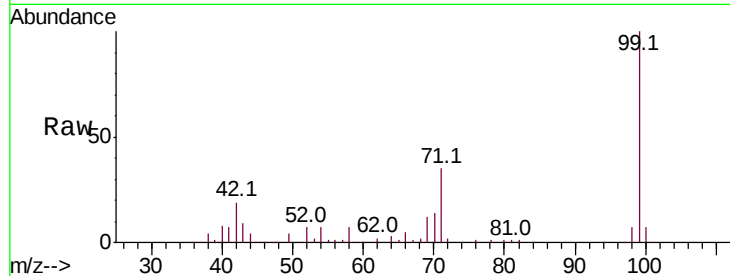

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

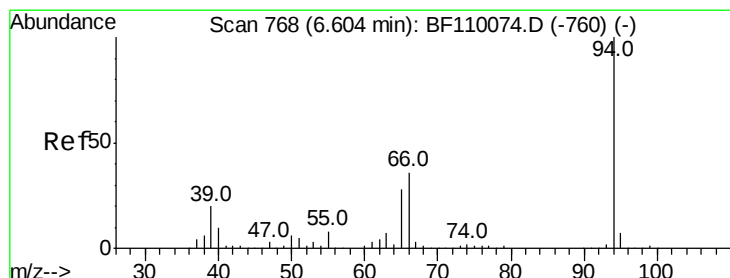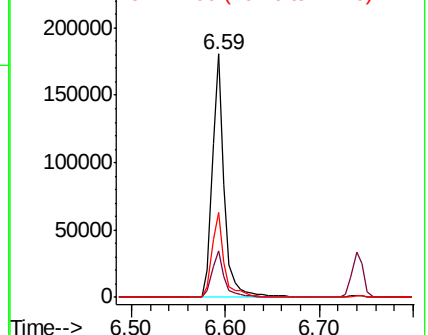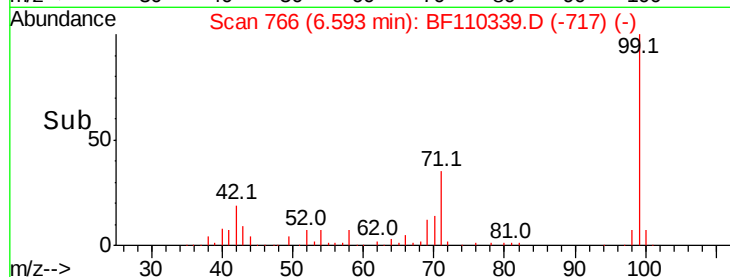

#10

Phenol

Concen: 2.769 ng

RT: 6.60 min Scan# 768

Delta R.T. -0.01 min

Lab File: BF110339.D

Acq: 31 Oct 2018 18:09


Tgt Ion: 94 Resp: 21073

Ion Ratio Lower Upper



94 100

65 30.9 25.3 65.3

66 45.1 54.5 94.5#

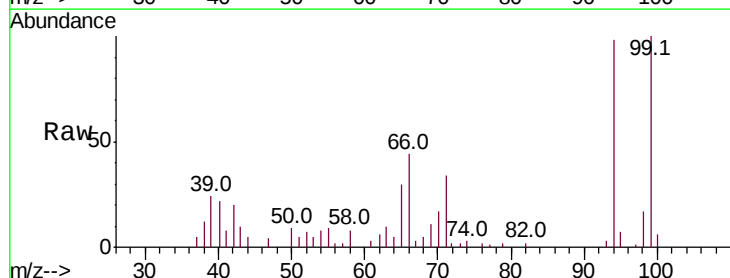

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1



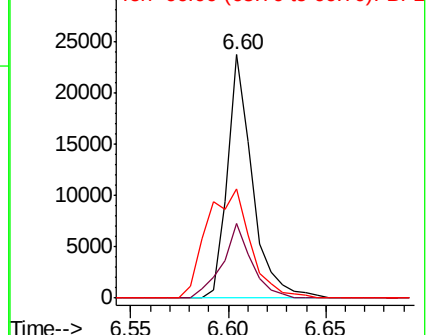
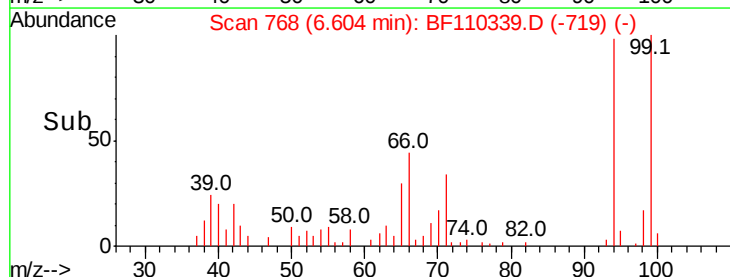




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.26 min Scan# 1049
Delta R.T. 0.00 min
Lab File: BF110339.D
Acq: 31 Oct 2018 18:09




Instrument :
BNA_F
ClientSampleId :
102918-TIPC-E-D-M

Tot Ion:	136	Resp:	365717
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.8	13.2
54	7.6	5.4	8.2
68	5.2	4.2	6.2

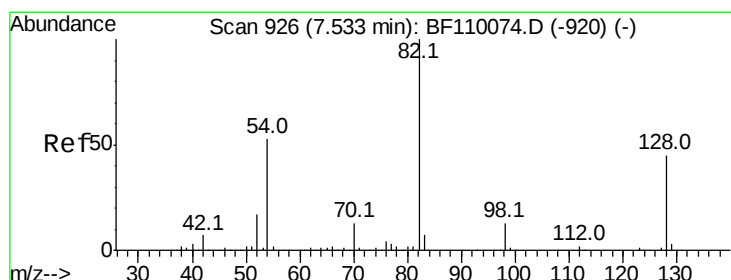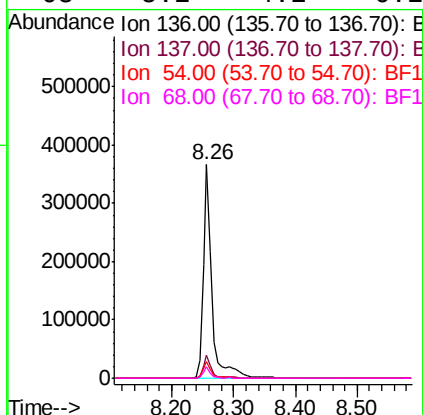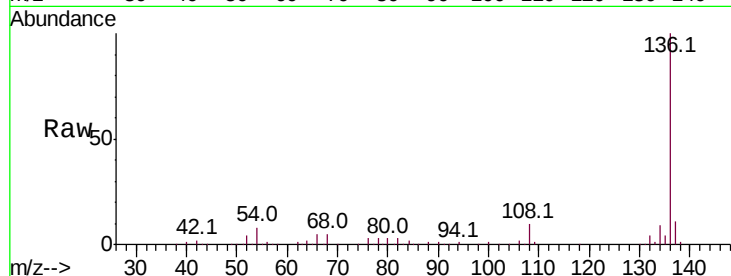

#23
Nitrobenzene-d5
Concen: 88.093 ng
RT: 7.54 min Scan# 927
Delta R.T. 0.00 min
Lab File: BF110339.D
Acq: 31 Oct 2018 18:09

Tgt Ion:	82	Resp:	543169
Ion	Ratio	Lower	Upper
82	100		
128	45.5	34.2	51.2
54	52.8	38.6	58.0


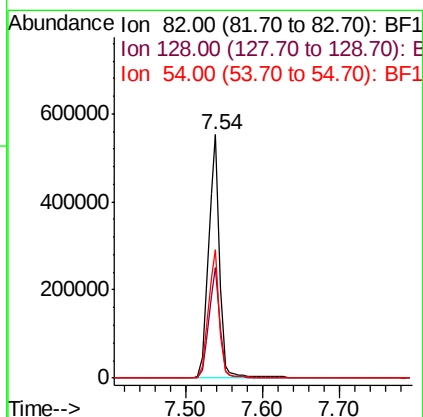

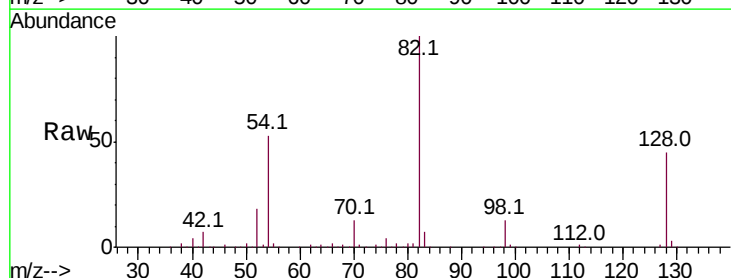




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.02 min Scan# 1348
Delta R.T. -0.01 min
Lab File: BF110339.D
Acq: 31 Oct 2018 18:09




Instrument :
BNA_F
ClientSampleId :
102918-TIPC-E-D-M


Tot Ion:164 Resp: 167895
Ion Ratio Lower Upper
164 100
162 101.6 83.0 124.6
160 44.3 37.0 55.6

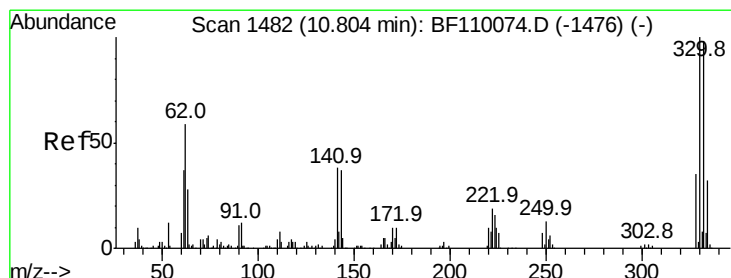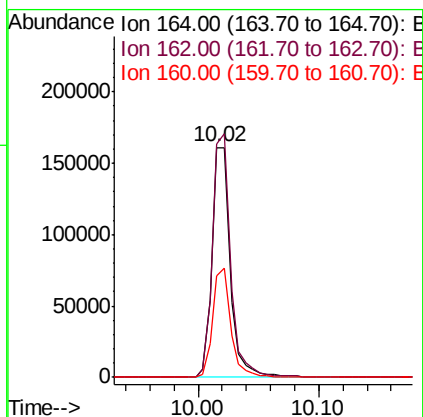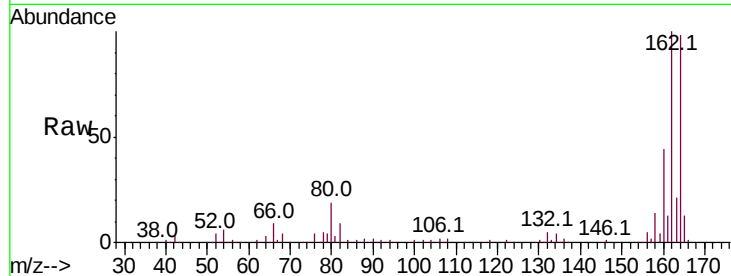

#42
2,4,6-Tribromophenol
Concen: 78.863 ng
RT: 10.82 min Scan# 1484
Delta R.T. 0.00 min
Lab File: BF110339.D
Acq: 31 Oct 2018 18:09

Tgt Ion:330 Resp: 131158
Ion Ratio Lower Upper
330 100
332 96.9 77.1 115.7
141 38.3 27.0 40.4

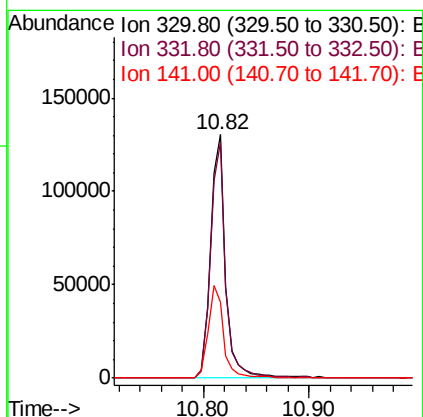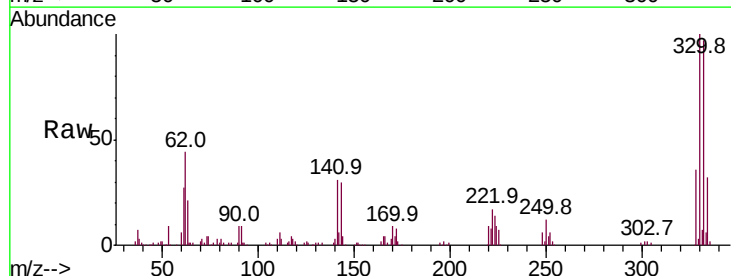


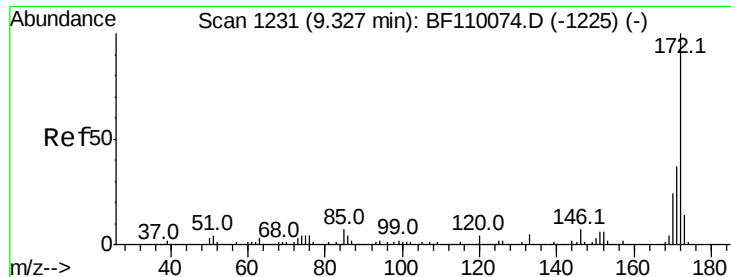




#45
 2-Fluorobiphenyl
 Concen: 93.522 ng
 RT: 9.33 min Scan# 1232
 Delta R.T. 0.00 min
 Lab File: BF110339.D
 Acq: 31 Oct 2018 18:09

Instrument :
 BNA_F
 ClientSampleId :
 102918-TIPC-E-D-M

Tot Ion	Ratio	Lower	Upper
172	100		
171	35.9	28.6	43.0
170	23.9	19.7	29.5

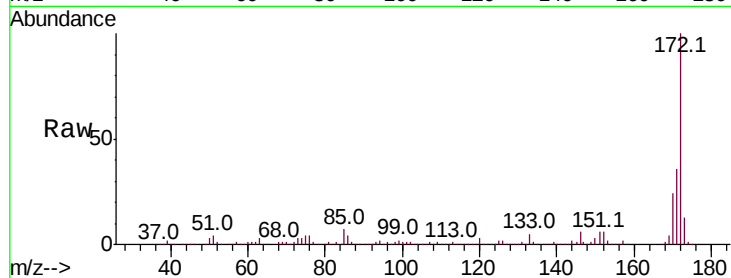


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

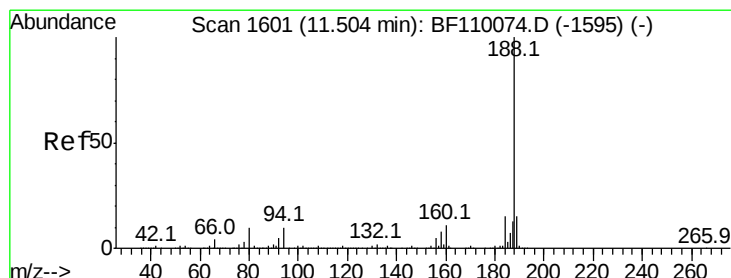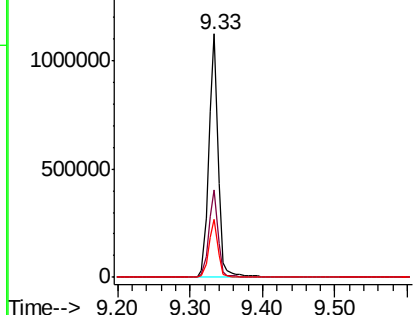




#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.52 min Scan# 1603
 Delta R.T. 0.00 min
 Lab File: BF110339.D
 Acq: 31 Oct 2018 18:09

Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.2	7.2	10.8
80	9.3	7.9	11.9

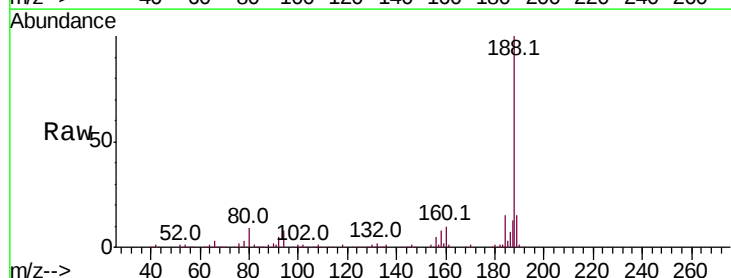

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF1
 Ion 80.00 (79.70 to 80.70): BF1

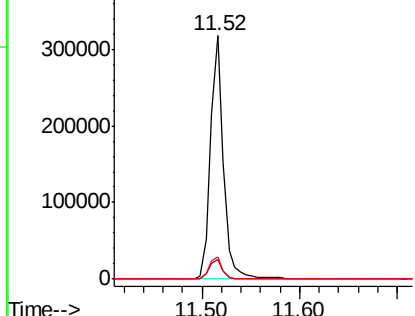



#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.17 min Scan# 2054

Delta R.T. 0.00 min

Lab File: BF110339.D

Acq: 31 Oct 2018 18:09

Instrument :

BNA_F

ClientSampleId :

102918-TIPC-E-D-M


Tot Ion:240 Resp: 170745

Ion Ratio Lower Upper

240 100

120 10.2 8.3 12.5




236 25.3 21.2 31.8

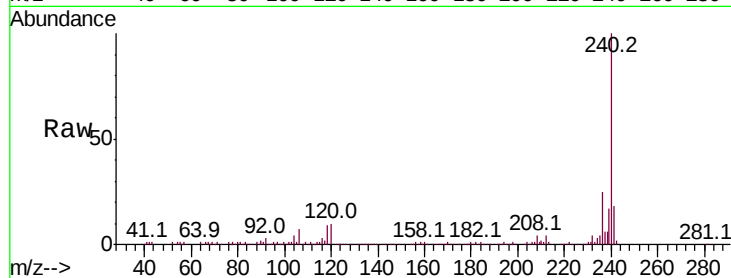

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

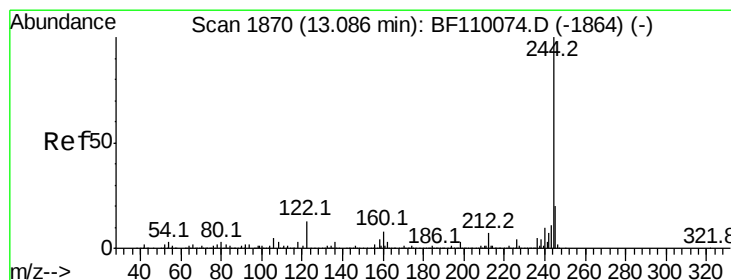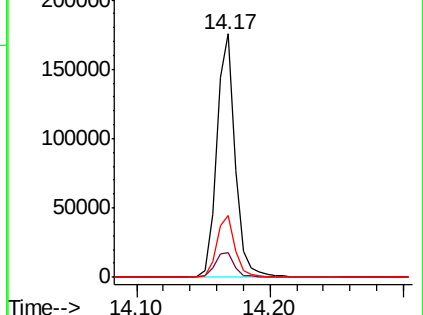

#79

Terphenyl-d14

Concen: 91.524 ng

RT: 13.10 min Scan# 1872

Delta R.T. -0.01 min

Lab File: BF110339.D

Acq: 31 Oct 2018 18:09


Tgt Ion:244 Resp: 751413

Ion Ratio Lower Upper

244 100

212 7.0 5.8 8.8



122 12.8 8.7 13.1

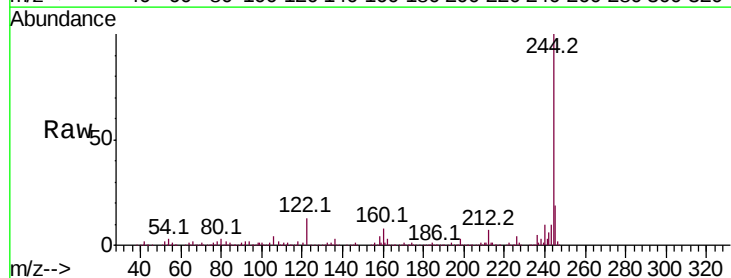


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

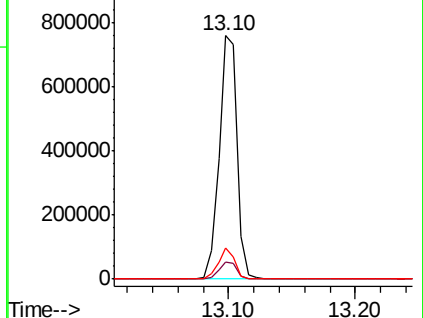


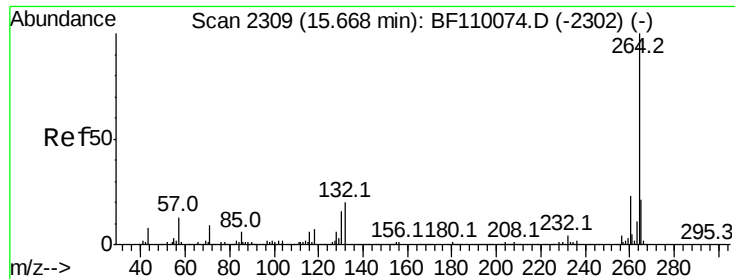

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.71 min Scan# 2316
 Delta R.T. 0.01 min
 Lab File: BF110339.D
 Acq: 31 Oct 2018 18:09

Instrument :
 BNA_F
 ClientSampleId :
 102918-TIPC-E-D-M

Tot Ion:	264	Resp:	148337
Ion	Ratio	Lower	Upper
264	100		
260	22.8	18.7	28.1
265	21.3	16.7	25.1

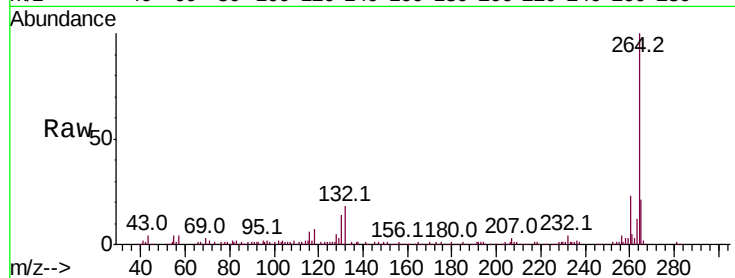

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

