


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF103118\
 Data File : BF110324.D
 Acq On : 31 Oct 2018 10:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 31 14:18:16 2018

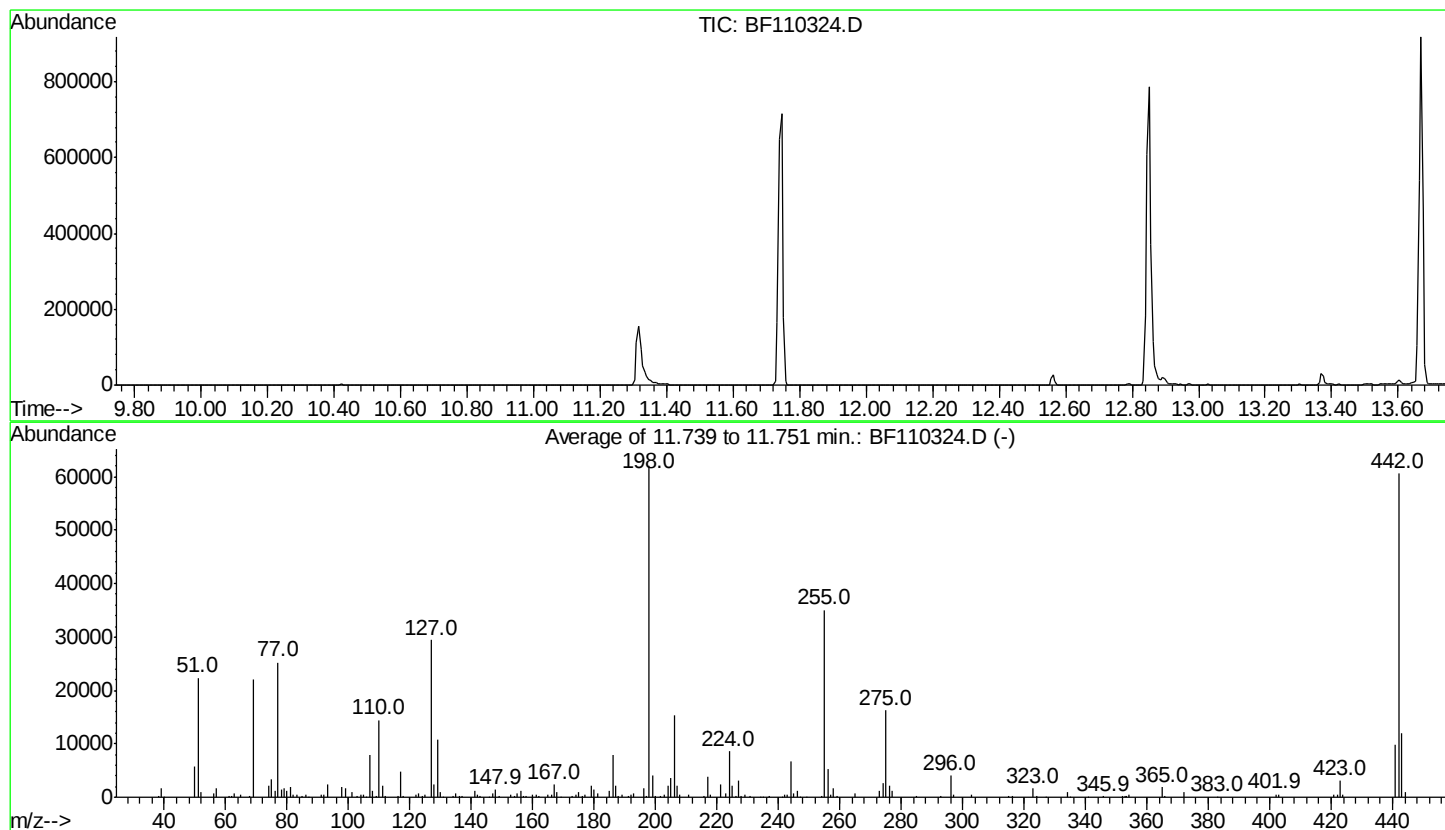

AutoFind: Scans 1641, 1642, 1643; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	22410	PASS
68	69	0.00	2	1.5	325	PASS
69	198	0.00	100	35.4	22007	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.3	29386	PASS
197	198	0.00	2	0.5	322	PASS
198	198	100	100	100.0	62082	PASS
199	198	5	9	6.6	4072	PASS
275	198	10	60	26.1	16234	PASS
365	198	1	100	2.9	1821	PASS
441	198	0.01	100	15.7	9766	PASS
442	198	50	100	97.6	60570	PASS
443	442	15	24	19.7	11934	PASS