


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF103118\
Data File : BF110350.D
Acq On : 1 Nov 2018 00:07
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 31 14:18:16 2018

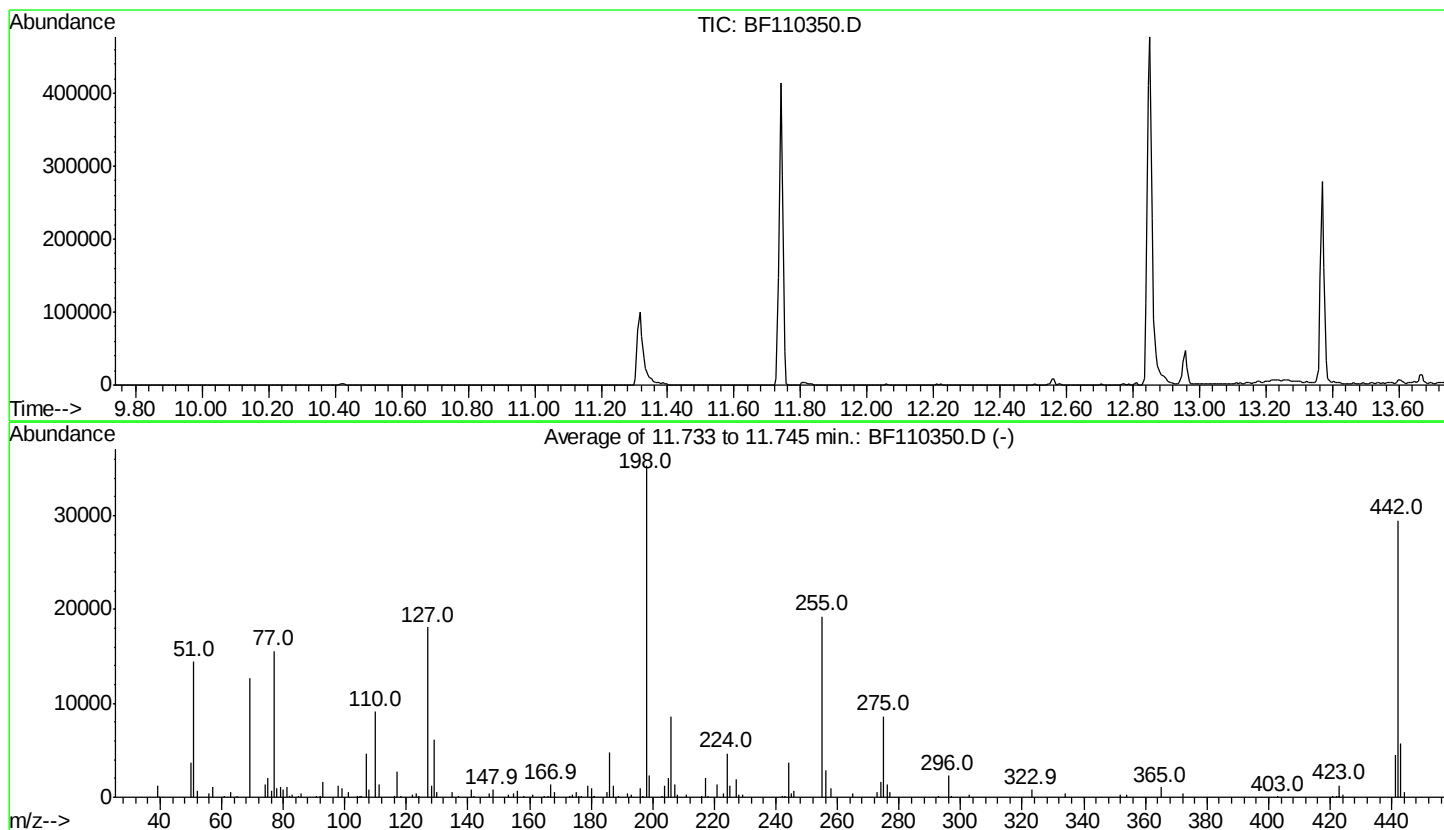

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	14403	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.1	12740	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.3	18117	PASS
197	198	0.00	2	0.4	135	PASS
198	198	100	100	100.0	35328	PASS
199	198	5	9	6.6	2334	PASS
275	198	10	60	24.5	8654	PASS
365	198	1	100	3.0	1043	PASS
441	198	0.01	100	12.9	4563	PASS
442	198	50	100	83.6	29529	PASS
443	442	15	24	19.6	5784	PASS