
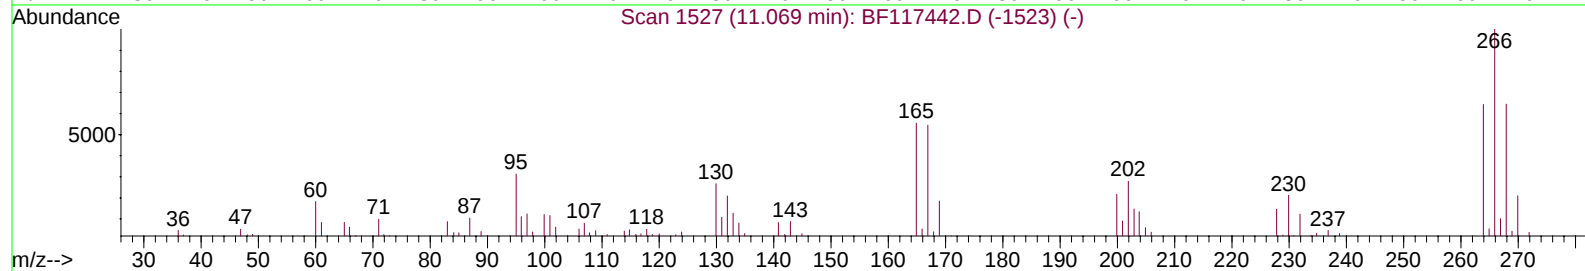
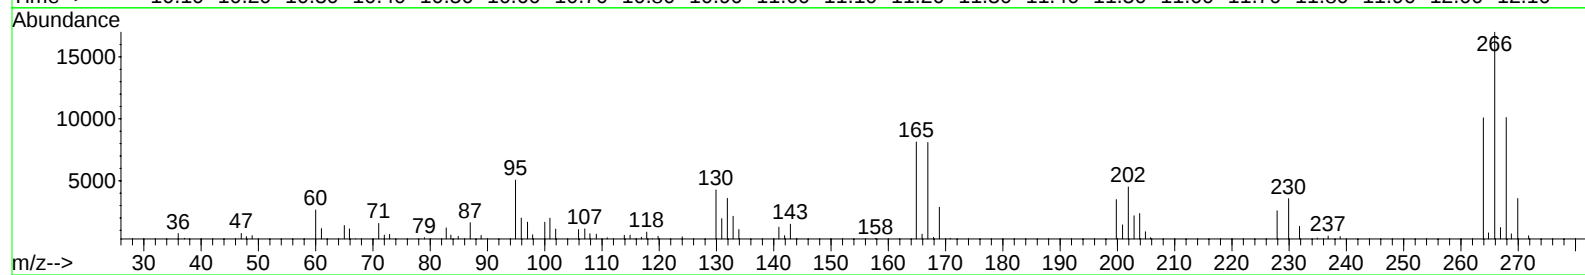


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF103119\
Data File : BF117651.D
Acq On : 31 Oct 2019 11:01
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 19:10:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

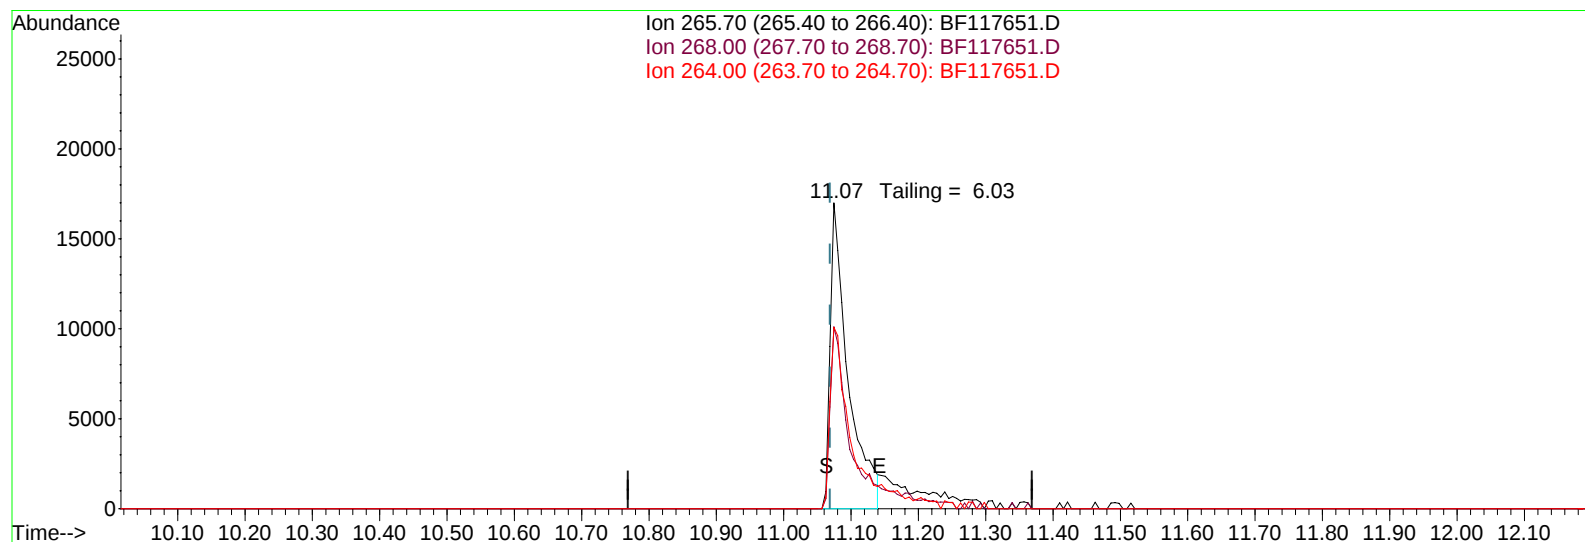

TIC: BF117651.D

(70) Pentachlorophenol (C)




11.074min (+0.006) 0.00ng

response 35618

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	59.48
264.00	64.30	59.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF103119\
Data File : BF117651.D
Acq On : 31 Oct 2019 11:01
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 19:10:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

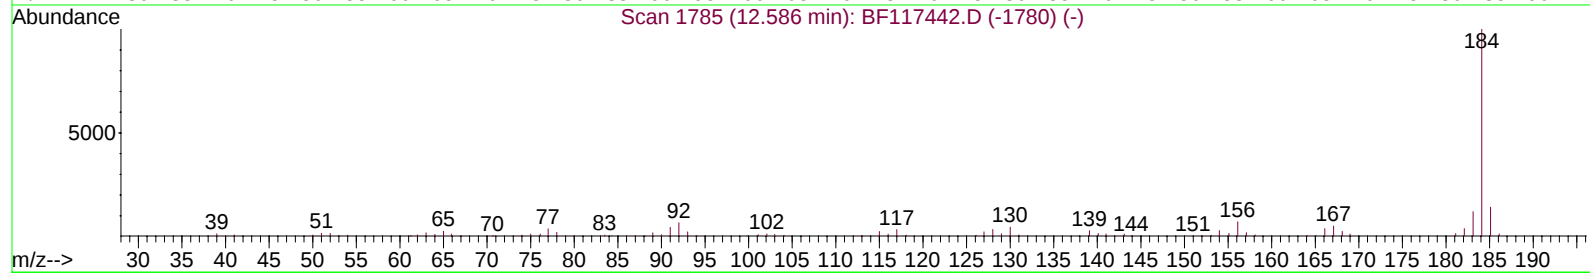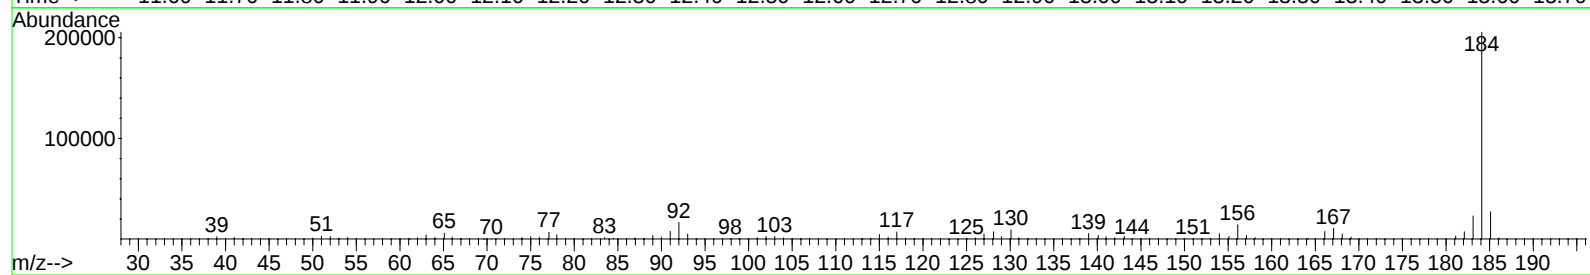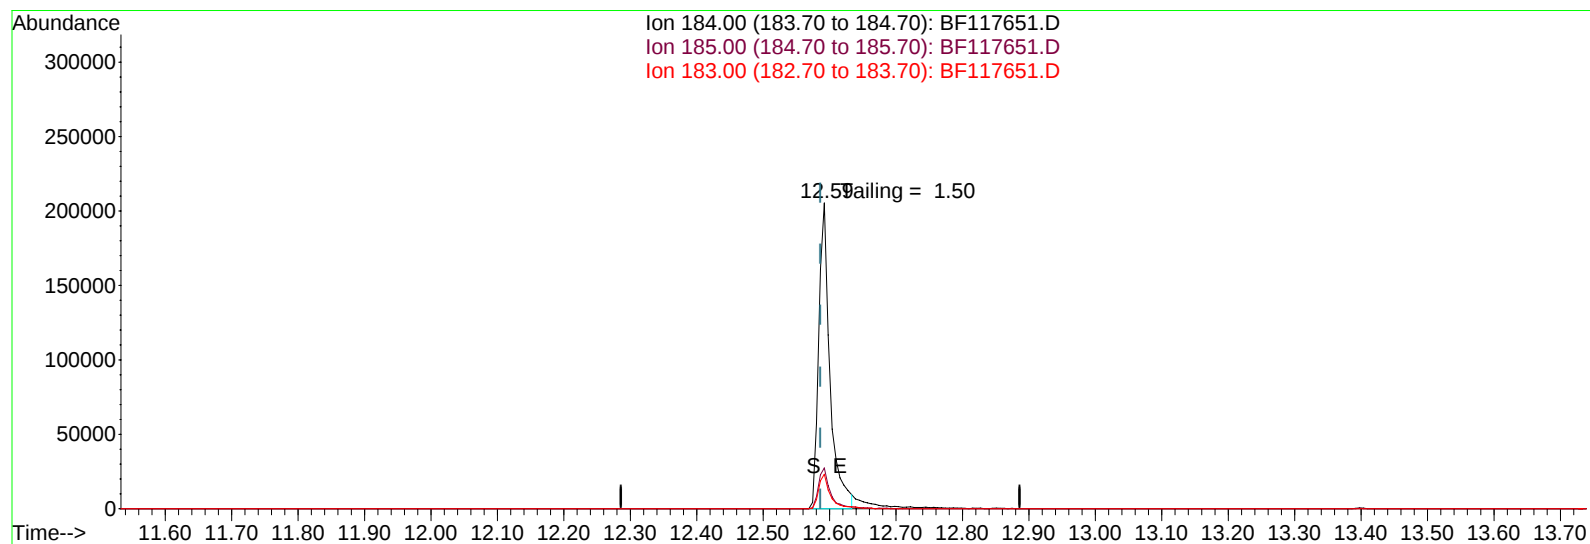

TIC: BF117651.D

(77) Benzidine

12.592min (+0.006) 0.00ng

response 258701

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	13.32
183.00	12.00	11.31
0.00	0.00	0.00