


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF103119\
 Data File : BF117651.D
 Acq On : 31 Oct 2019 11:01
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 18 18:53:31 2019

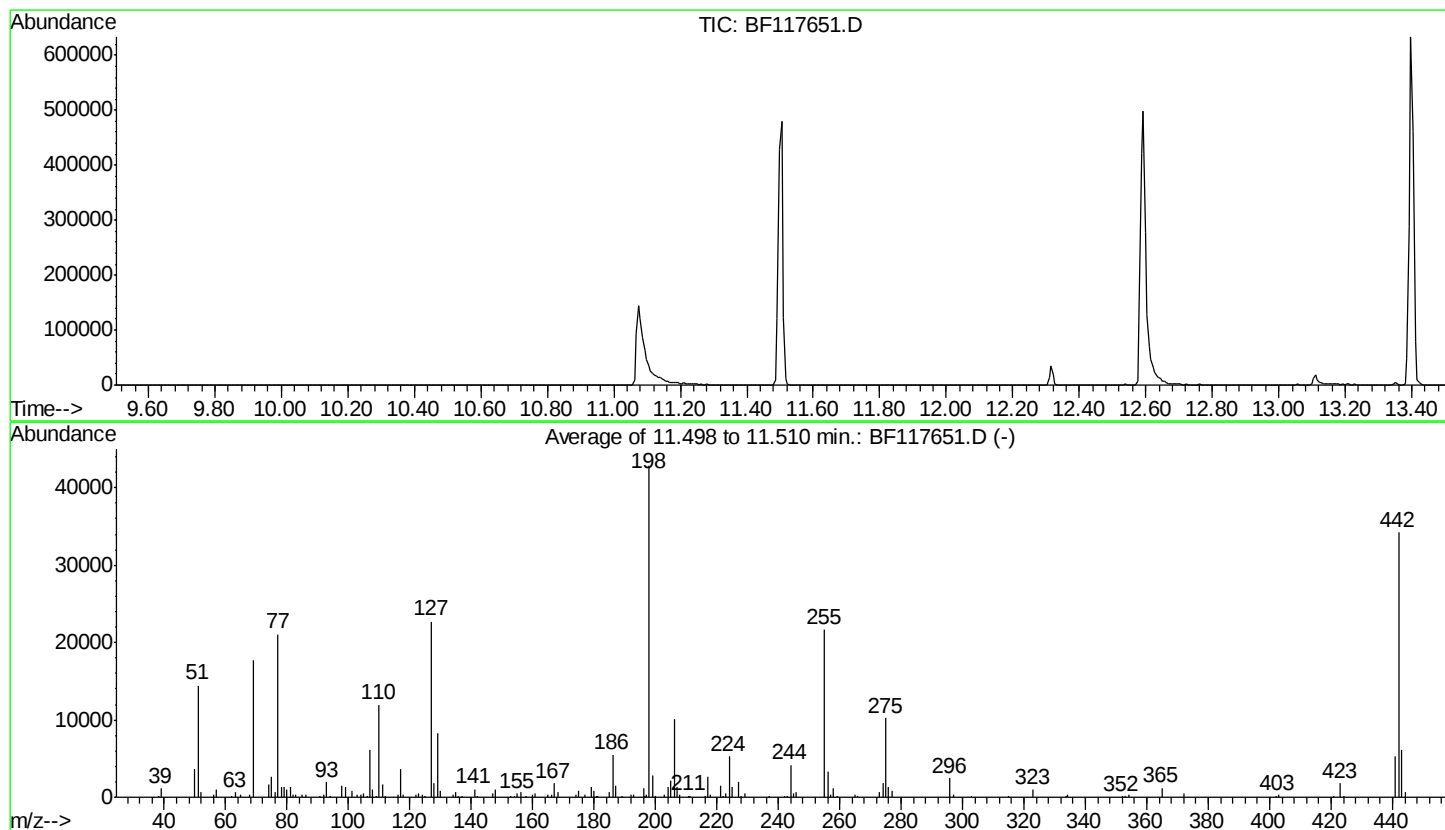

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	14469	PASS
68	69	0.00	2	1.4	255	PASS
69	198	0.00	100	41.4	17759	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.9	22676	PASS
197	198	0.00	2	0.6	263	PASS
198	198	100	100	100.0	42868	PASS
199	198	5	9	6.7	2889	PASS
275	198	10	60	23.8	10214	PASS
365	198	1	100	2.8	1208	PASS
441	198	0.01	100	12.3	5261	PASS
442	198	50	100	79.9	34253	PASS
443	442	15	24	17.9	6136	PASS