
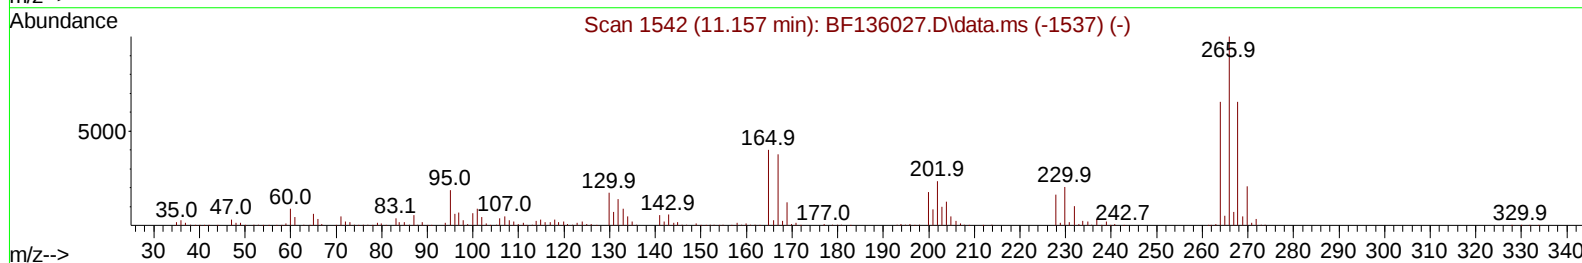
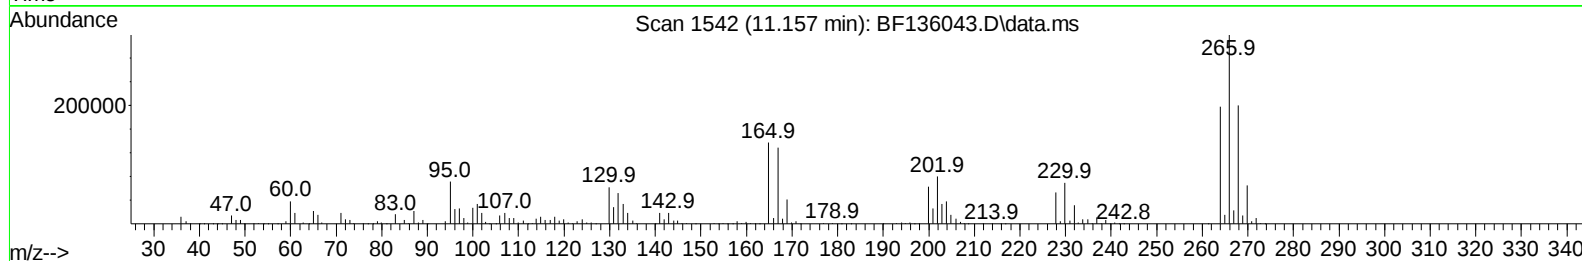


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103123\
Data File : BF136043.D
Acq On : 31 Oct 2023 10:55
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 20:42:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 01:13:02 2023
Response via : Initial Calibration

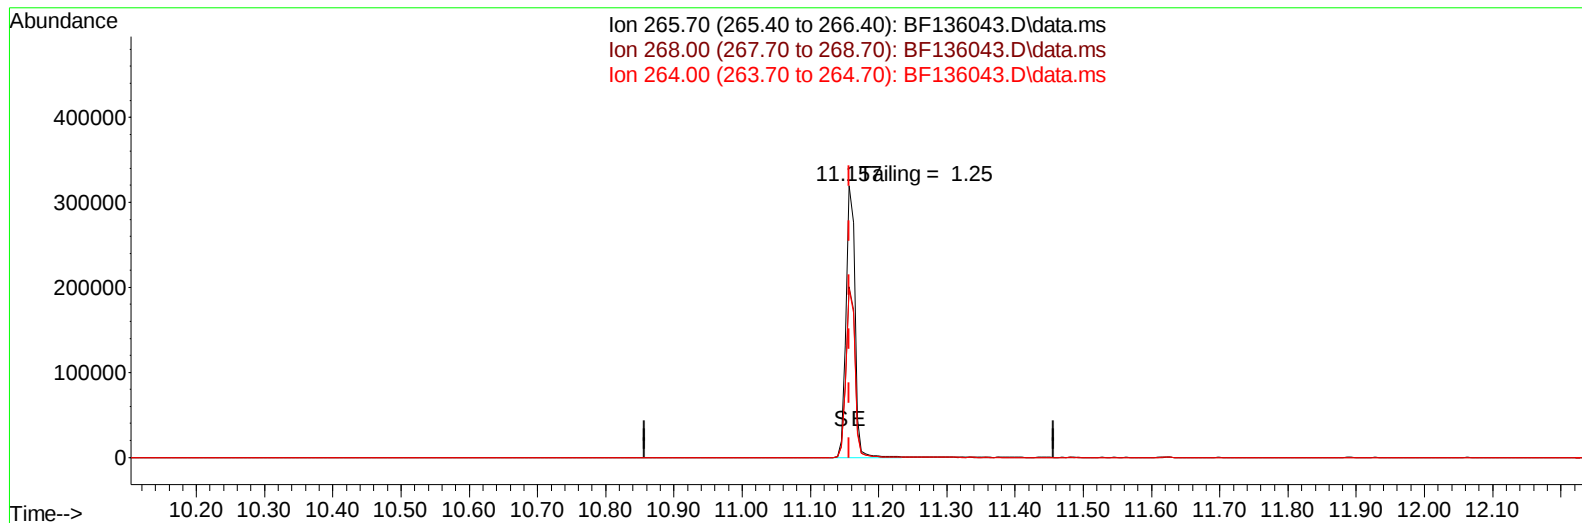

TIC: BF136043.D\data.ms

(70) Pentachlorophenol (C)




11.157min (+ 0.000) 281214.54 ng

response 289185

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.74
264.00	65.30	62.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103123\
Data File : BF136043.D
Acq On : 31 Oct 2023 10:55
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 20:42:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 01:13:02 2023
Response via : Initial Calibration

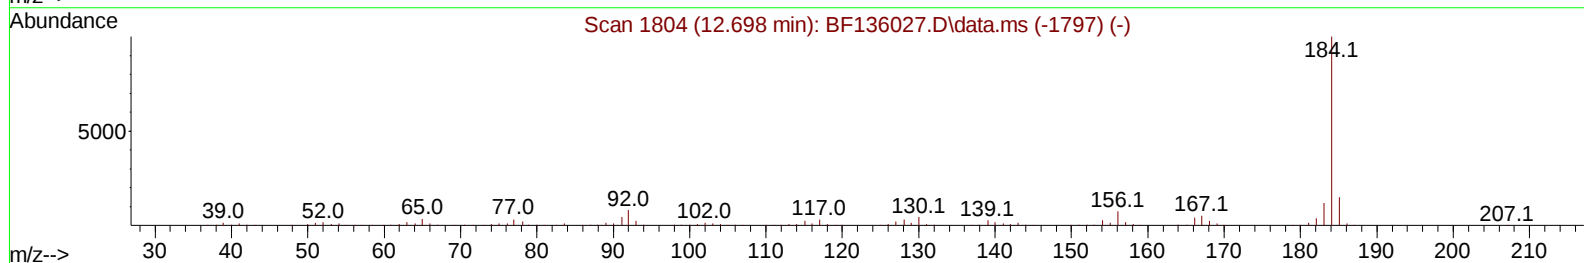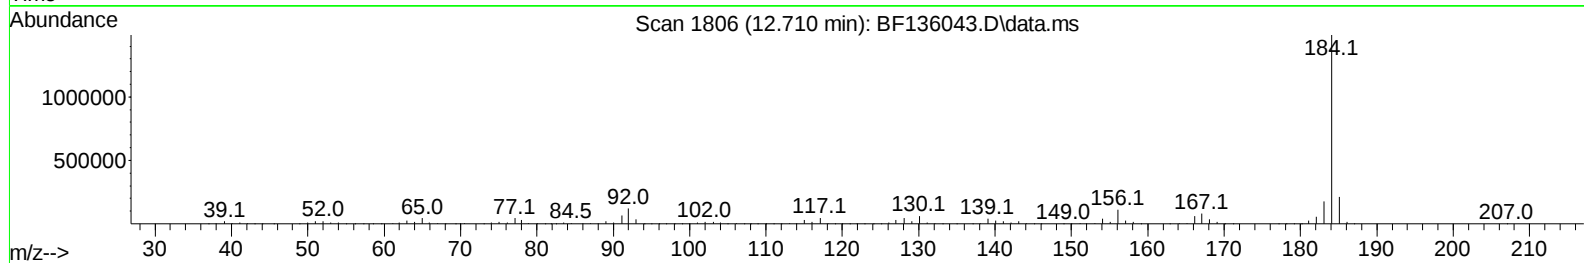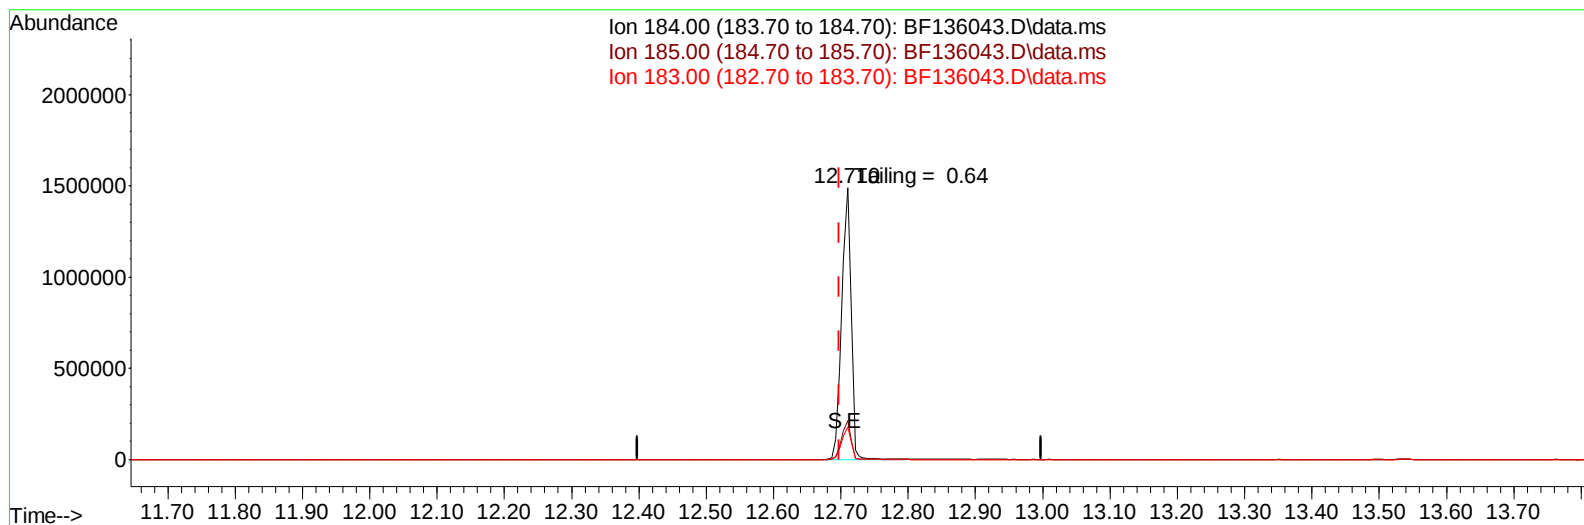

TIC: BF136043.D\data.ms

(77) Benzidine**12.710min (+ 0.012) 136030.11 ng****response 1429072**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.18
183.00	11.90	11.99
0.00	0.00	0.00