
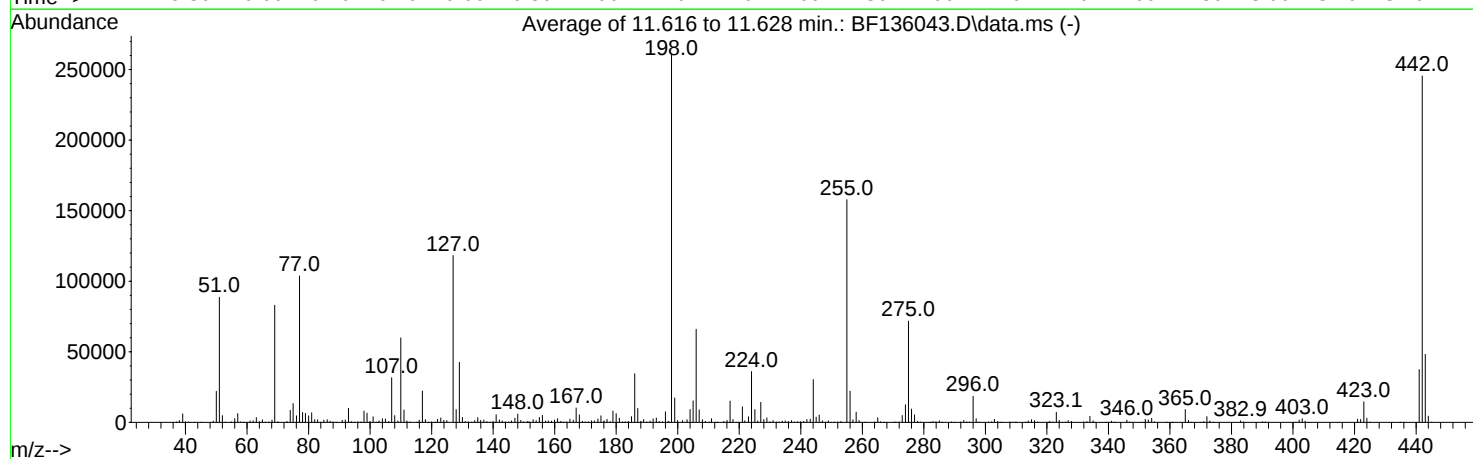


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103123\
 Data File : BF136043.D
 Acq On : 31 Oct 2023 10:55
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 31 01:13:02 2023

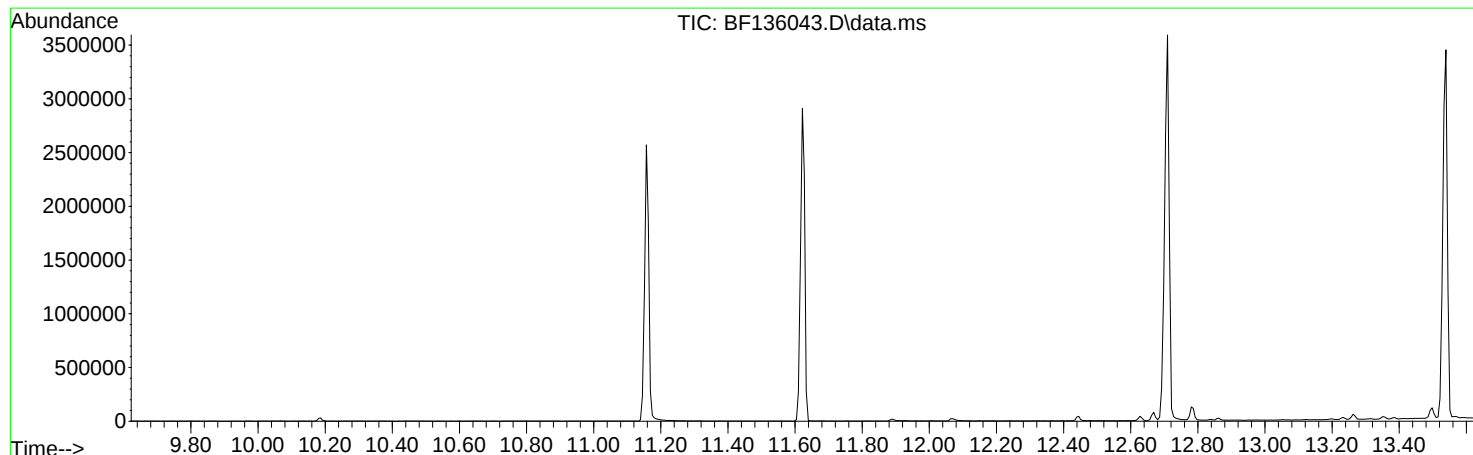




AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	88667	PASS
68	69	0.00	2	1.9	1611	PASS
69	198	0.00	100	31.9	83043	PASS
70	69	0.00	2	0.4	344	PASS
127	198	10	80	45.4	118253	PASS
197	198	0.00	2	0.3	767	PASS
198	198	100	100	100.0	260672	PASS
199	198	5	9	6.7	17404	PASS
275	198	10	60	27.5	71779	PASS
365	198	1	100	3.5	9100	PASS
441	198	0.01	100	14.4	37478	PASS
442	442	50	100	100.0	245515	PASS
443	442	15	24	19.7	48248	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103123\
Data File : BF136043.D
Acq On : 31 Oct 2023 10:55
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 31 20:42:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 01:13:02 2023
Response via : Initial Calibration

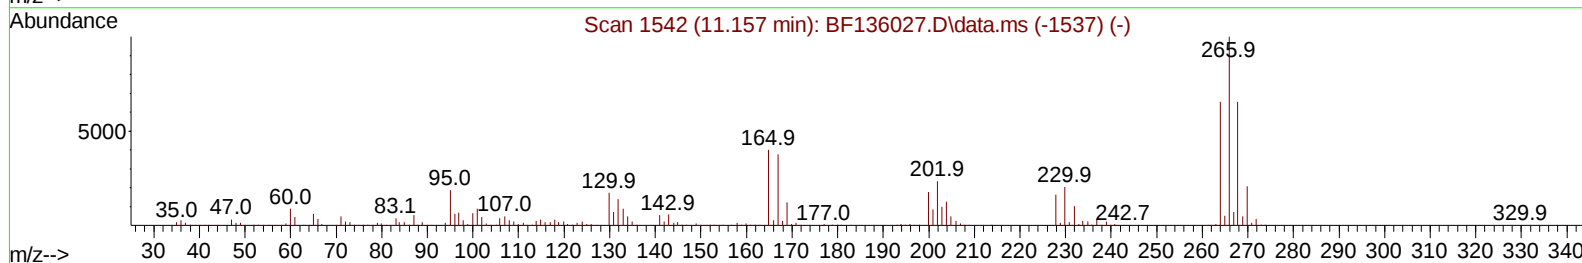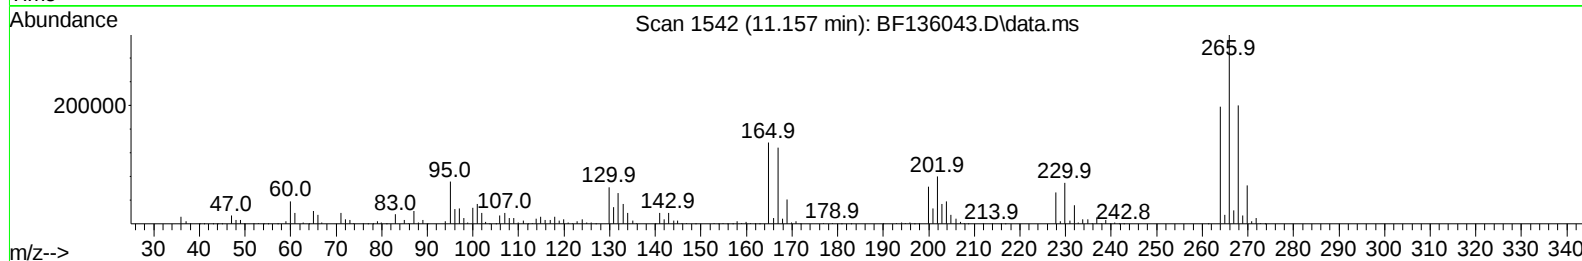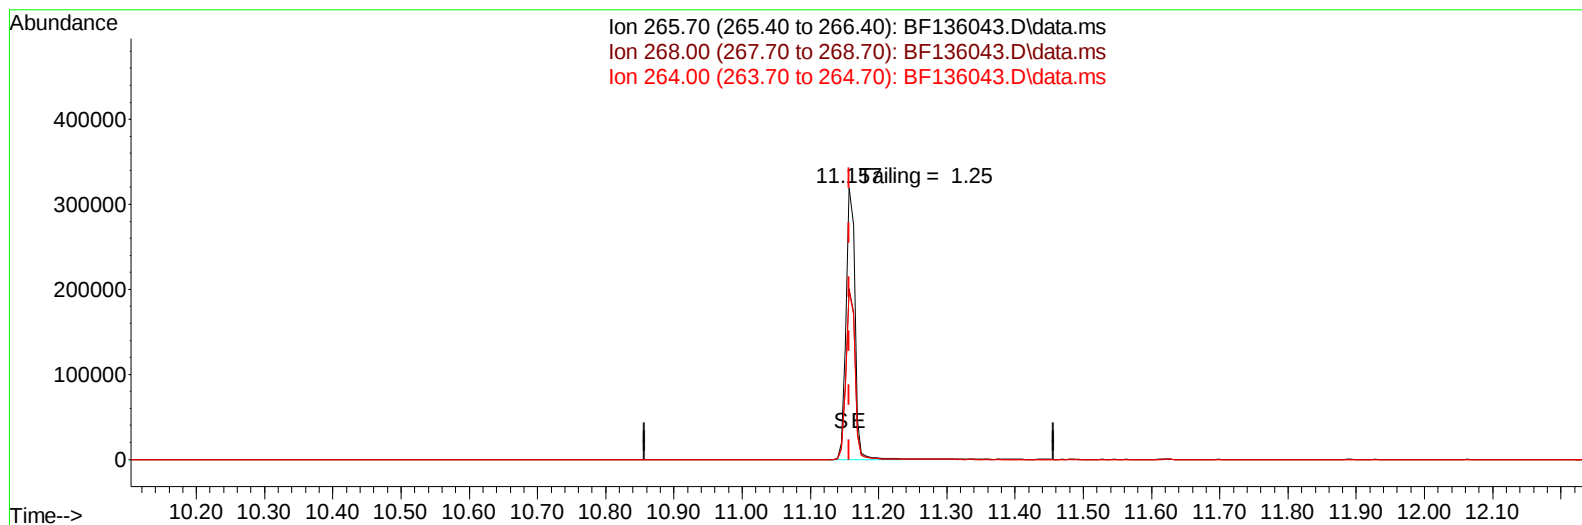

TIC: BF136043.D\data.ms

(70) Pentachlorophenol (C)

11.157min (+ 0.000) 281214.54 ng




response 289185

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.74
264.00	65.30	62.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103123\
Data File : BF136043.D
Acq On : 31 Oct 2023 10:55
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 31 20:42:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 01:13:02 2023
Response via : Initial Calibration

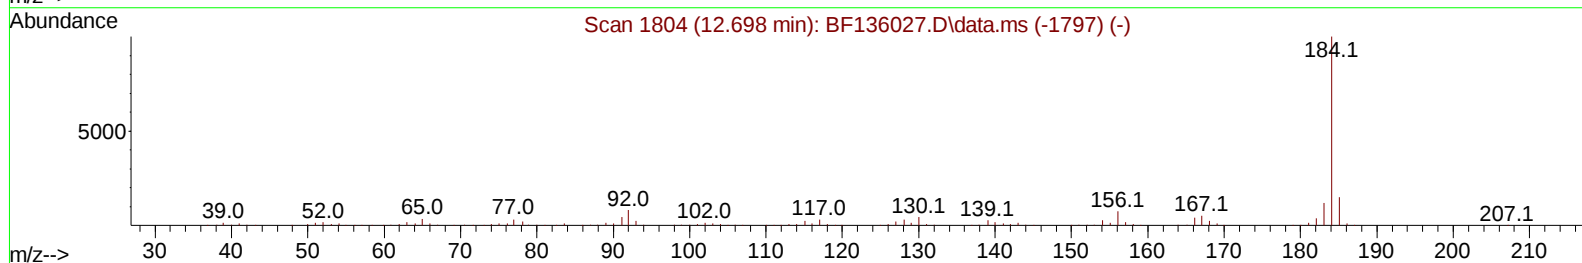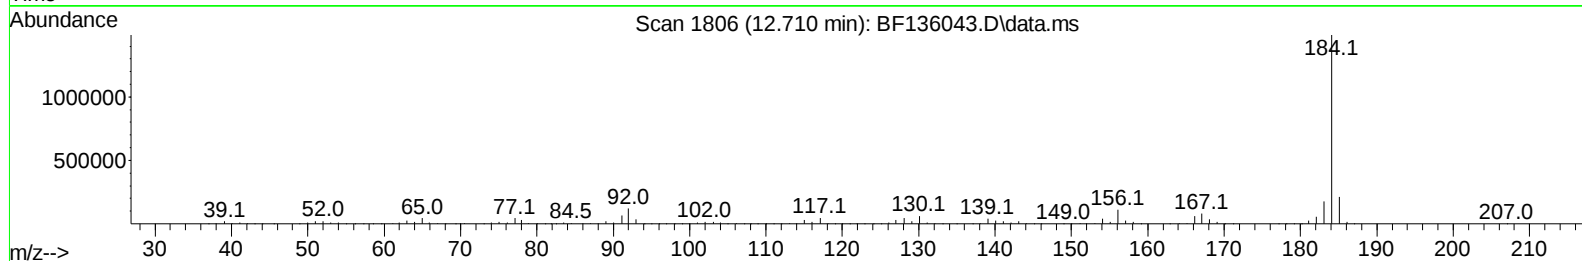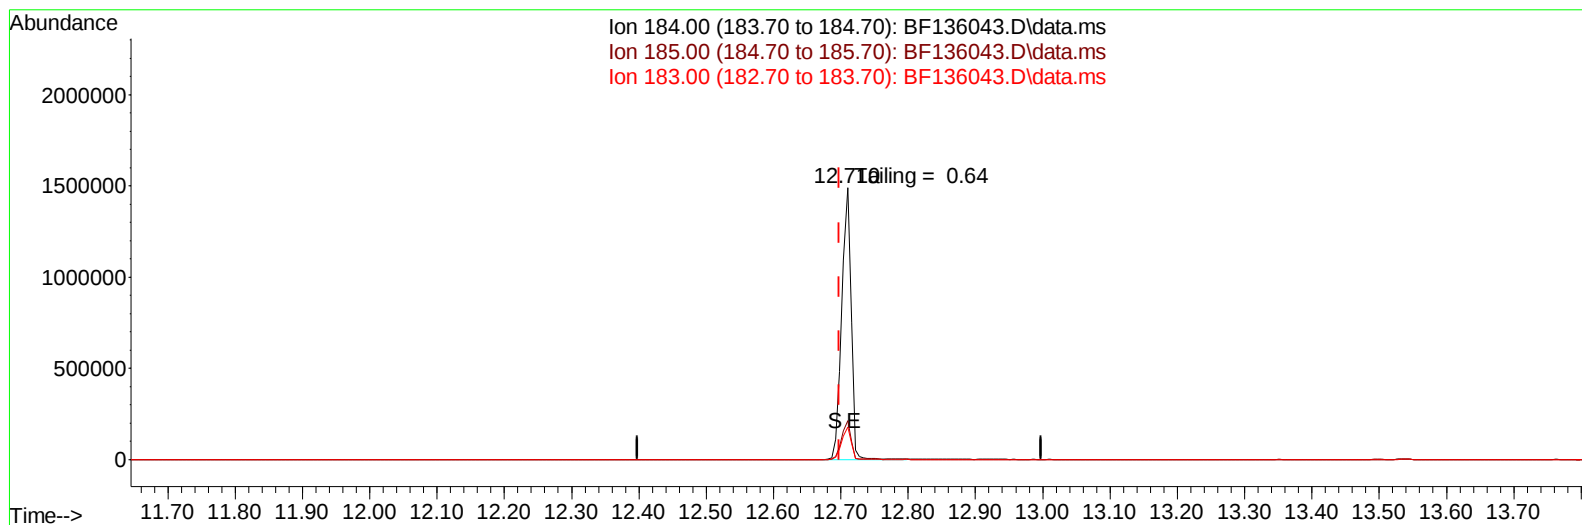

TIC: BF136043.D\data.ms

(77) Benzidine

12.710min (+ 0.012) 136030.11 ng

response 1429072

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.18
183.00	11.90	11.99
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/31/2023	BNA_F	<u>BF136043.D</u>
Compound Name	Response	Retention Time
DDT	645325	13.539
DDD	10292	13.263
DDE	351	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10643	655968	1.62

Instrument :
BNA_F
ClientSampleId :
DFTPP