
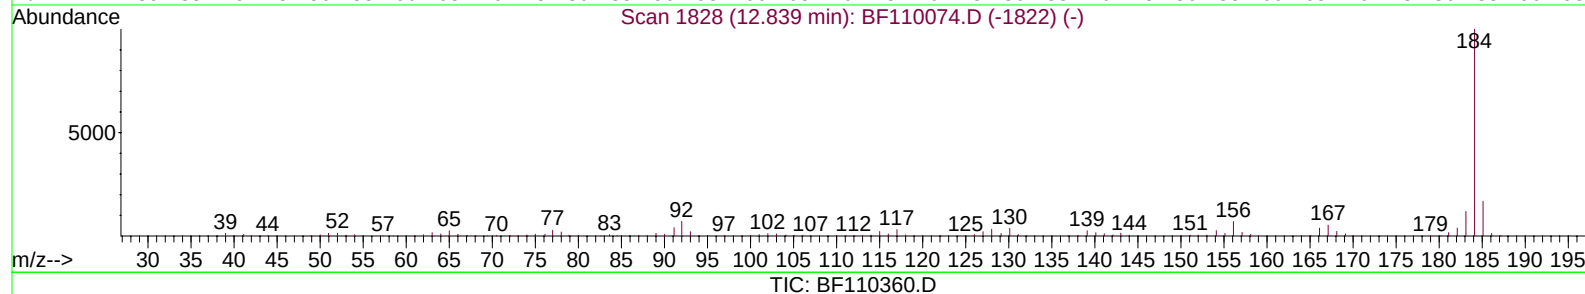
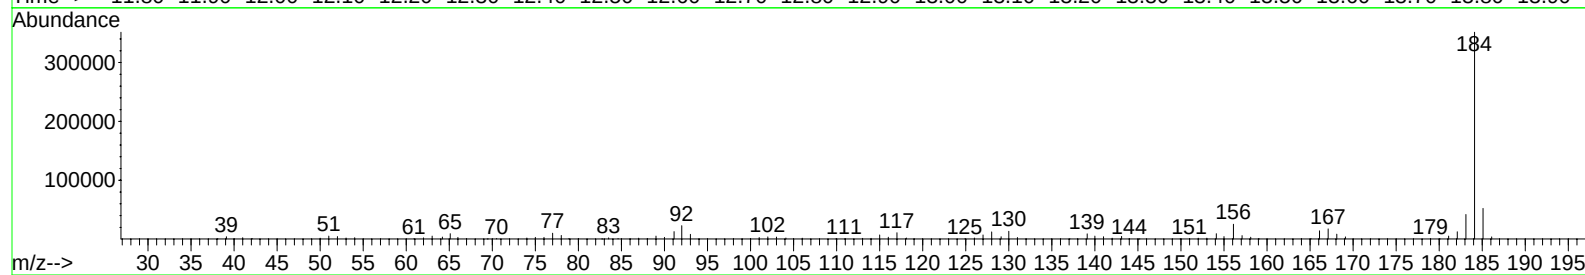


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110118\
 Data File : BF110360.D
 Acq On : 1 Nov 2018 11:10
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 09:46:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 01 16:06:12 2018
 Response via : Initial Calibration

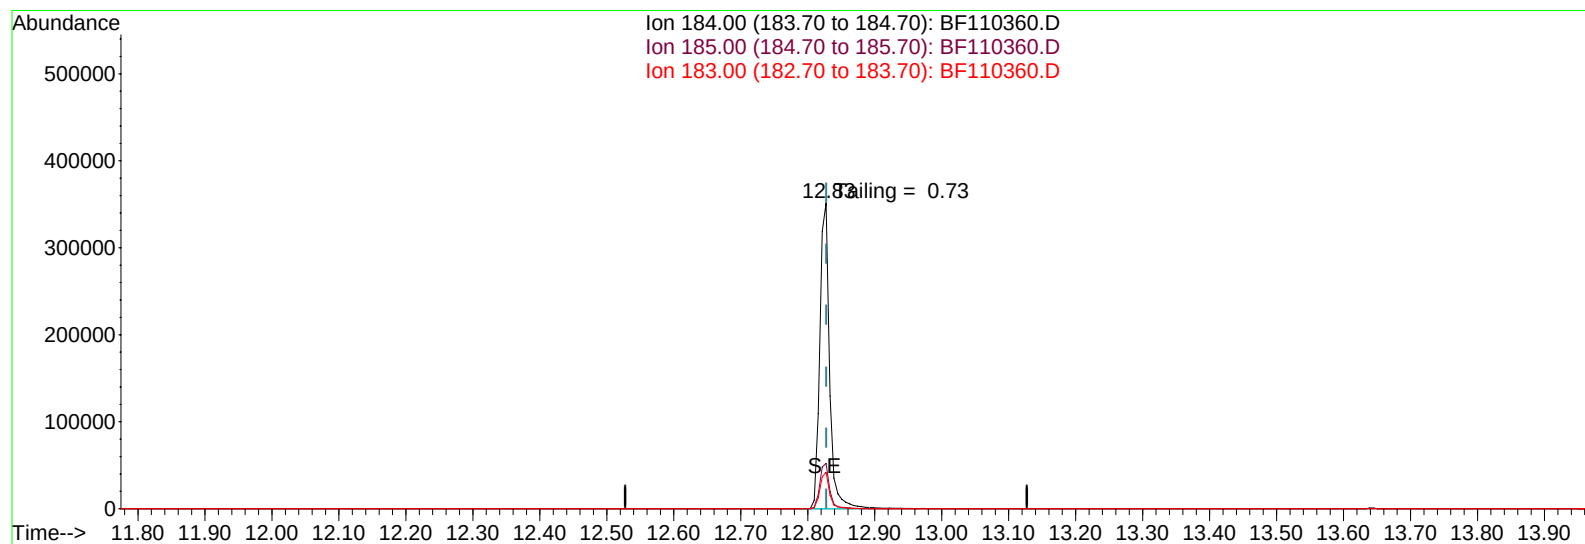

(77) Benzidine




12.827min (+0.000) 0.00ng

response 358149

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.89
183.00	11.80	11.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110118\
 Data File : BF110360.D
 Acq On : 1 Nov 2018 11:10
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 09:46:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 01 16:06:12 2018
 Response via : Initial Calibration

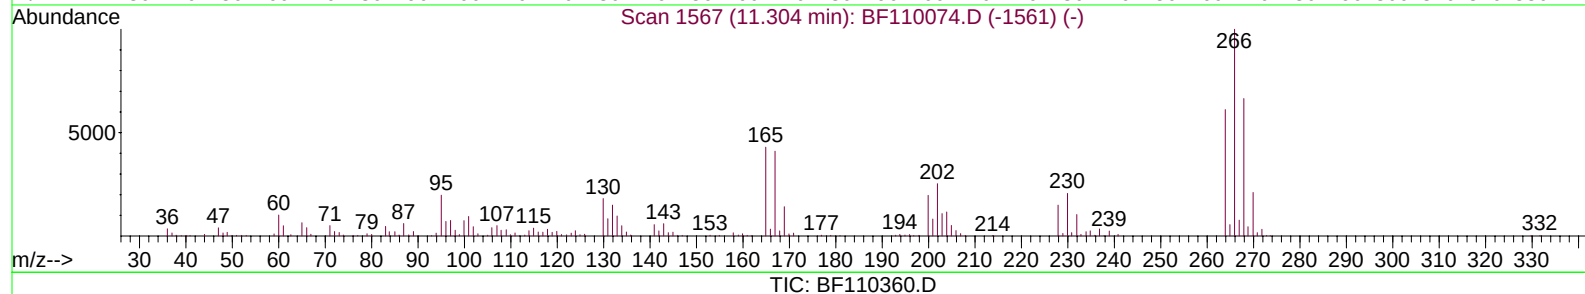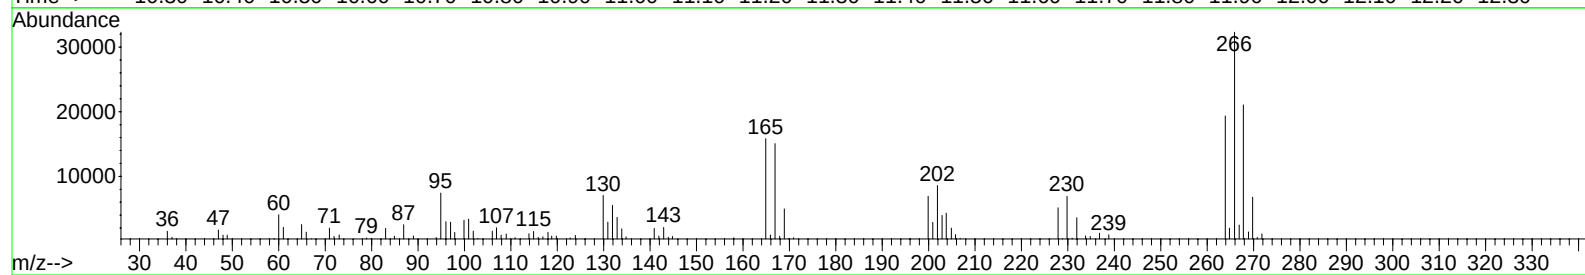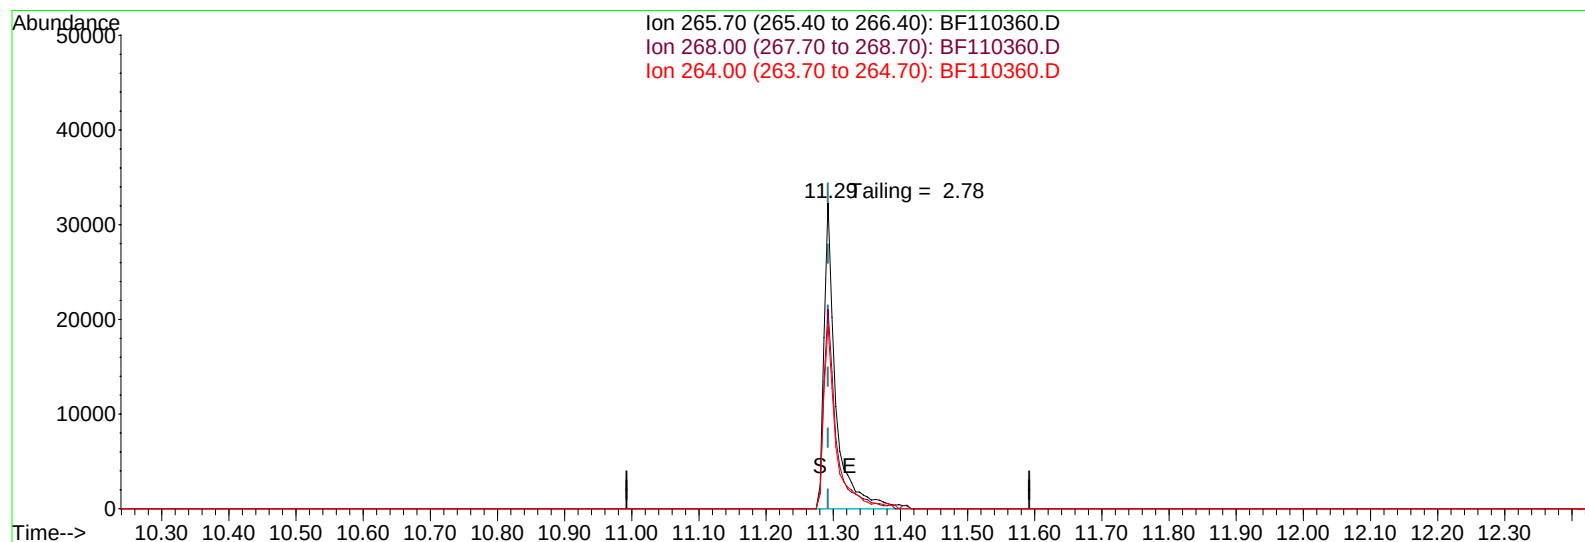

(70) Pentachlorophenol (C)

11.292min (+0.000) 54376.94ng

response 39777

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	65.17
264.00	63.20	59.90
0.00	0.00	0.00