
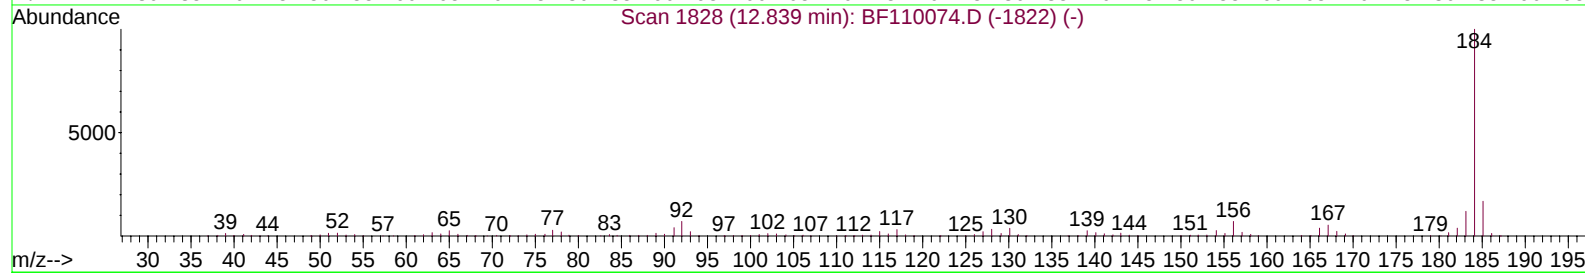
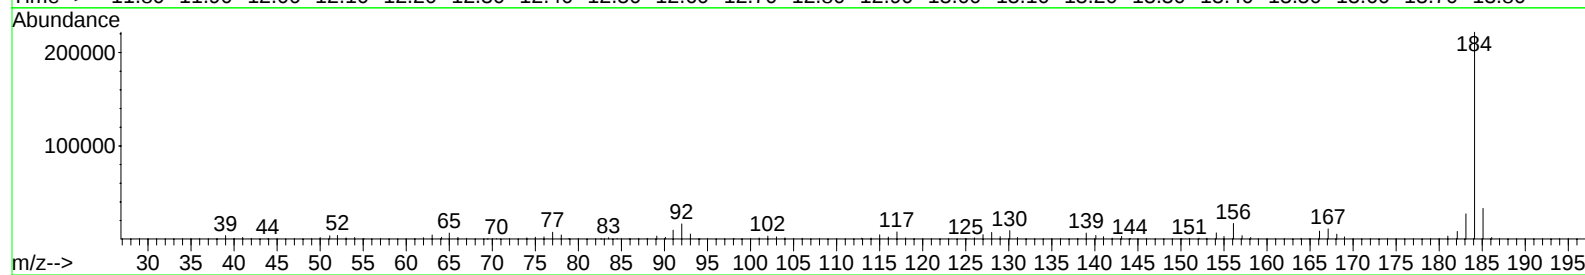


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110118\  
Data File   : BF110385.D  
Acq On      : 2 Nov 2018    1:47  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Nov 02 09:52:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 01 16:06:12 2018
Response via : Initial Calibration

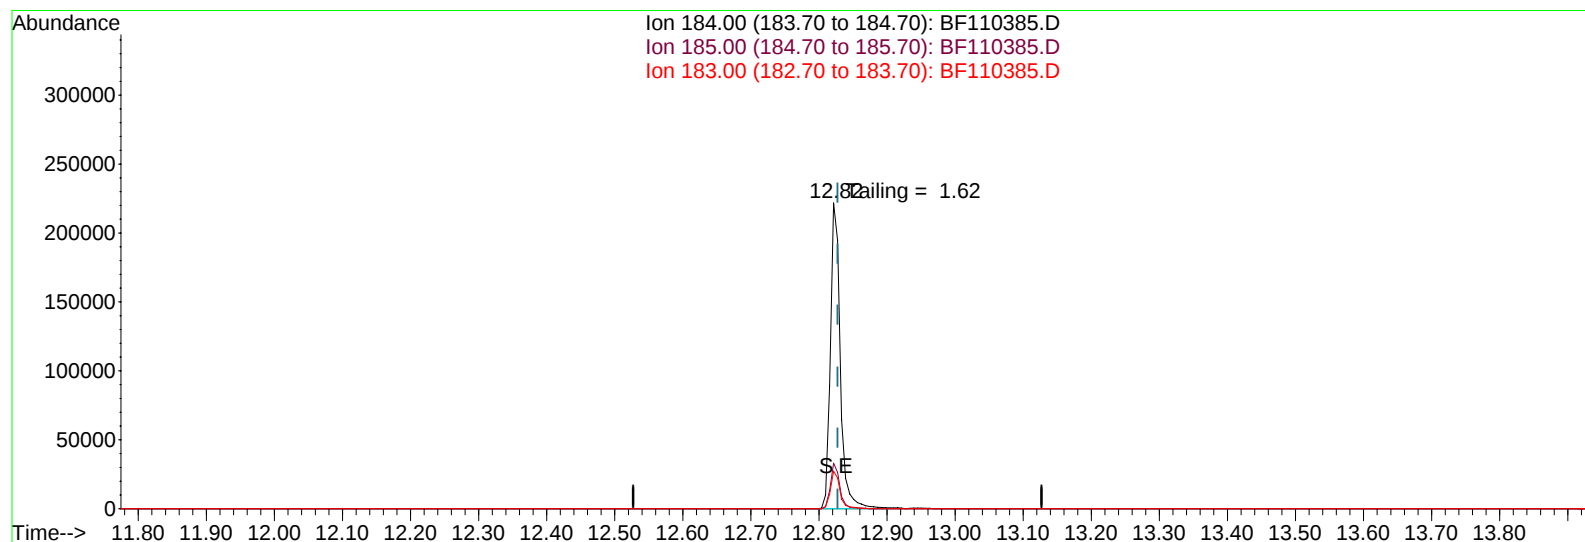

TIC: BF110385.D

(77) Benzidine




12.822min (-0.006) 0.00ng

response 225107

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.92
183.00	11.80	12.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110118\
 Data File : BF110385.D
 Acq On : 2 Nov 2018 1:47
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 09:52:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 01 16:06:12 2018
 Response via : Initial Calibration

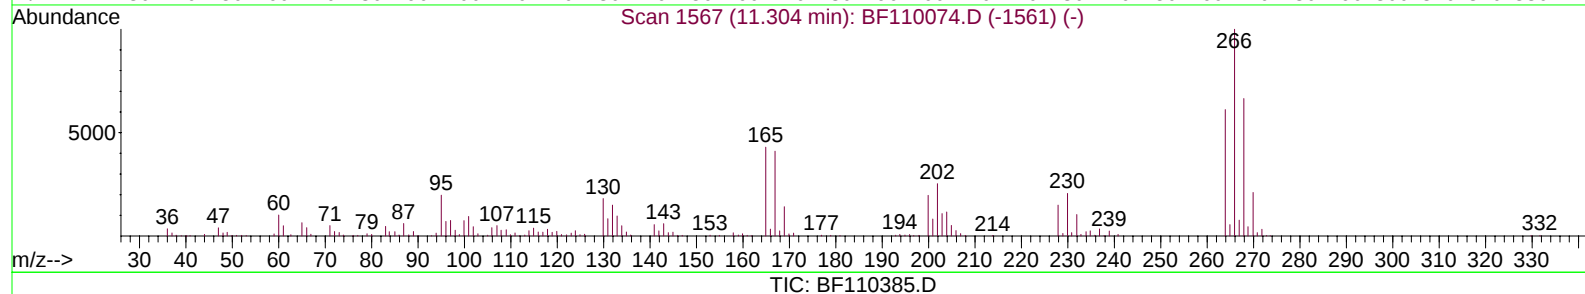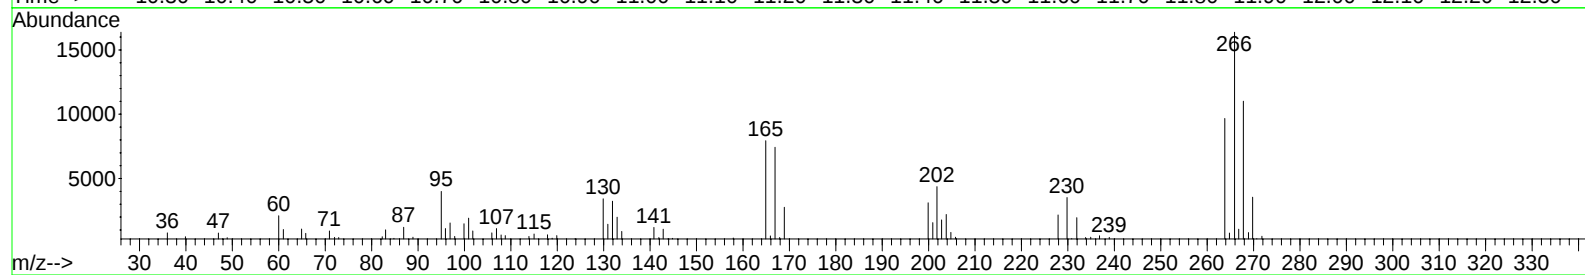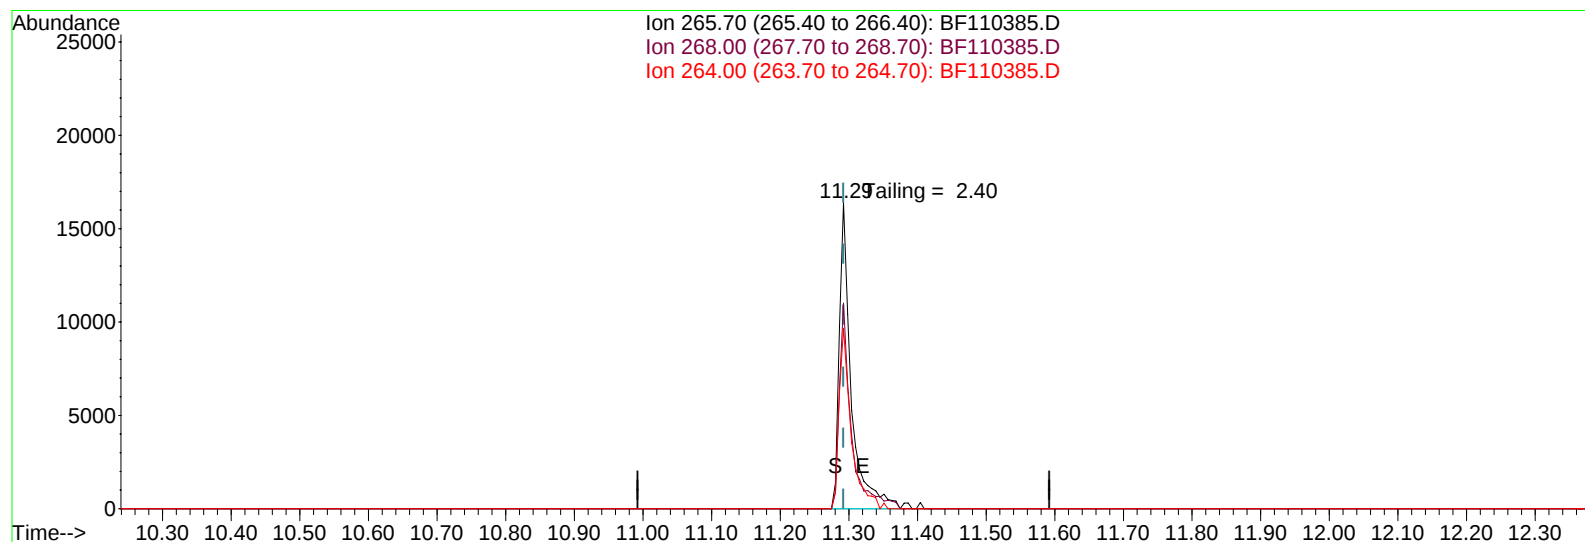

(70) Pentachlorophenol (C)

11.292min (+0.000) 0.00ng

response 19809

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	67.25
264.00	63.20	59.02
0.00	0.00	0.00