


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110118\
 Data File : BF110385.D
 Acq On : 2 Nov 2018 1:47
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 01 16:06:12 2018

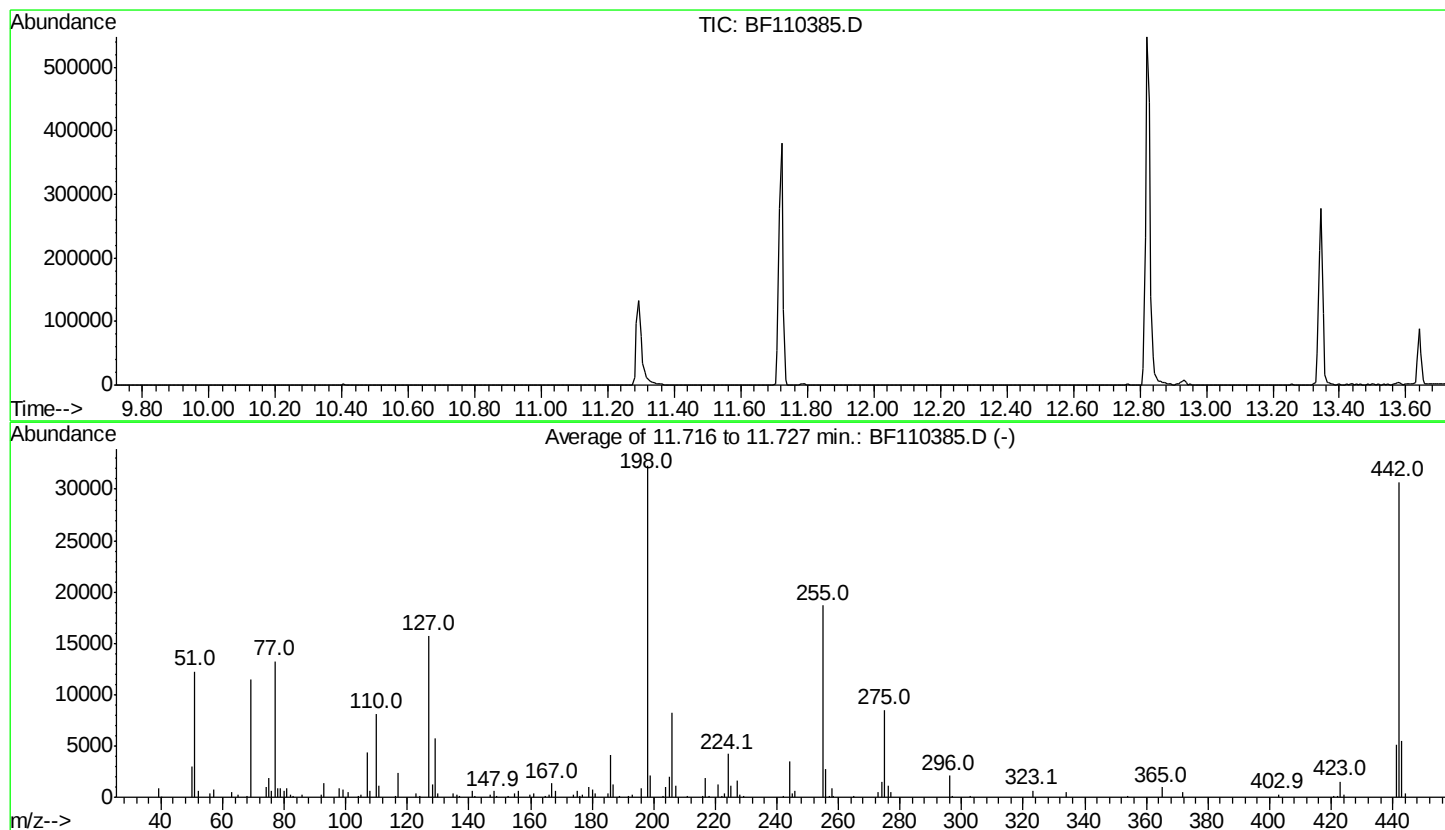

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	12256	PASS
68	69	0.00	2	1.0	120	PASS
69	198	0.00	100	35.5	11456	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.7	15743	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	32309	PASS
199	198	5	9	6.6	2140	PASS
275	198	10	60	26.4	8523	PASS
365	198	1	100	3.0	976	PASS
441	198	0.01	100	15.8	5103	PASS
442	198	50	100	95.2	30744	PASS
443	442	15	24	17.9	5490	PASS