
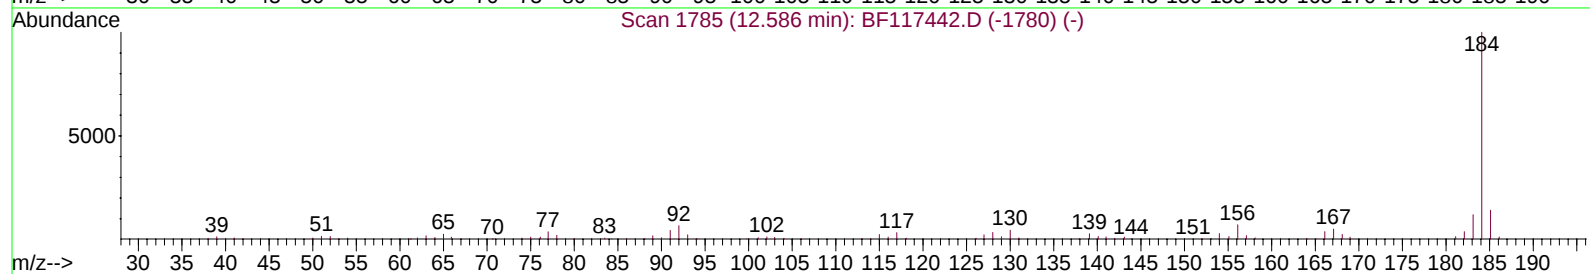
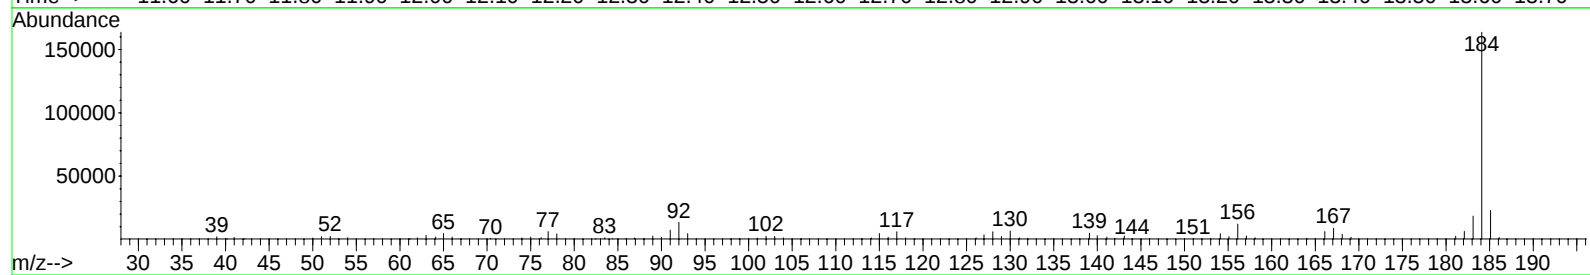


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110119\
 Data File : BF117674.D
 Acq On : 1 Nov 2019 11:21
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 18:18:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 18 18:53:31 2019
 Response via : Initial Calibration

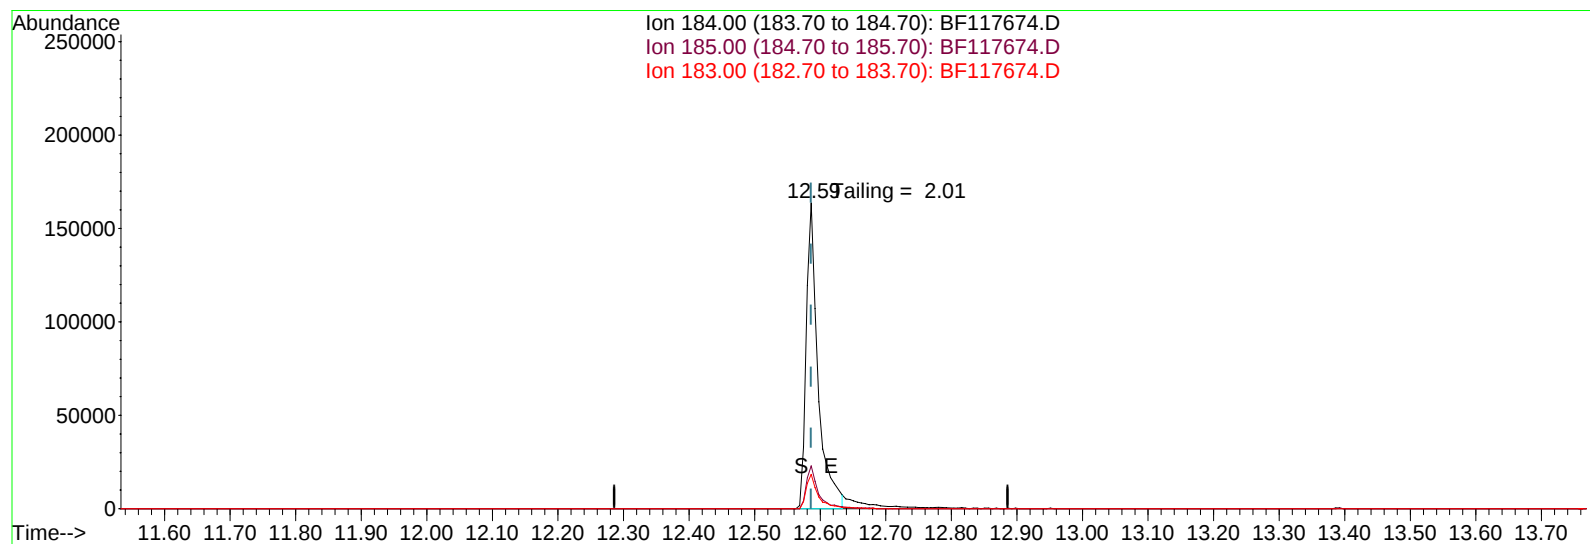

TIC: BF117674.D

(77) Benzidine




12.586min (+0.000) 0.00ng

response 222167

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.01
183.00	12.00	11.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110119\
Data File : BF117674.D
Acq On : 1 Nov 2019 11:21
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 18:18:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 18:53:31 2019
Response via : Initial Calibration

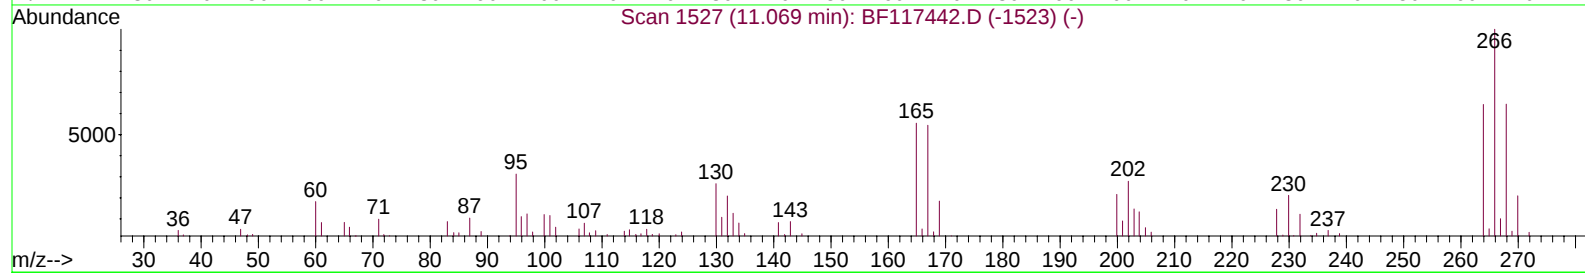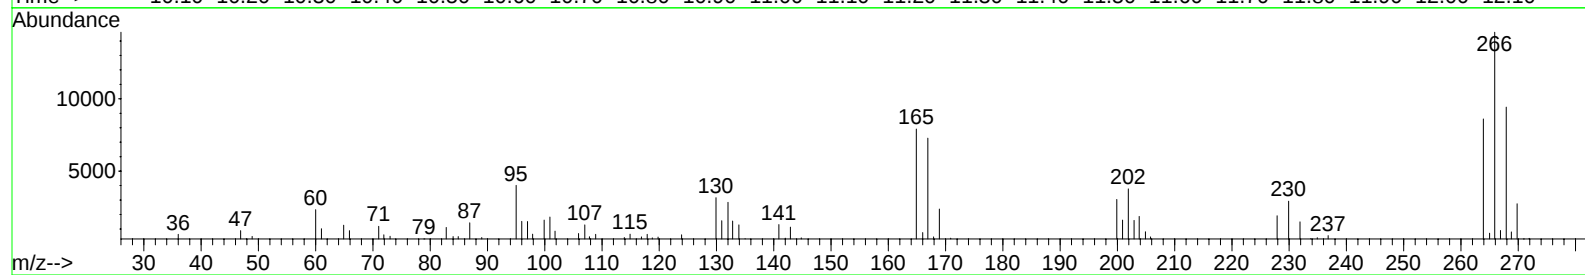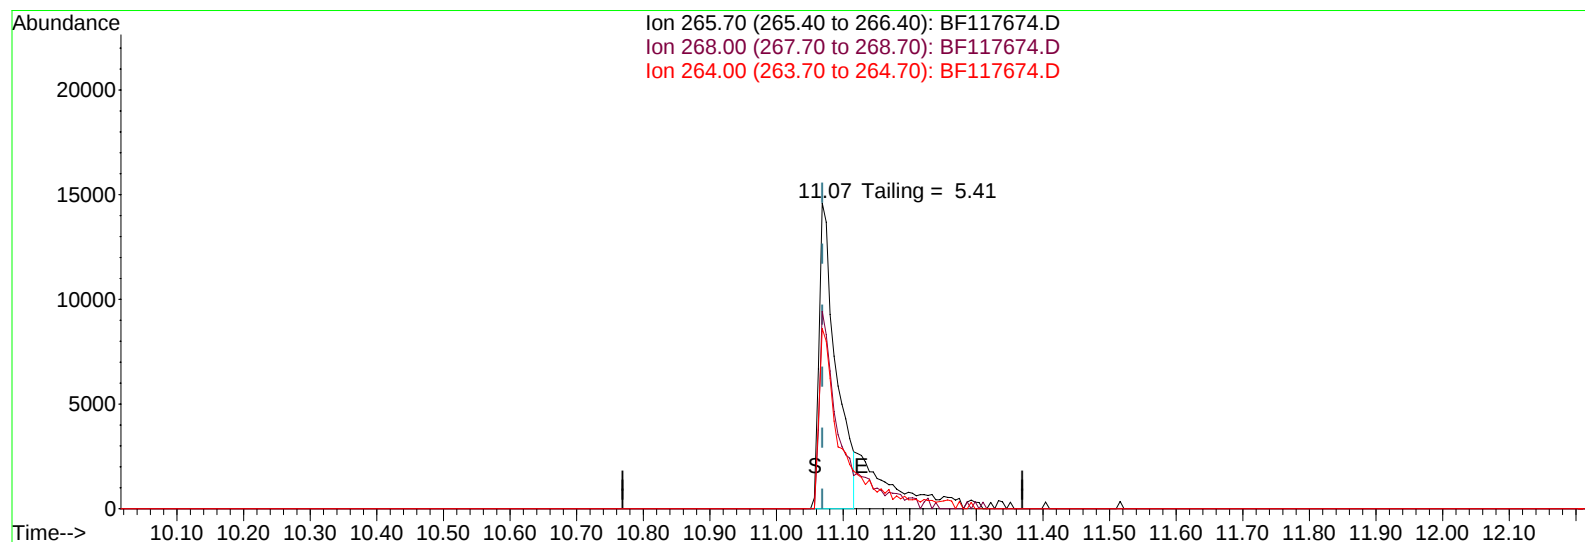

TIC: BF117674.D

(70) Pentachlorophenol (C)

11.069min (+0.000) 0.00ng

response 33844

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	64.58
264.00	64.30	58.92
0.00	0.00	0.00