


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110119\
 Data File : BF117674.D
 Acq On : 1 Nov 2019 11:21
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 18 18:53:31 2019

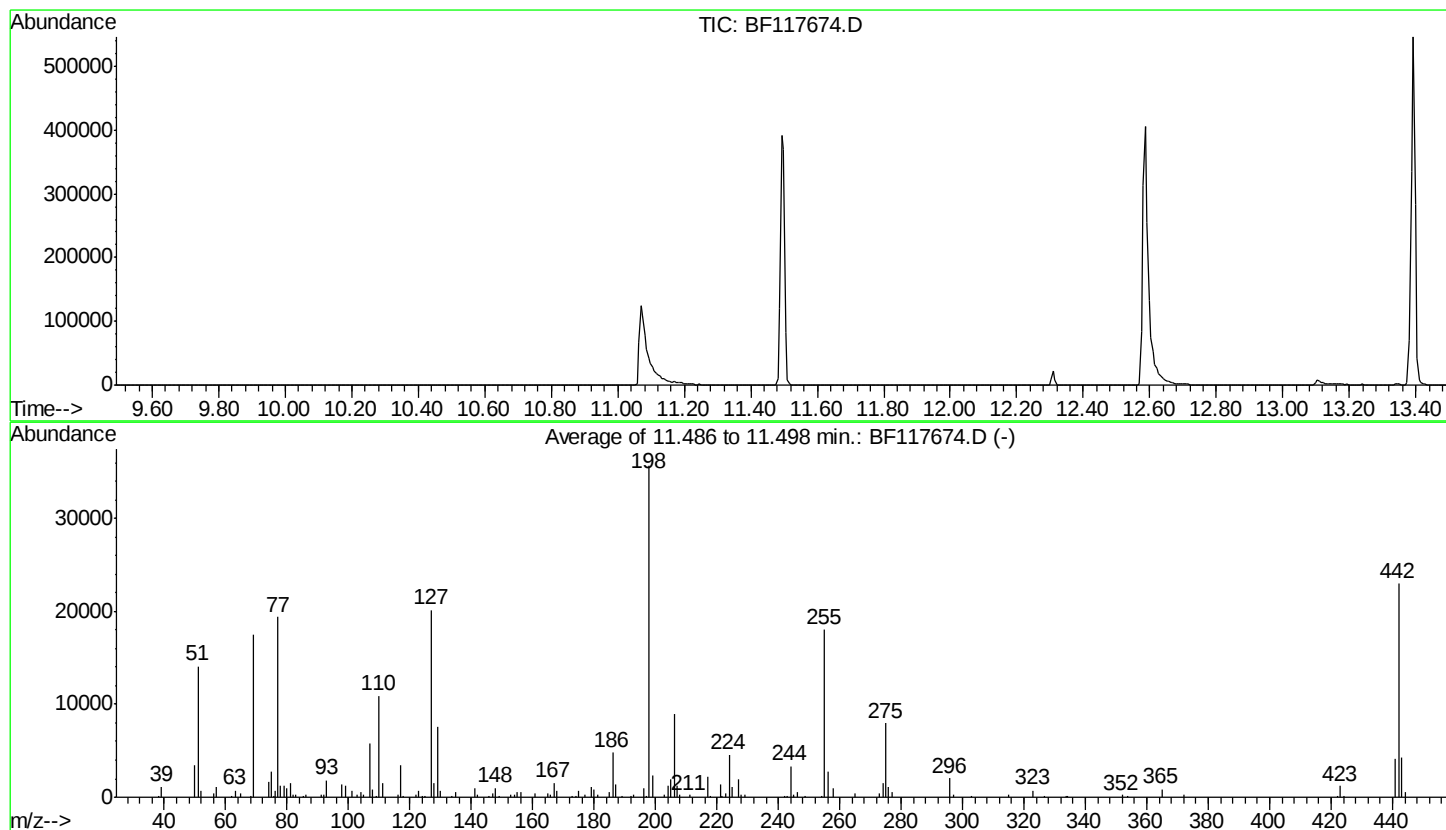

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	14125	PASS
68	69	0.00	2	1.0	170	PASS
69	198	0.00	100	49.0	17498	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.4	20130	PASS
197	198	0.00	2	0.3	105	PASS
198	198	100	100	100.0	35697	PASS
199	198	5	9	6.6	2361	PASS
275	198	10	60	22.3	7970	PASS
365	198	1	100	2.5	888	PASS
441	198	0.01	100	11.4	4081	PASS
442	198	50	100	64.4	22976	PASS
443	442	15	24	18.5	4242	PASS