
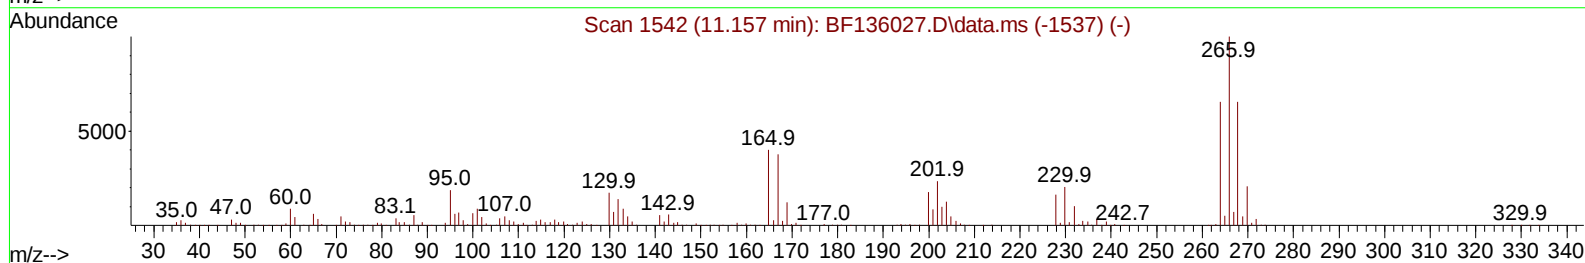
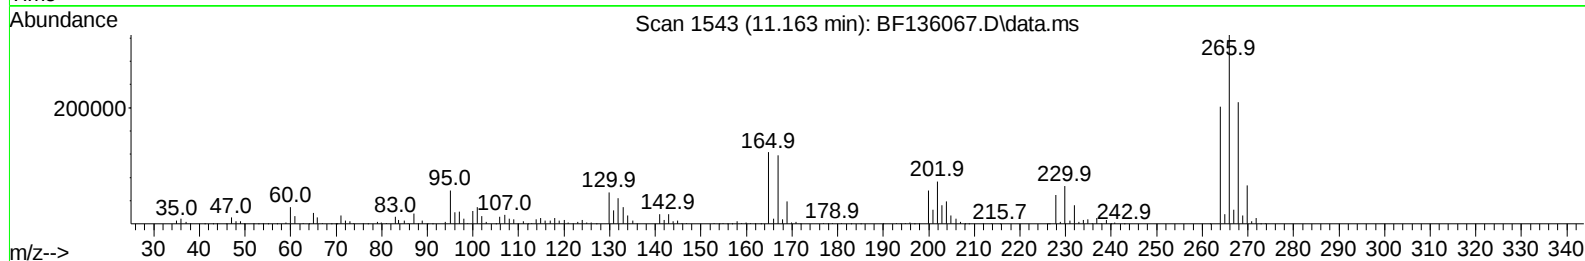


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF110123\  
Data File : BF136067.D  
Acq On : 01 Nov 2023 10:19  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 11:31:53 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF103023.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Oct 31 01:13:02 2023  
Response via : Initial Calibration

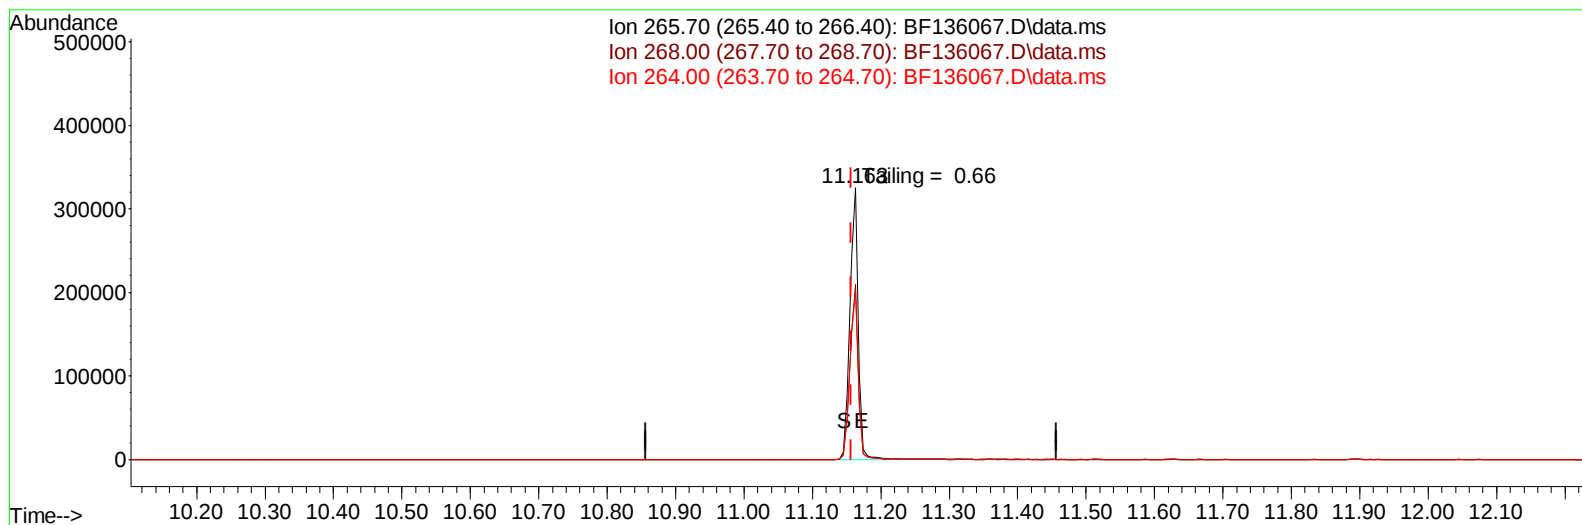




TIC: BF136067.D\data.ms

**(70) Pentachlorophenol (C)****11.163min (+ 0.006) 316136.19 ng****response 277355**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.30  | 64.48  |
| 264.00 | 65.30  | 61.98  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF110123\  
Data File : BF136067.D  
Acq On : 01 Nov 2023 10:19  
Operator : CG\JU  
Sample : DFTTP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 11:31:53 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF103023.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Oct 31 01:13:02 2023  
Response via : Initial Calibration

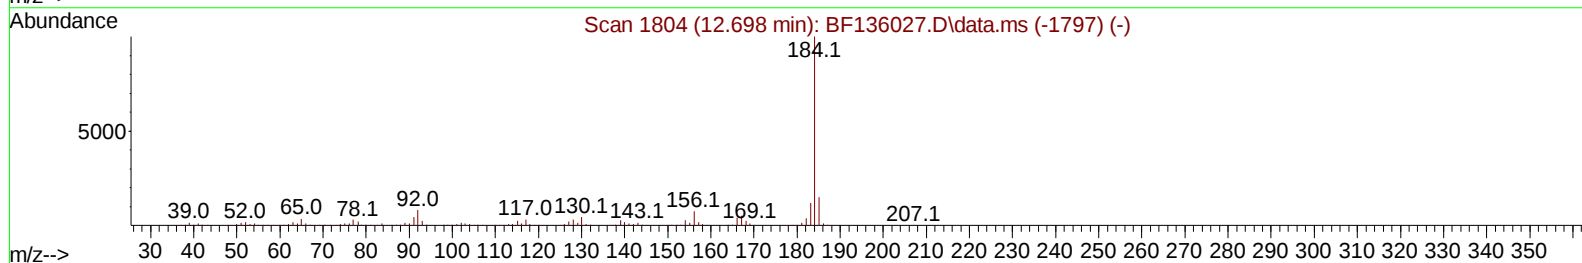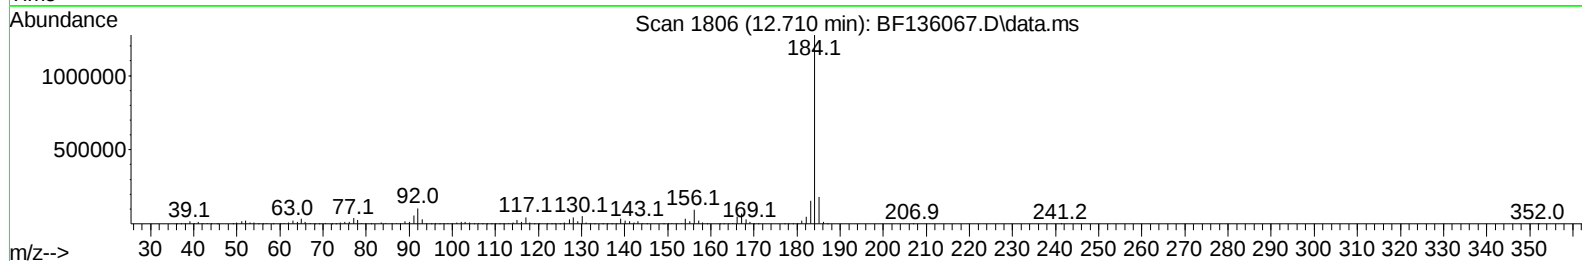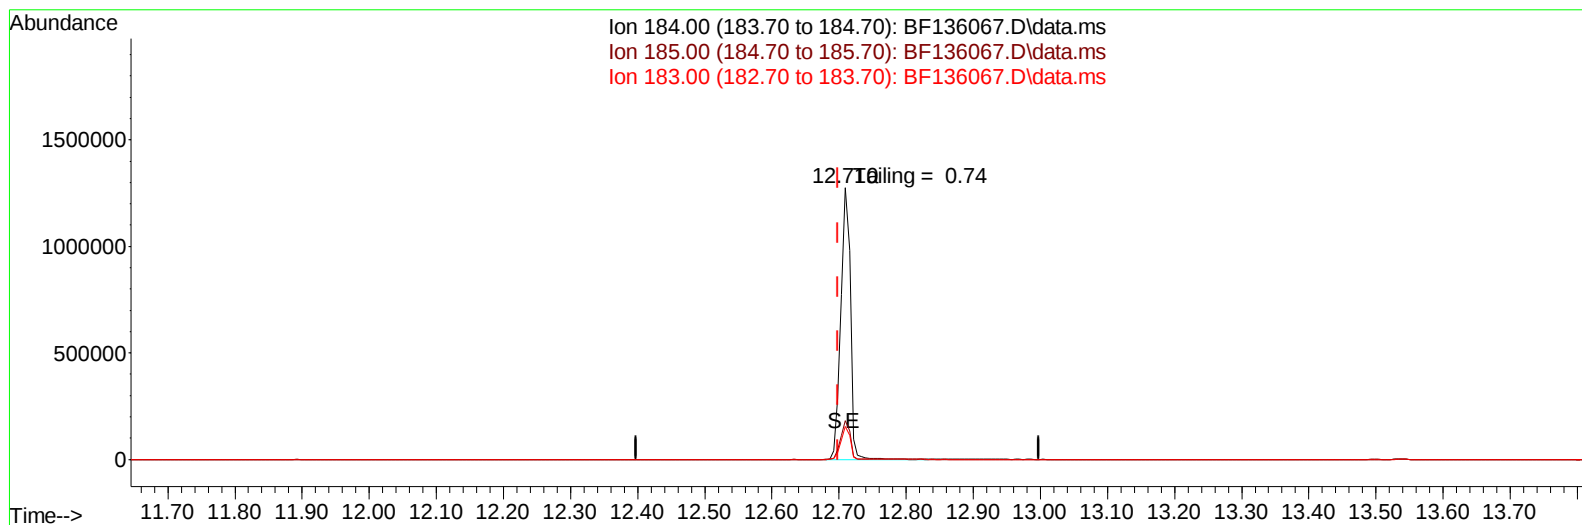

TIC: BF136067.D\data.ms

**(77) Benzidine****12.710min (+ 0.012) 128544.59 ng****response 1245204**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.80  | 14.33  |
| 183.00 | 11.90  | 12.11  |
| 0.00   | 0.00   | 0.00   |