


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110123\
 Data File : BF136067.D
 Acq On : 01 Nov 2023 10:19
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 31 01:13:02 2023

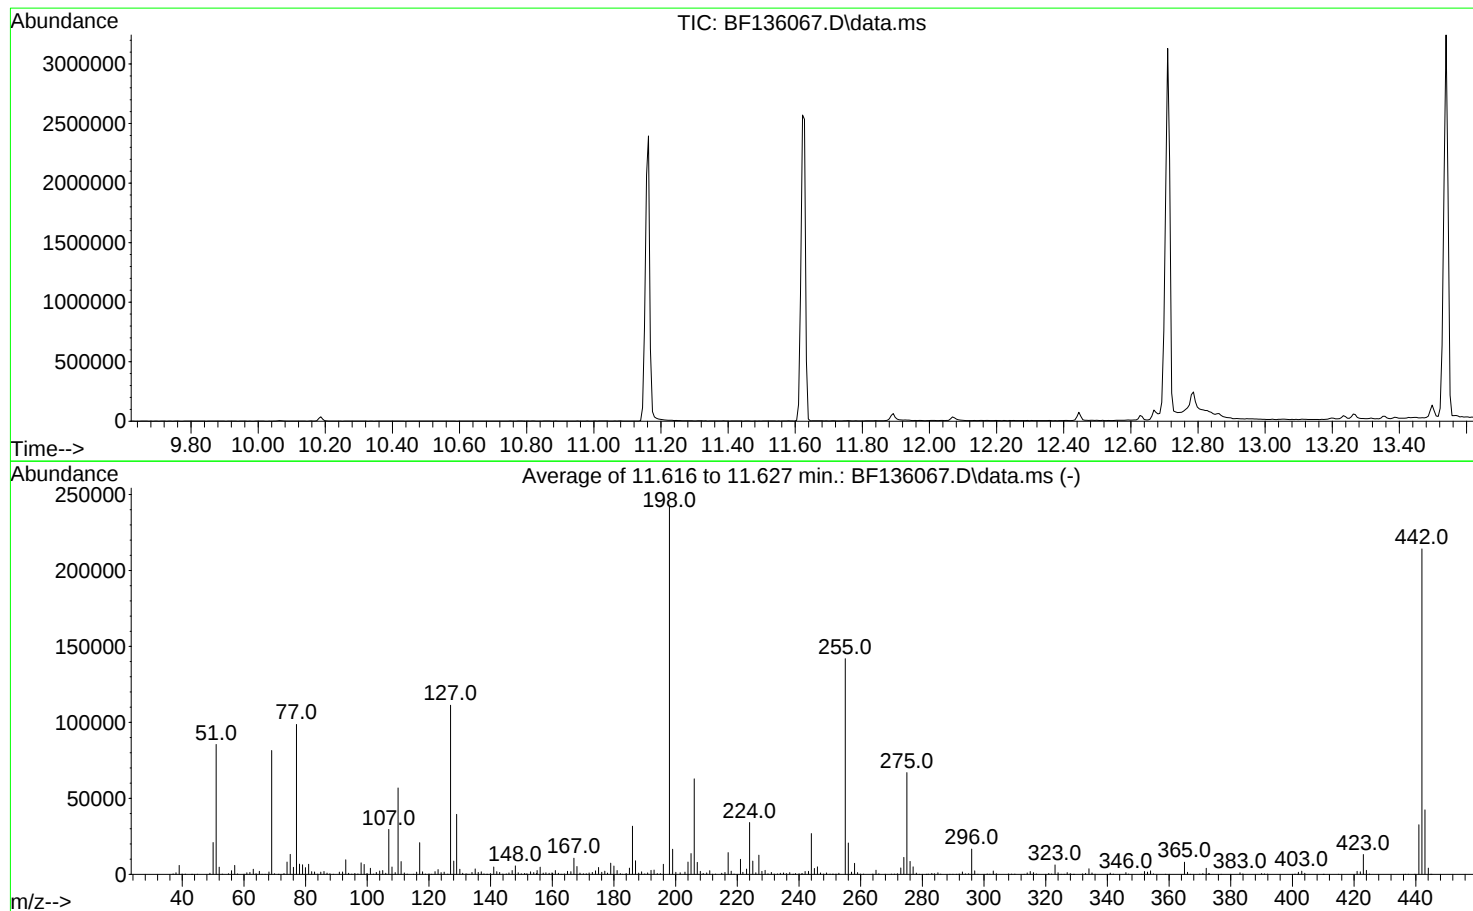




AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	85469	PASS
68	69	0.00	2	1.9	1586	PASS
69	198	0.00	100	33.7	81469	PASS
70	69	0.00	2	0.5	423	PASS
127	198	10	80	46.0	111328	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	242080	PASS
199	198	5	9	6.8	16490	PASS
275	198	10	60	27.7	66979	PASS
365	198	1	100	3.3	8037	PASS
441	198	0.01	100	13.5	32616	PASS
442	442	50	100	100.0	214211	PASS
443	442	15	24	19.8	42421	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110123\
Data File : BF136067.D
Acq On : 01 Nov 2023 10:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 01 11:31:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 01:13:02 2023
Response via : Initial Calibration

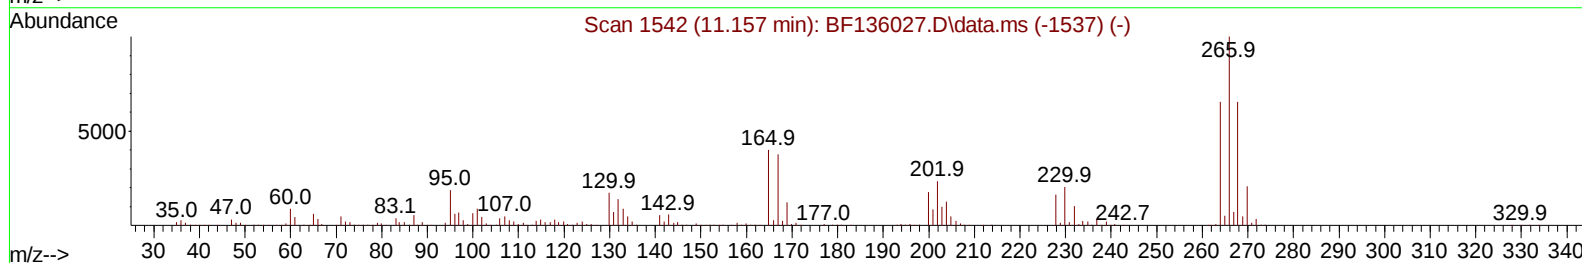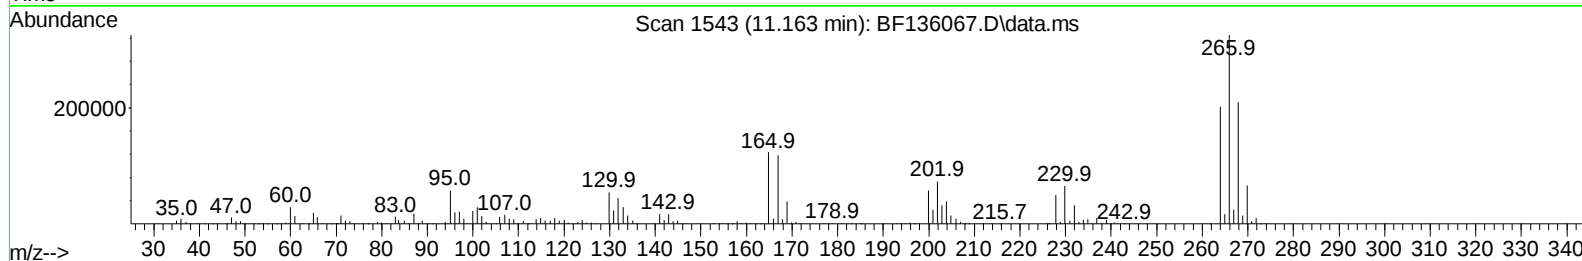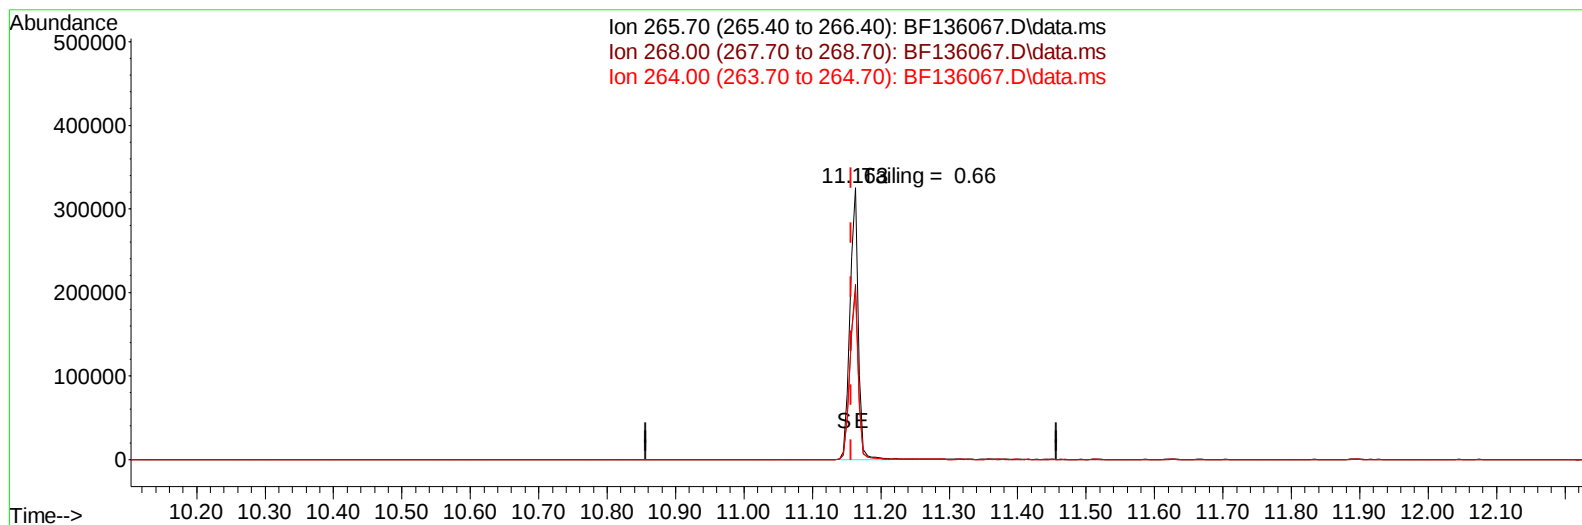

TIC: BF136067.D\data.ms

(70) Pentachlorophenol (C)

11.163min (+ 0.006) 316136.19 ng




response 277355

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.48
264.00	65.30	61.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110123\
 Data File : BF136067.D
 Acq On : 01 Nov 2023 10:19
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 01 11:31:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 31 01:13:02 2023
 Response via : Initial Calibration

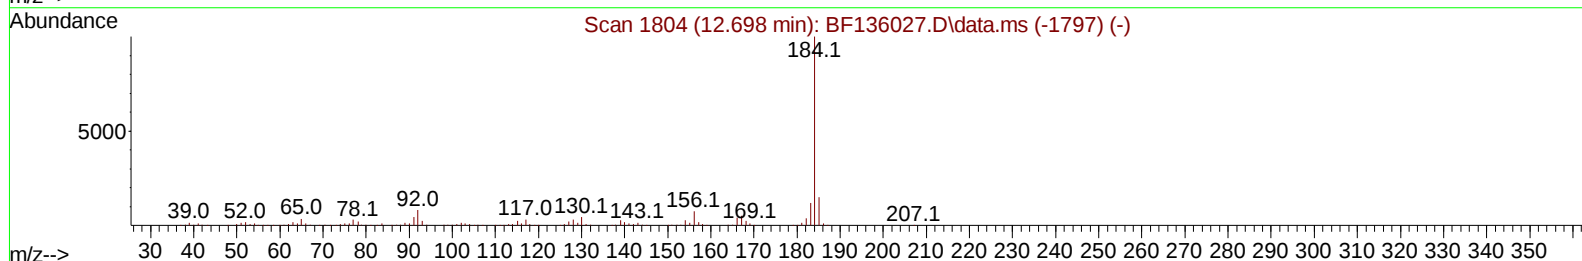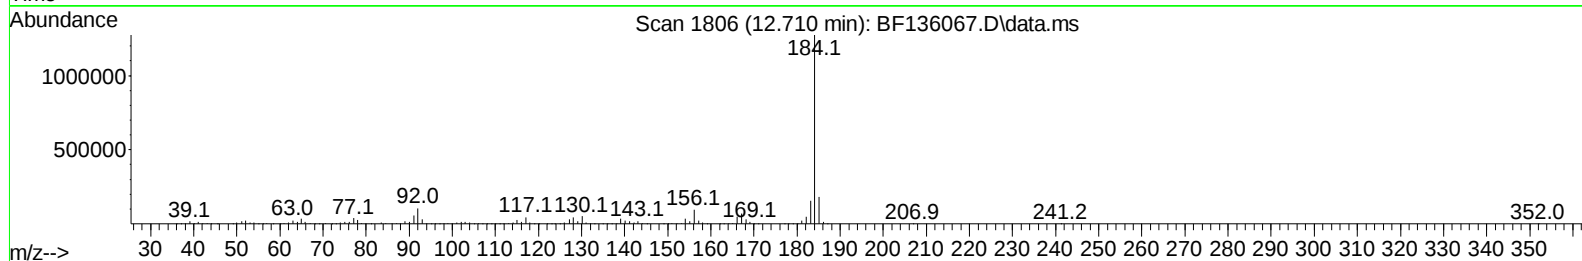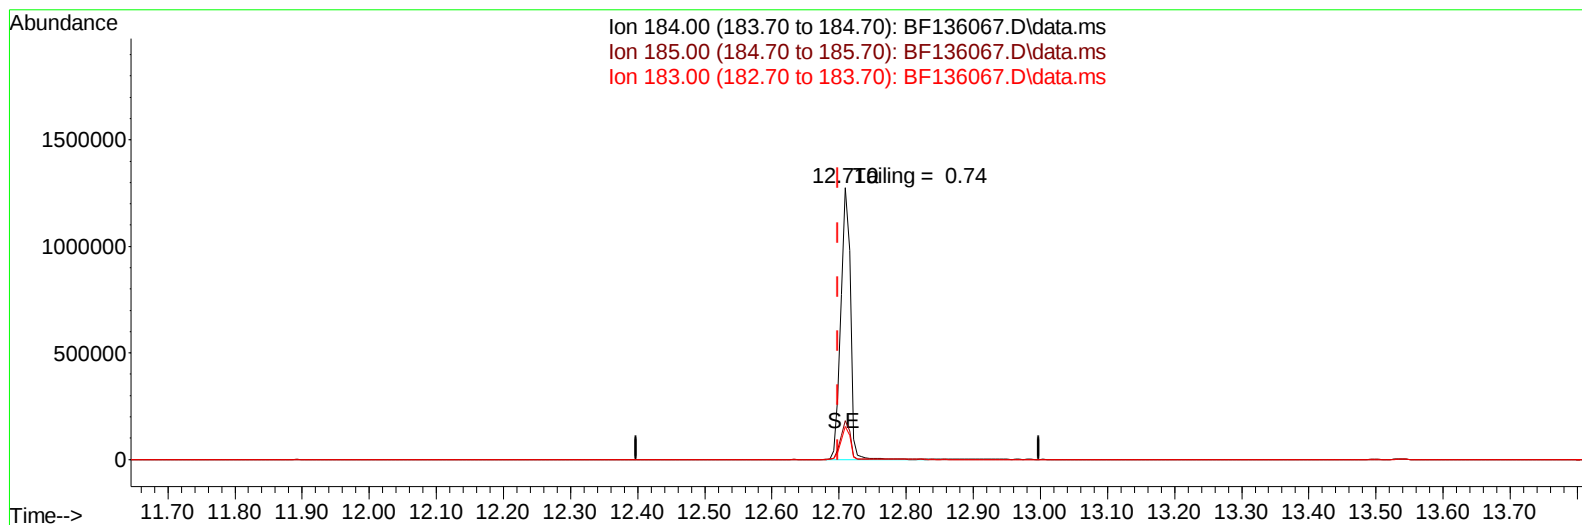

TIC: BF136067.D\data.ms

(77) Benzidine

12.710min (+ 0.012) 128544.59 ng

response 1245204

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.33
183.00	11.90	12.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/1/2023	BNA_F	<u>BF136067.D</u>
Compound Name	Response	Retention Time
DDT	580535	13.539
DDD	10275	13.268
DDE	466	12.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10741	591276	1.82

Instrument :
BNA_F
ClientSampleId :
DFTPP