
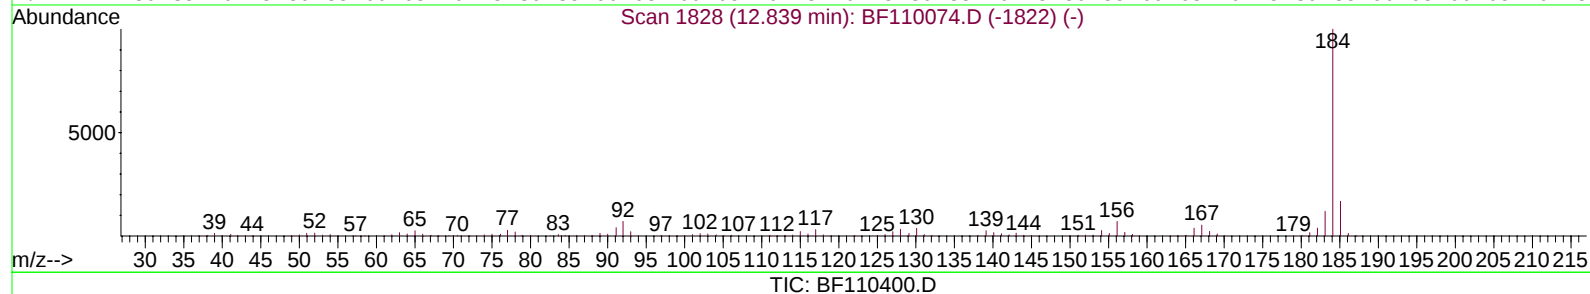
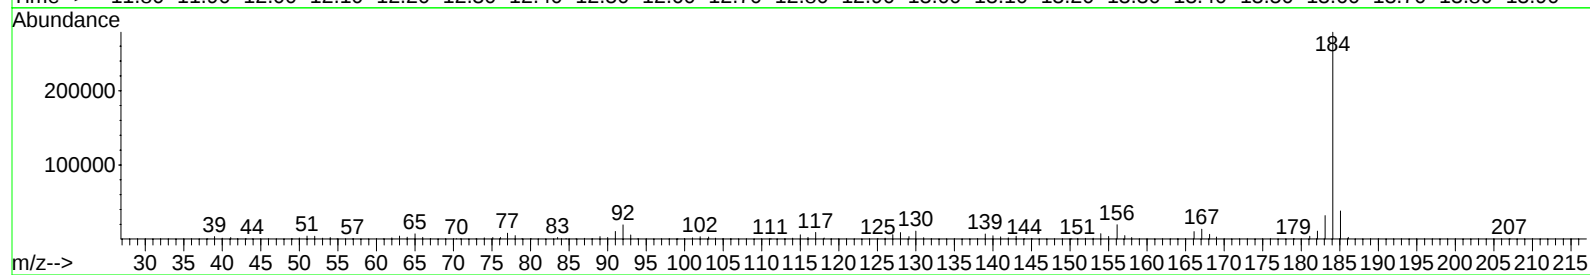


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110218\
Data File : BF110400.D
Acq On : 2 Nov 2018 9:15
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 05:35:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 01 16:06:12 2018
Response via : Initial Calibration

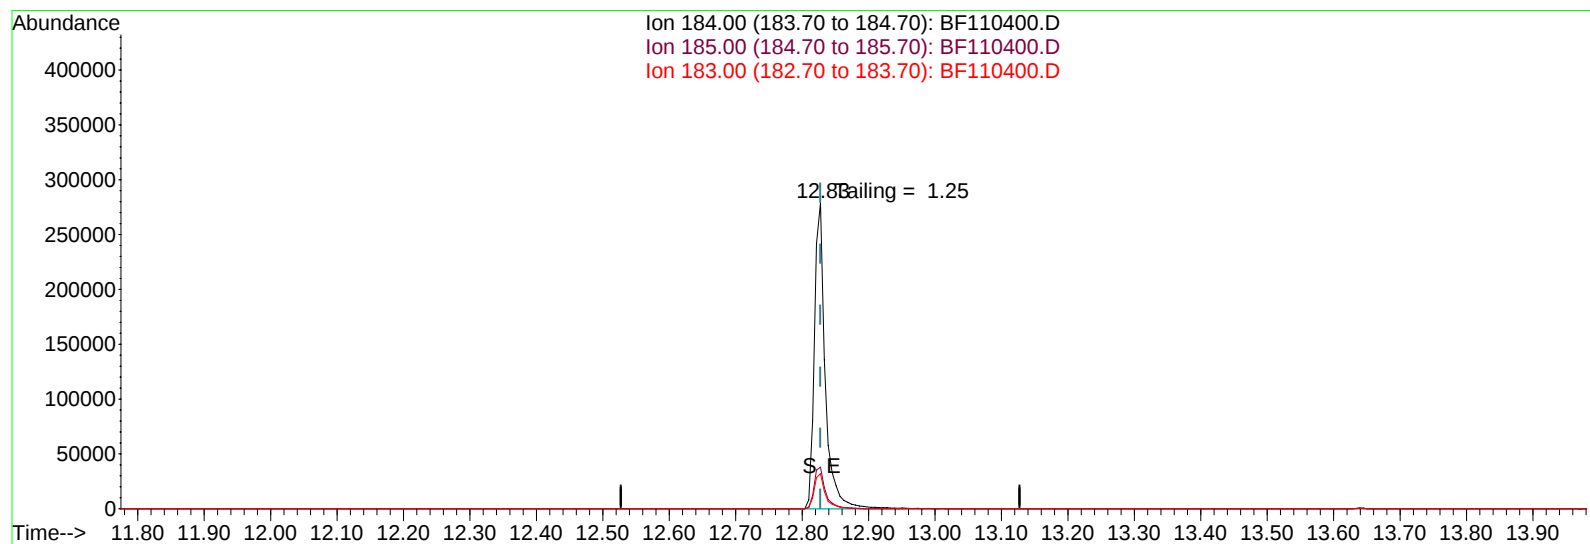

(77) Benzidine




12.827min (+0.000) 0.00ng

response 319129

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	13.63
183.00	11.80	11.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110218\
Data File : BF110400.D
Acq On : 2 Nov 2018 9:15
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 05:35:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 01 16:06:12 2018
Response via : Initial Calibration

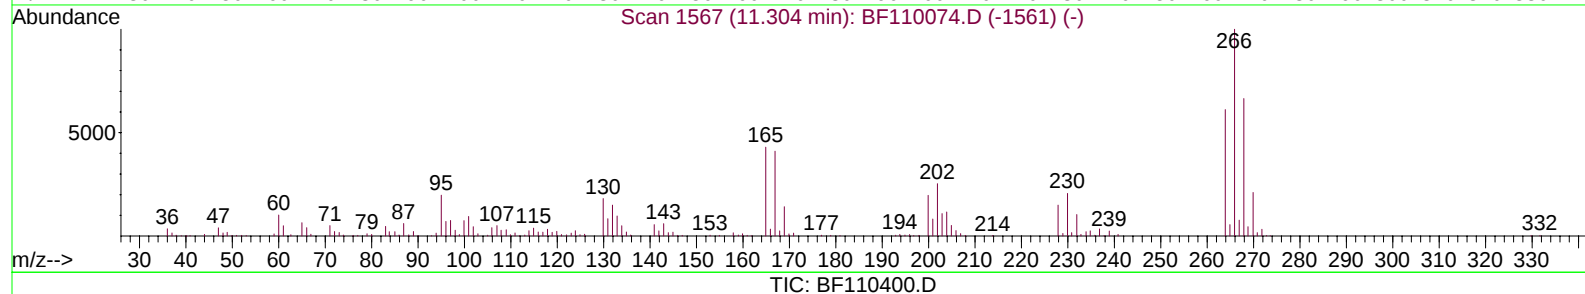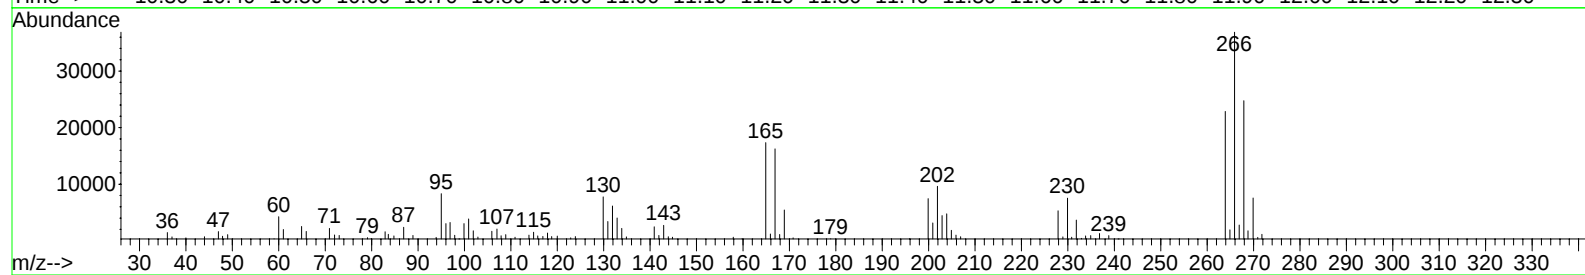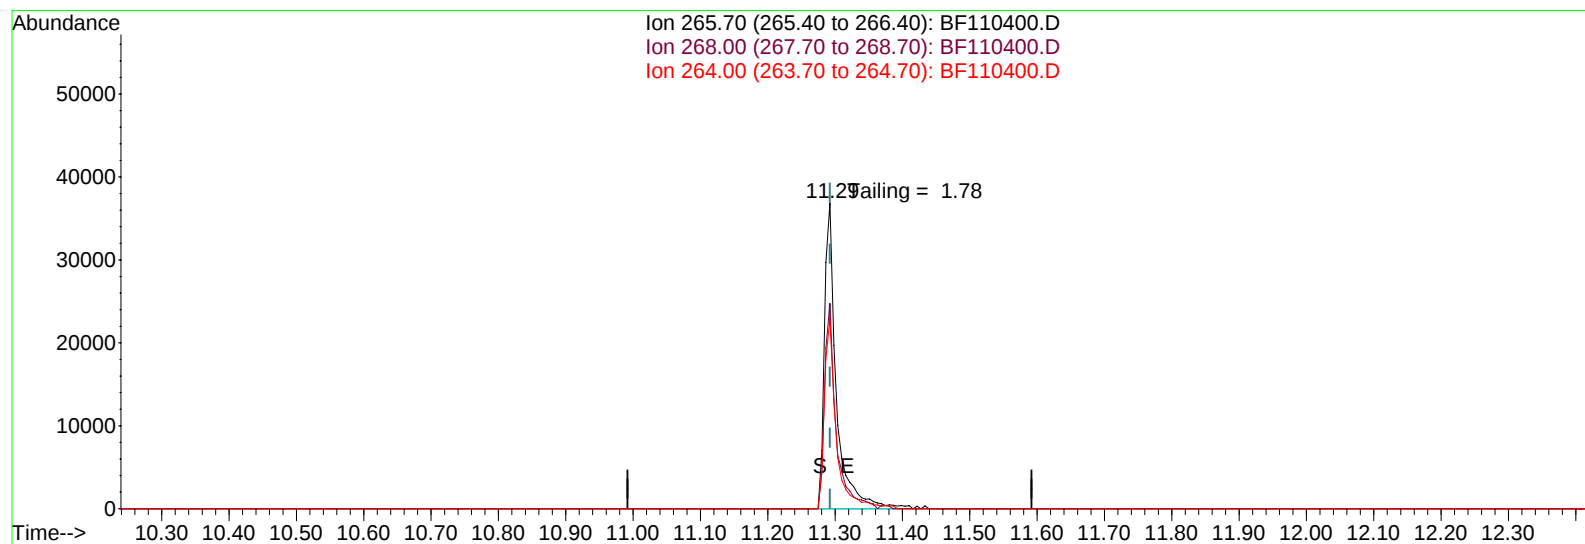

(70) Pentachlorophenol (C)

11.292min (+0.000) 52852.75ng

response 45756

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	67.12
264.00	63.20	62.04
0.00	0.00	0.00