
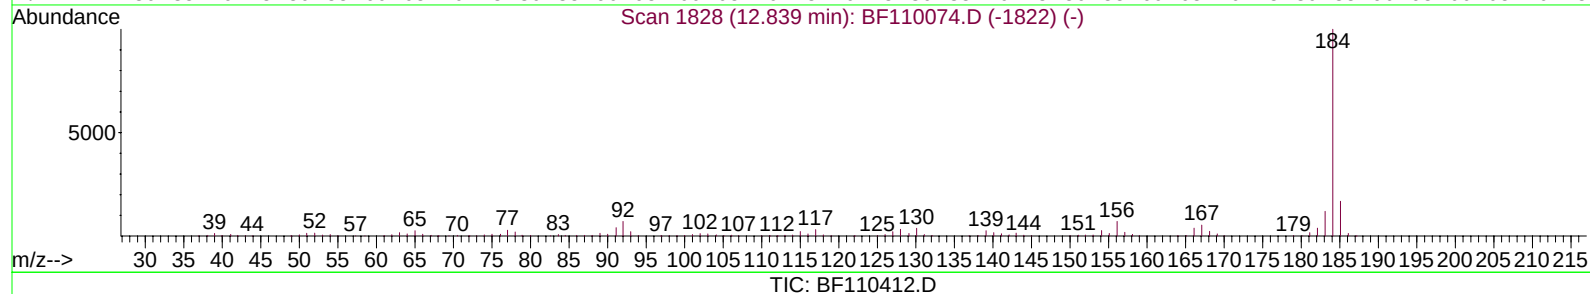
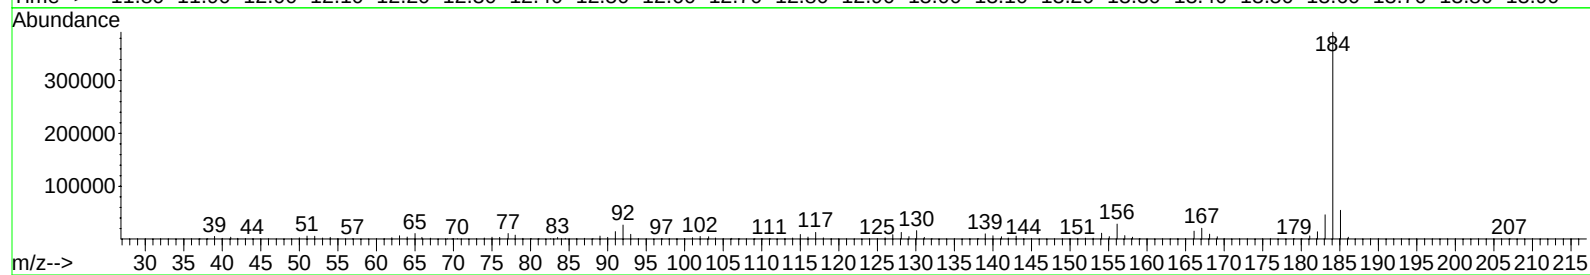


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110218\
 Data File : BF110412.D
 Acq On : 2 Nov 2018 15:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 05:41:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 01 16:06:12 2018
 Response via : Initial Calibration

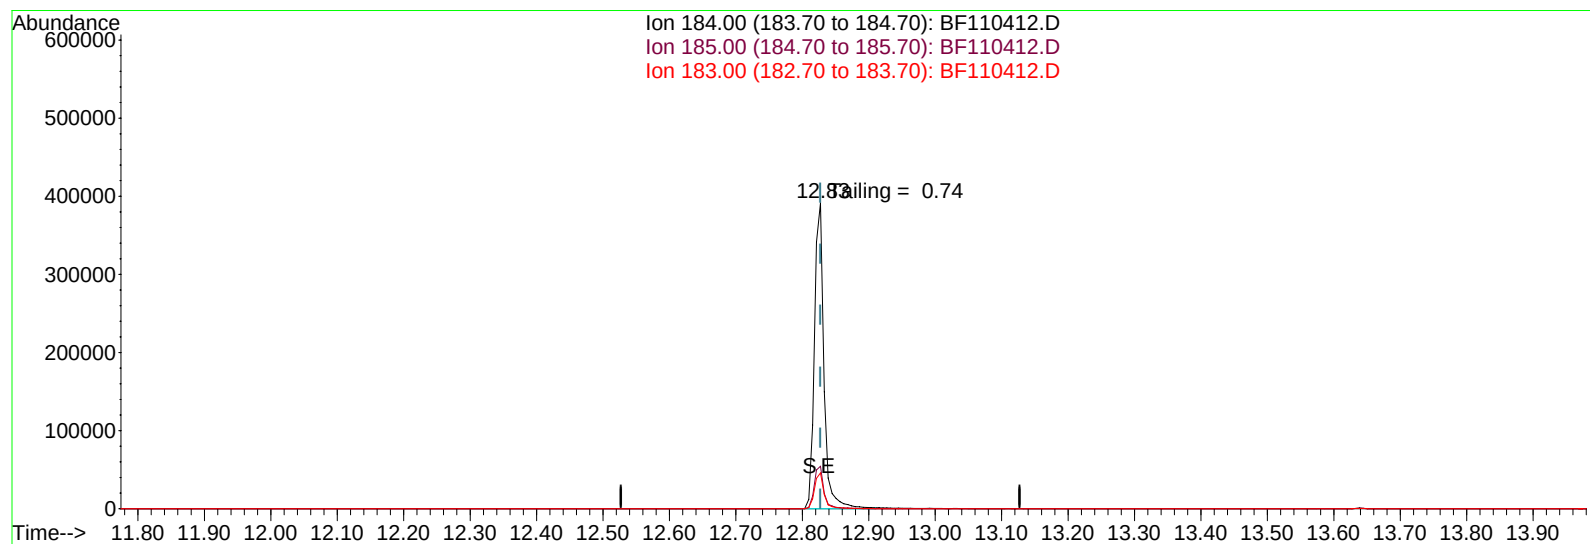

(77) Benzidine




12.827min (0.000) 0.00ng

response 394784

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	13.90
183.00	11.80	11.74
0.00	0.00	0.00

```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110218\  
Data File   : BF110412.D  
Acq On      : 2 Nov 2018 15:23  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Nov 03 05:41:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 01 16:06:12 2018
Response via : Initial Calibration

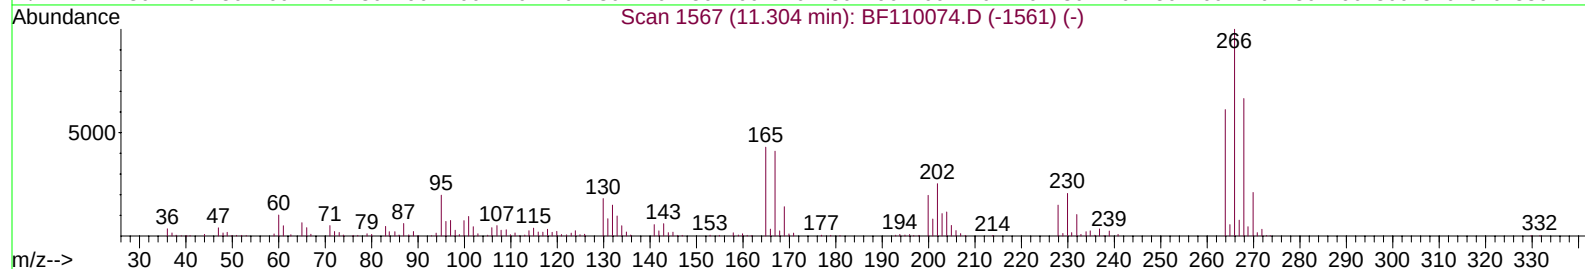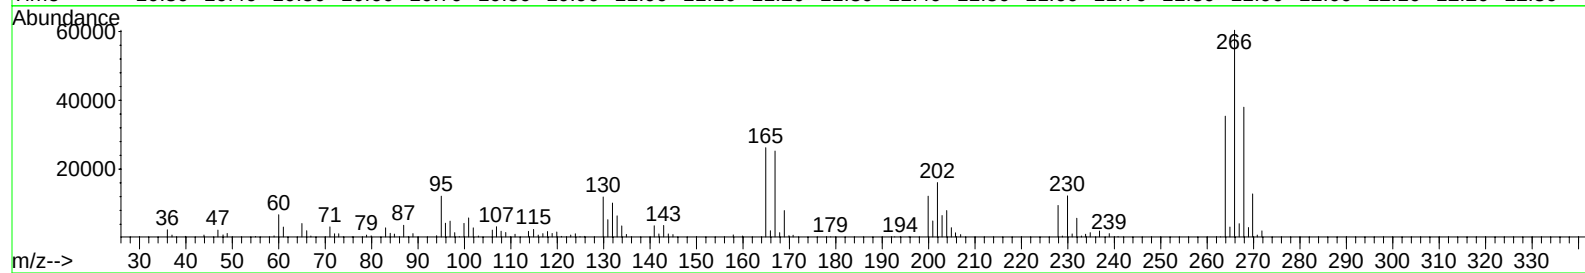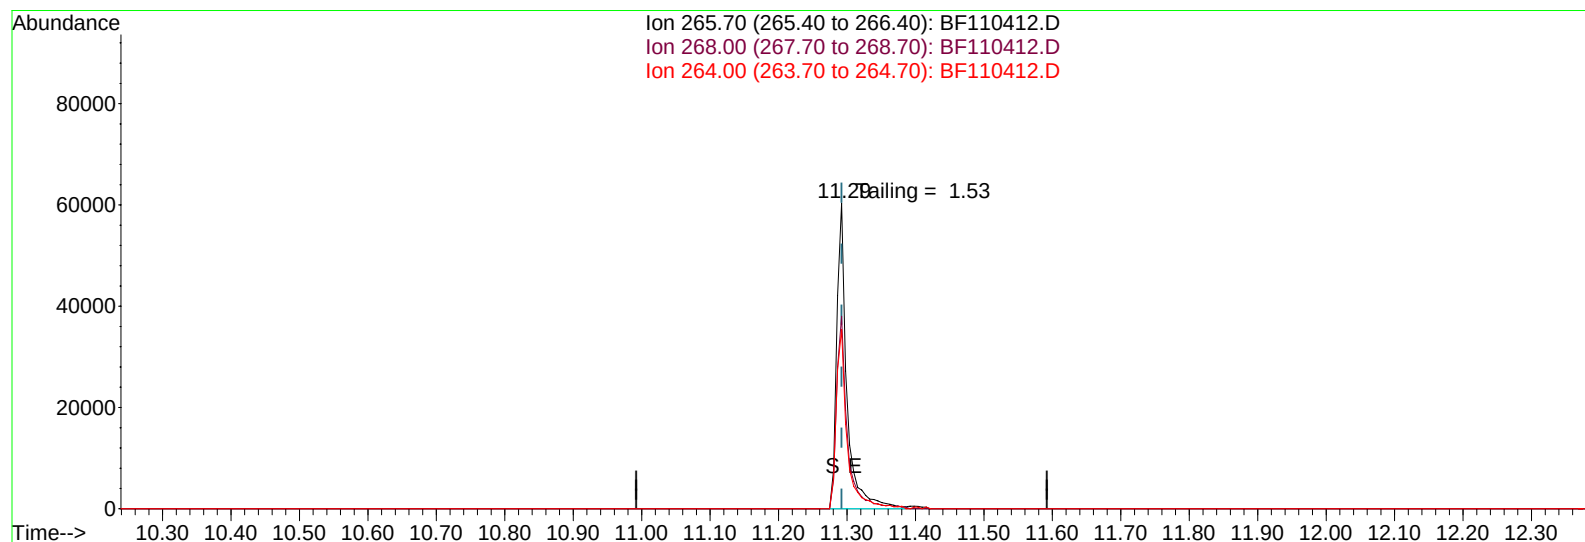

(70) Pentachlorophenol (C)

11.292min (+0.000) 38295.64ng

response 62709

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	62.96
264.00	63.20	58.61
0.00	0.00	0.00