
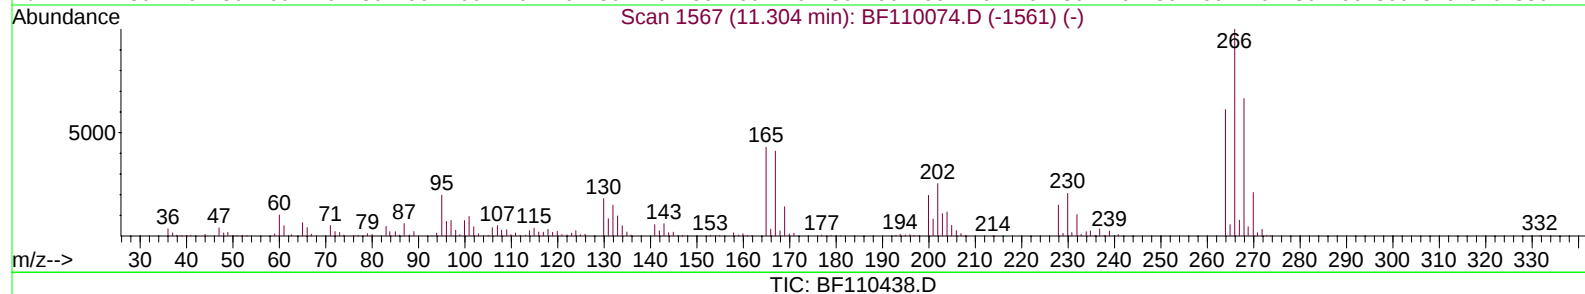
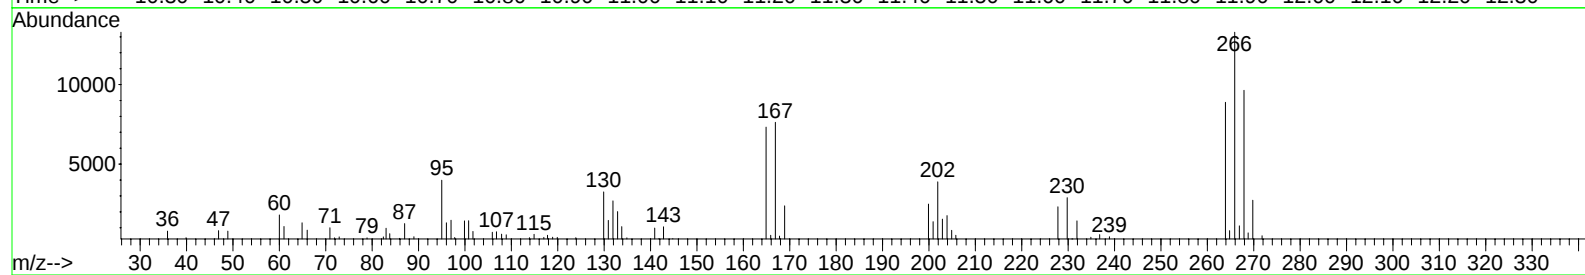


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110218\
Data File : BF110438.D
Acq On : 3 Nov 2018 3:50
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 05:37:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 01 16:06:12 2018
Response via : Initial Calibration

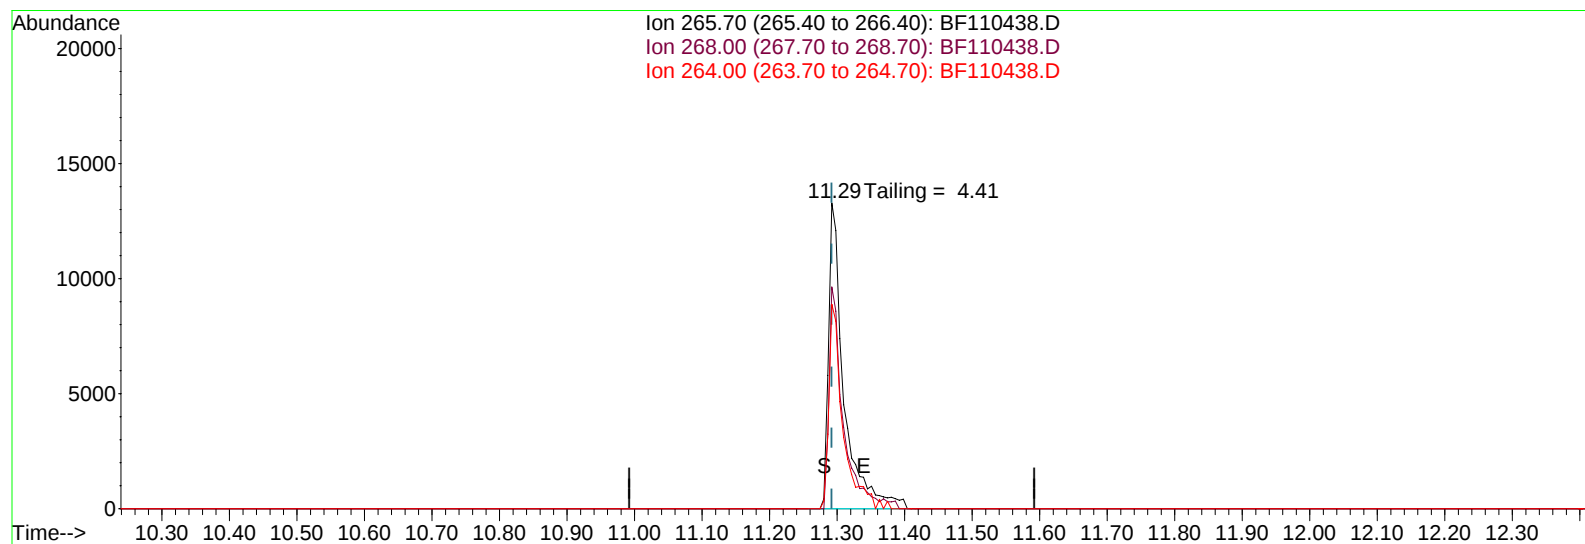

(70) Pentachlorophenol (C)




11.292min (+0.000) 0.00ng

response 21034

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	72.55
264.00	63.20	66.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF110218\
 Data File : BF110438.D
 Acq On : 3 Nov 2018 3:50
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 05:37:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF102318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 01 16:06:12 2018
 Response via : Initial Calibration

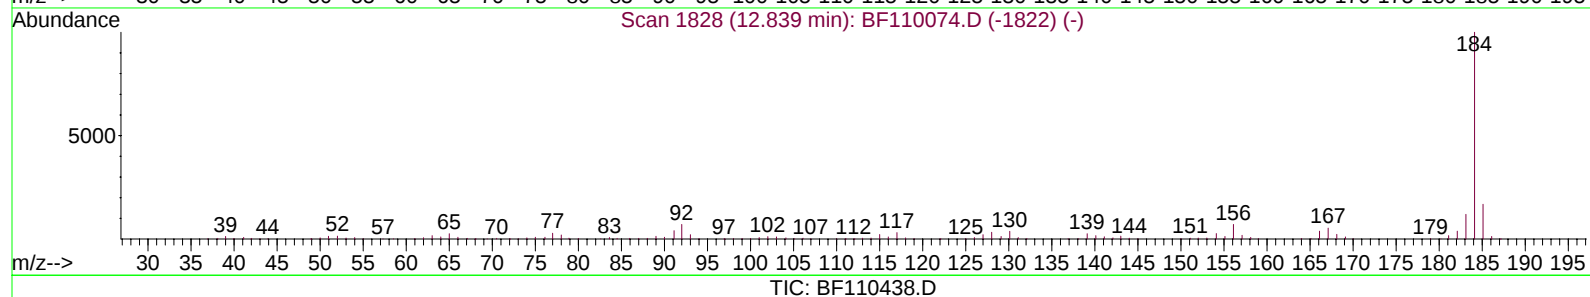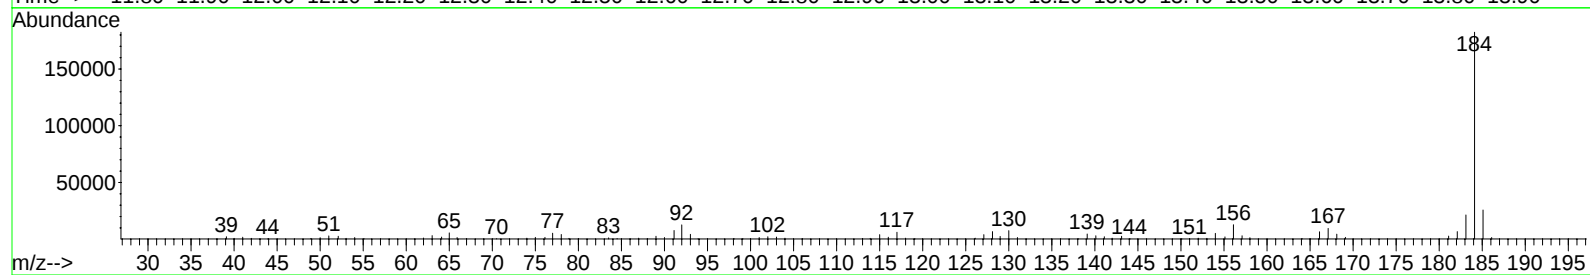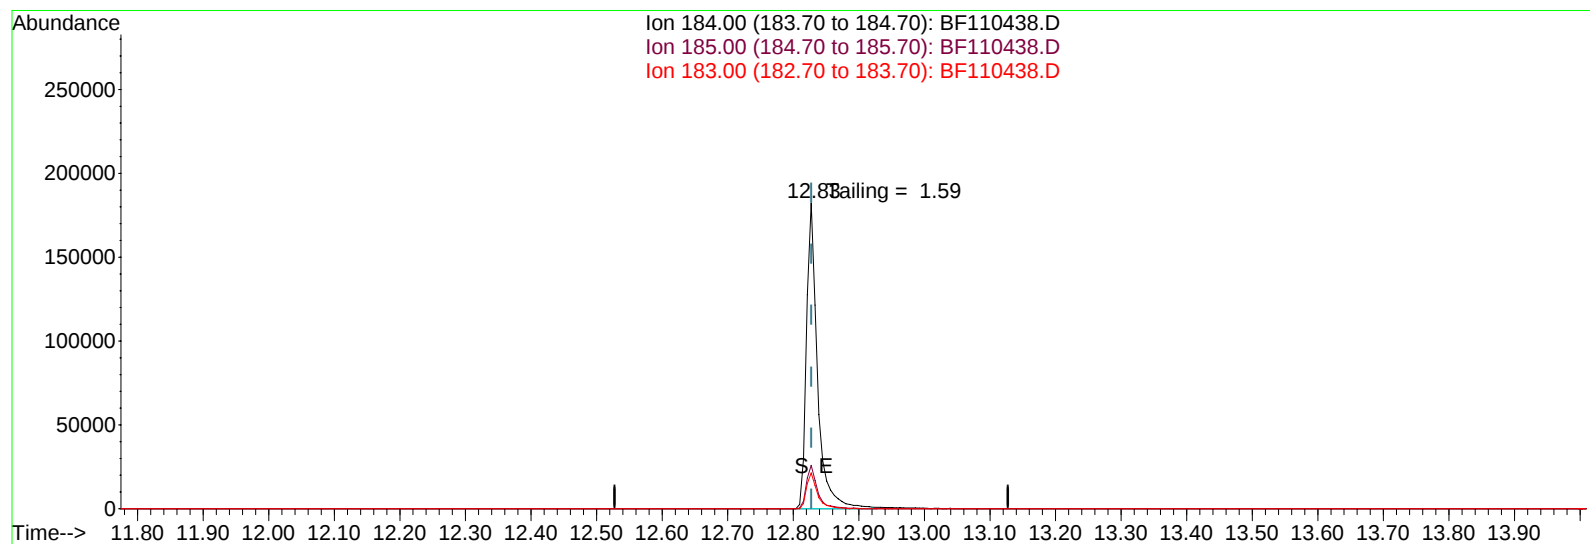

(77) Benzidine

12.827min (+0.000) 0.00ng

response 217751

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.18
183.00	11.80	11.73
0.00	0.00	0.00