


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110218\
 Data File : BF110412.D
 Acq On : 2 Nov 2018 15:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 01 16:06:12 2018

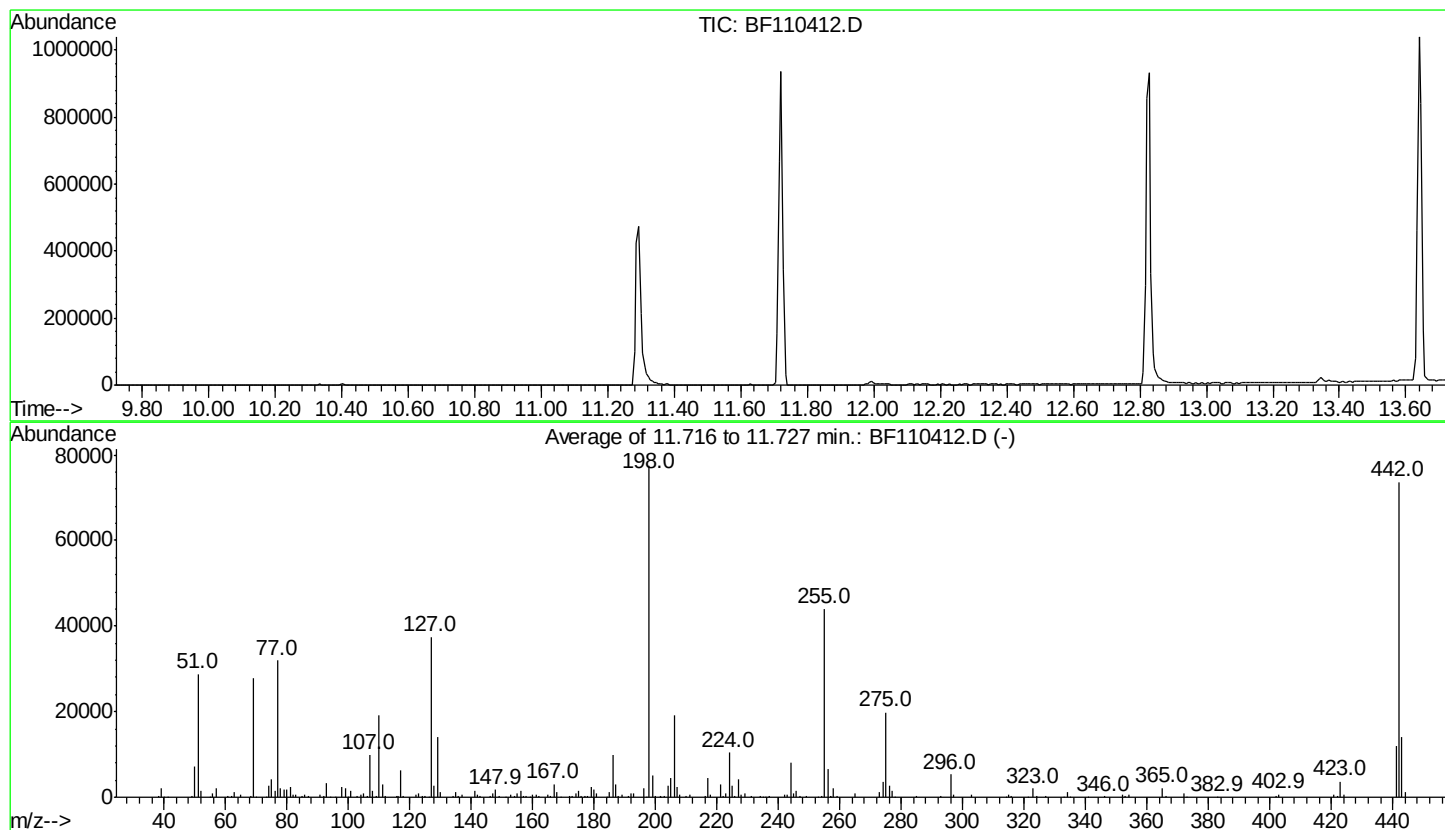

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	28787	PASS
68	69	0.00	2	1.2	348	PASS
69	198	0.00	100	36.0	27917	PASS
70	69	0.00	2	0.4	112	PASS
127	198	10	80	48.3	37451	PASS
197	198	0.00	2	0.1	110	PASS
198	198	100	100	100.0	77488	PASS
199	198	5	9	6.5	5053	PASS
275	198	10	60	25.7	19877	PASS
365	198	1	100	2.9	2221	PASS
441	198	0.01	100	15.3	11854	PASS
442	198	50	100	95.0	73640	PASS
443	442	15	24	19.2	14152	PASS