

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110223\
 Data File : BF136095.D
 Acq On : 02 Nov 2023 14:54
 Operator : CG\JU
 Sample : PB156561BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB156561BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136095.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.175	5	15	19	rVB	41983	64549	1.34%	0.228%
2	5.063	500	506	517	rBV	333835	492504	10.26%	1.742%
3	5.457	568	573	576	rBV	3340350	3654317	76.11%	12.924%
4	6.457	736	743	745	rBV	3070329	3630006	75.61%	12.838%
5	6.816	801	804	808	rBV	961542	760237	15.83%	2.689%
6	7.381	894	900	903	rBV	2383757	2446830	50.96%	8.654%
7	8.098	1017	1022	1025	rBV	1349061	1028716	21.43%	3.638%
8	9.181	1200	1206	1209	rBV	4908323	4522276	94.19%	15.994%
9	9.857	1317	1321	1324	rBV	1511563	1192318	24.83%	4.217%
10	10.651	1451	1456	1459	rBV	3093190	2881264	60.01%	10.190%
11	11.351	1571	1575	1578	rBV	1491972	1249367	26.02%	4.419%
12	12.951	1842	1847	1851	rBV	4473733	4801054	100.00%	16.980%
13	14.004	2022	2026	2030	rBV	1012338	849302	17.69%	3.004%
14	15.492	2274	2279	2287	rBV	565012	702359	14.63%	2.484%




Sum of corrected areas: 28275099

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110223\
Data File : BF136095.D
Acq On : 02 Nov 2023 14:54
Operator : CG\JU
Sample : PB156561BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156561BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

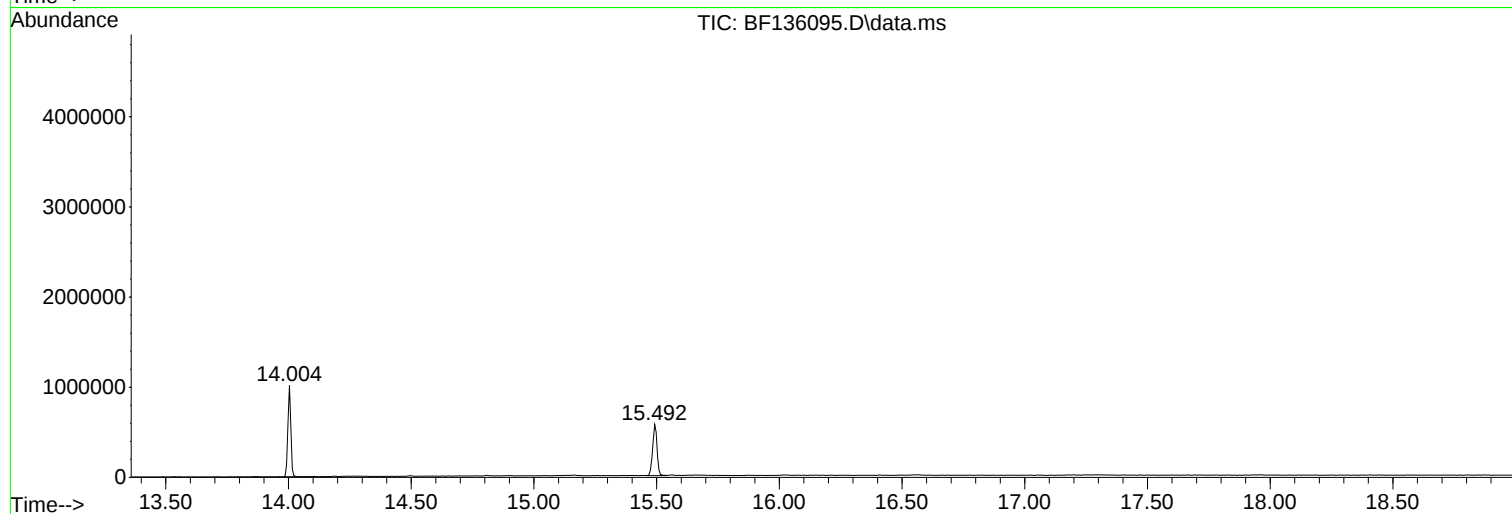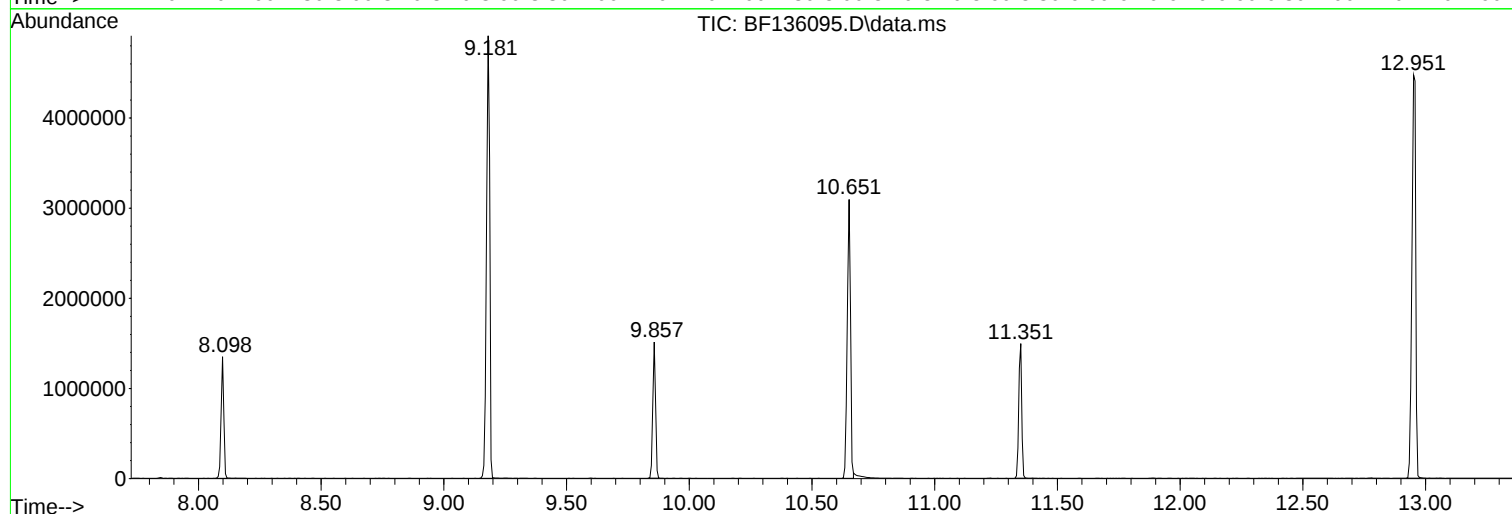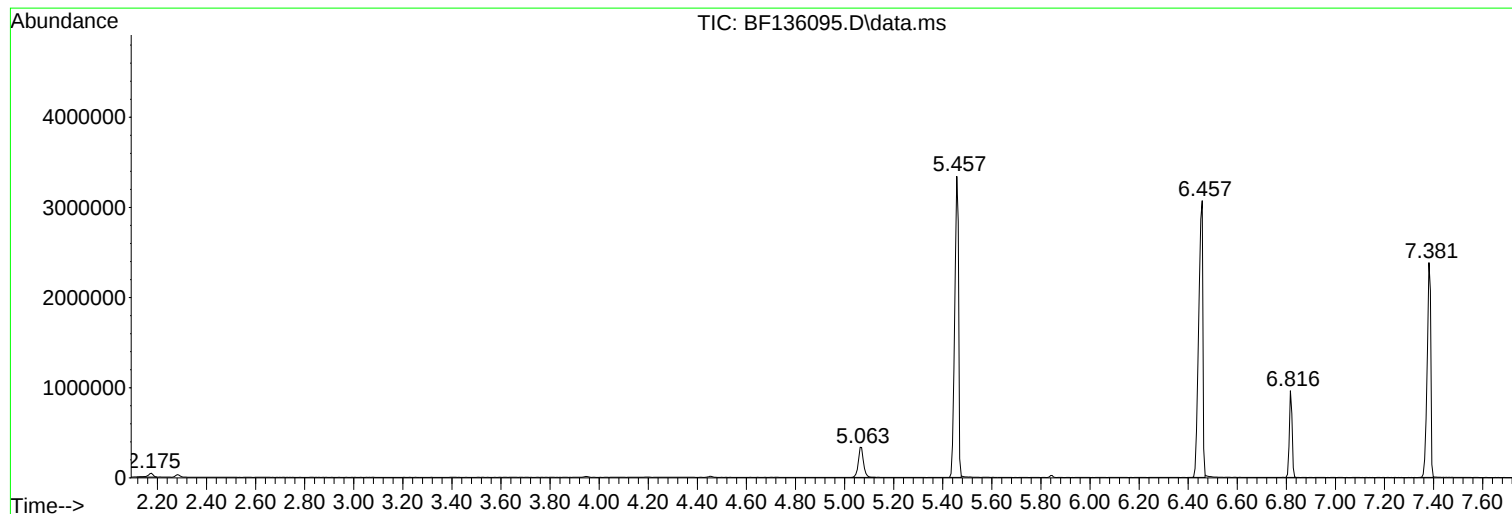

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110223\
Data File : BF136095.D
Acq On : 02 Nov 2023 14:54
Operator : CG\JU
Sample : PB156561BL
Misc :
ALS Vial : 6 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB156561BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
5.063	12.96 ng	492504	1,4-Dichlorobenzene-d4		6.816	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	53
2	Acetic acid, cyano-, 1,1-dimethy...		141	C7H11NO2	001116-98-9	32
3	2,3-Butanedione, monooxime		101	C4H7NO2	000057-71-6	25
4	1-Propen-2-ol, acetate		100	C5H8O2	000108-22-5	10
5	Acetone		58	C3H6O	000067-64-1	9

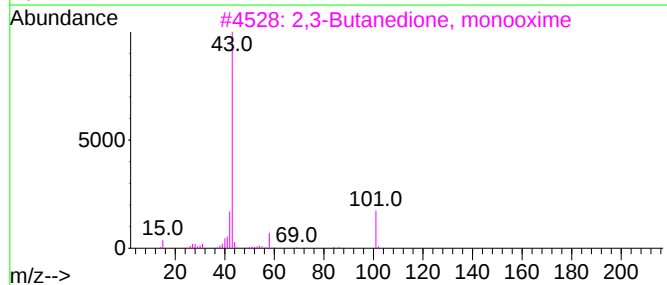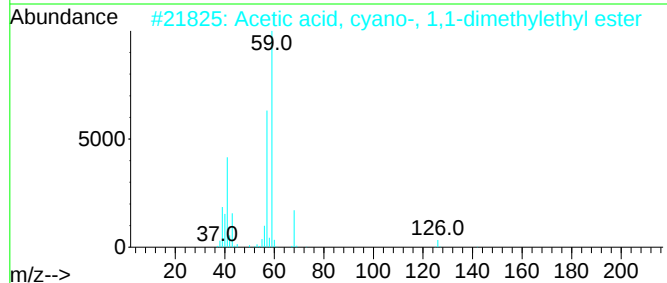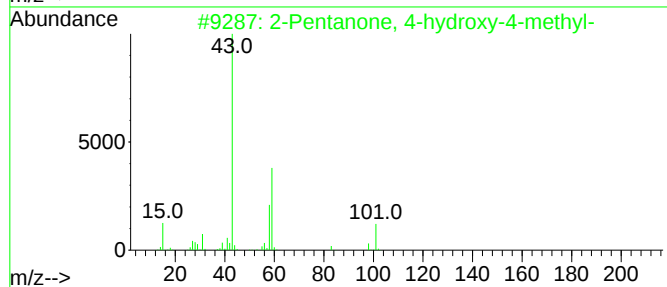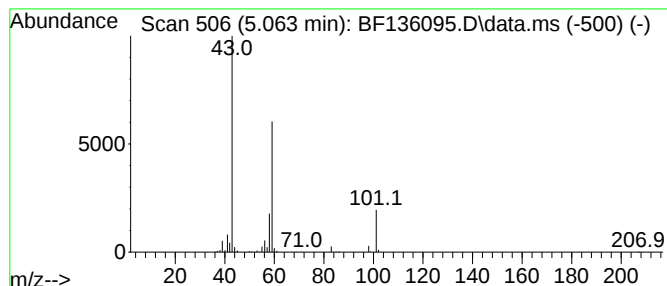

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110223\
Data File : BF136095.D
Acq On : 02 Nov 2023 14:54
Operator : CG\JU
Sample : PB156561BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156561BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.063	13.0	ng	492504	1	6.816	760237	20.0