

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110223\
 Data File : BF136097.D
 Acq On : 02 Nov 2023 15:54
 Operator : CG\JU
 Sample : PB156660BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB156660BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136097.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.075	500	508	515	rBV	81887	115134	2.54%	0.430%
2	5.457	567	573	576	rBV	3292315	3484743	76.85%	13.001%
3	6.451	736	742	745	rBV	2921473	3463799	76.39%	12.923%
4	6.816	801	804	808	rVB	920542	749918	16.54%	2.798%
5	7.381	894	900	903	rBV	2297946	2324594	51.27%	8.673%
6	8.098	1017	1022	1025	rBV	1323391	1026452	22.64%	3.830%
7	9.180	1200	1206	1209	rBV	4977430	4303625	94.91%	16.056%
8	9.857	1317	1321	1324	rBV	1547843	1198269	26.43%	4.471%
9	10.651	1451	1456	1459	rBV	3065751	2731038	60.23%	10.189%
10	11.351	1571	1575	1578	rBV	1546336	1269135	27.99%	4.735%
11	12.951	1842	1847	1851	rBV	4365909	4534438	100.00%	16.917%
12	14.004	2022	2026	2030	rBV	1009411	871348	19.22%	3.251%
13	15.492	2273	2279	2285	rBV	596657	731109	16.12%	2.728%




Sum of corrected areas: 26803602

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110223\
Data File : BF136097.D
Acq On : 02 Nov 2023 15:54
Operator : CG\JU
Sample : PB156660BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156660BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

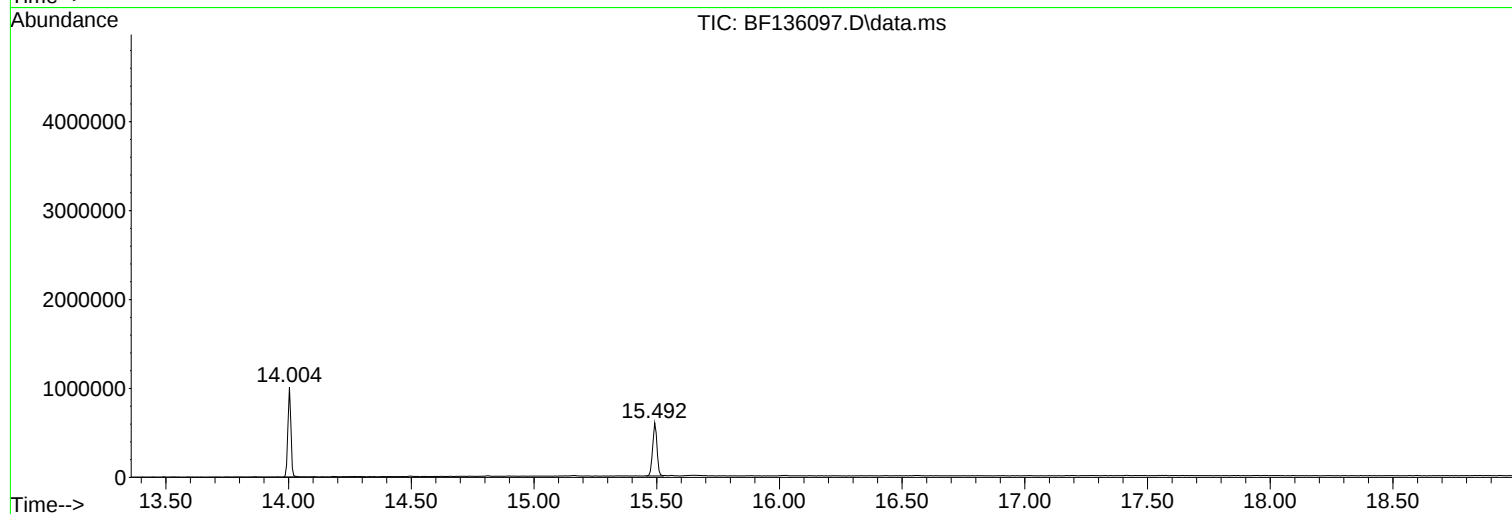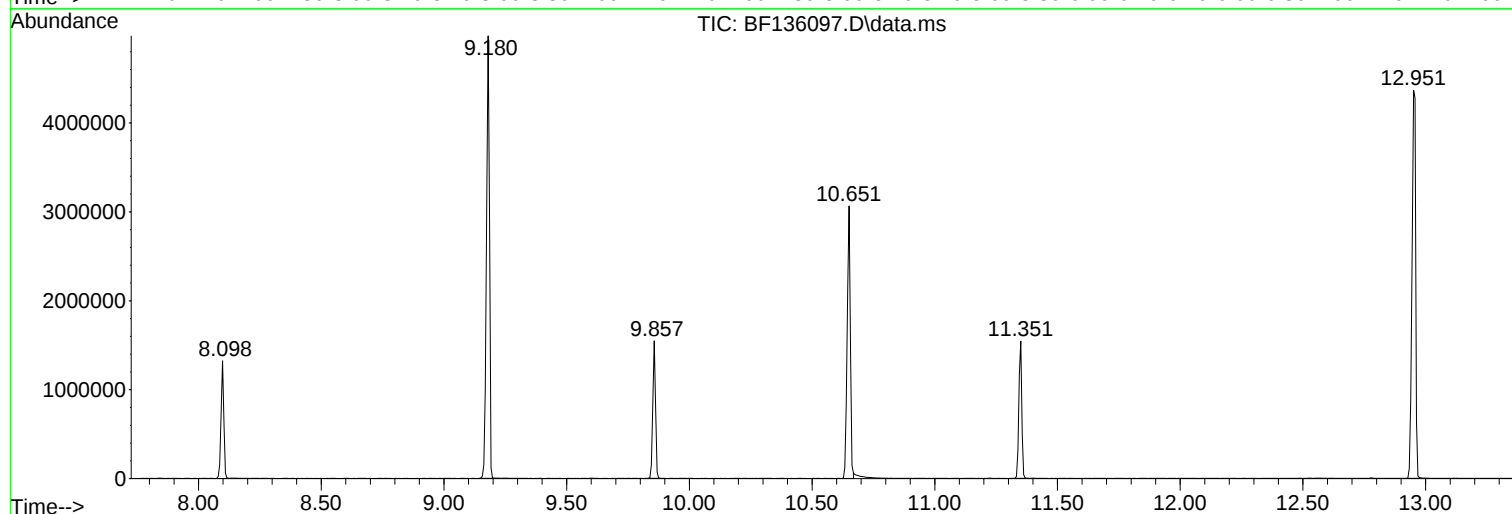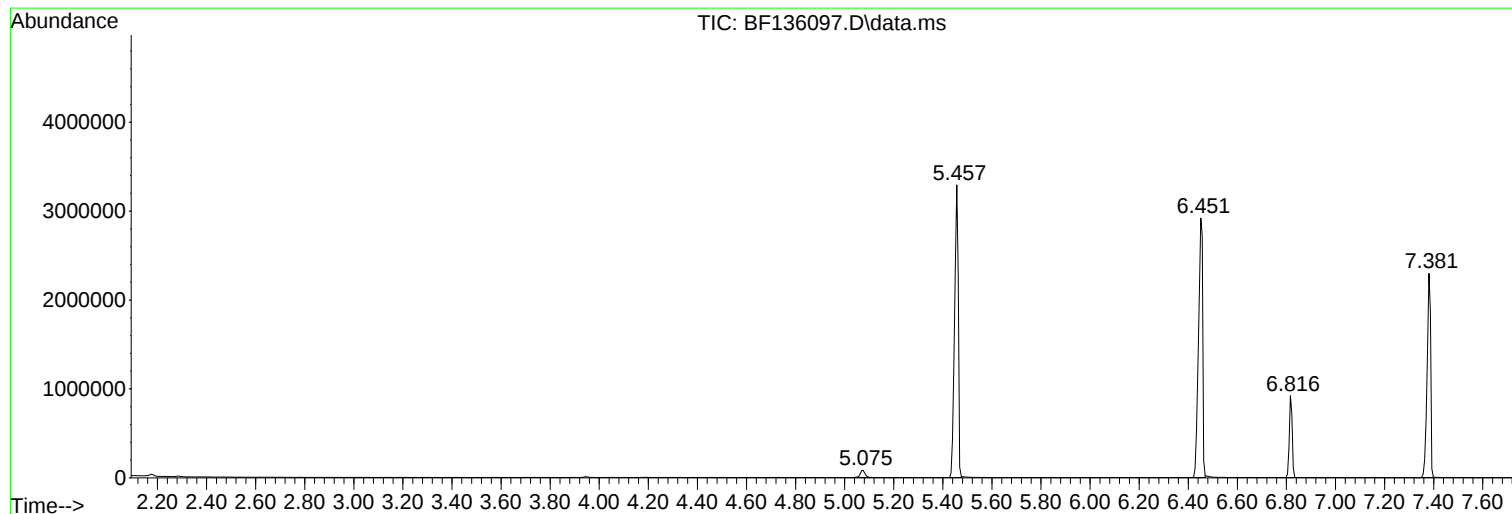

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110223\
Data File : BF136097.D
Acq On : 02 Nov 2023 15:54
Operator : CG\JU
Sample : PB156660BL
Misc :
ALS Vial : 8 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB156660BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
5.075	3.07 ng	115134	1,4-Dichlorobenzene-d4		6.816	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	53
2	1-Propen-2-ol, acetate		100	C5H8O2	000108-22-5	12
3	Acetone		58	C3H6O	000067-64-1	9
4	Morpholine, 4-methyl-		101	C5H11NO	000109-02-4	9
5	Formamide, N,N-diethyl-		101	C5H11NO	000617-84-5	9

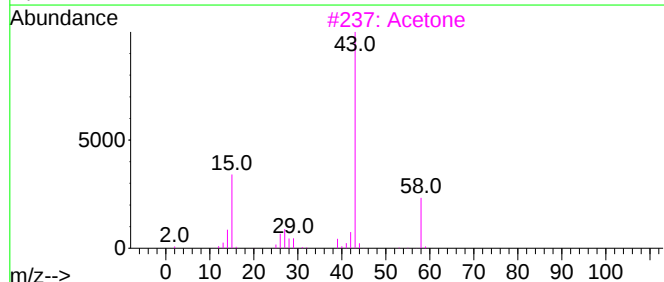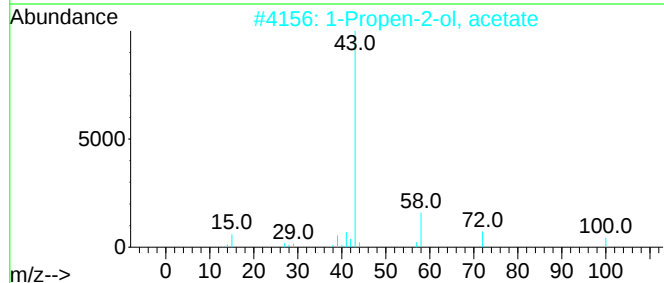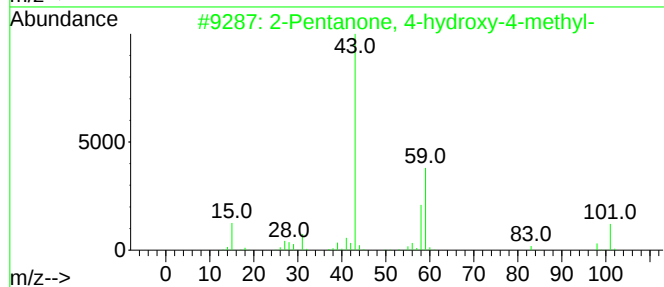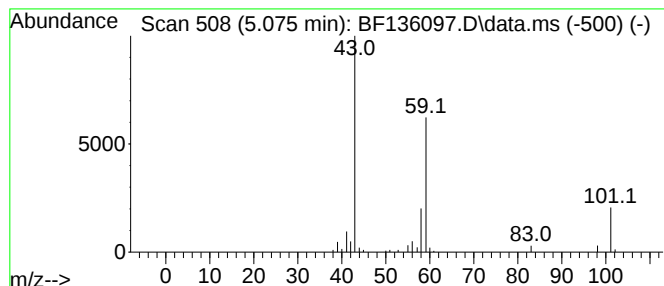

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110223\
Data File : BF136097.D
Acq On : 02 Nov 2023 15:54
Operator : CG\JU
Sample : PB156660BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156660BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.075	3.1	ng	115134	1	6.816	749918	20.0