

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110223\
 Data File : BF136100.D
 Acq On : 02 Nov 2023 17:29
 Operator : CG\JU
 Sample : 05040-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EB-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136100.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.034	498	501	508	rVB	48398	56062	1.51%	0.317%
2	5.440	566	570	574	rBV	1433128	1276114	34.45%	7.211%
3	6.439	736	740	744	rBV	936867	783032	21.14%	4.425%
4	6.816	801	804	808	rBV	910603	712851	19.24%	4.028%
5	7.381	895	900	903	rBV	2213240	2248021	60.69%	12.704%
6	8.098	1018	1022	1025	rBV	1266821	950758	25.67%	5.373%
7	8.345	1062	1064	1075	rVB	45257	51067	1.38%	0.289%
8	9.180	1202	1206	1209	rBV	4398727	3704307	100.00%	20.933%
9	9.857	1317	1321	1324	rBV	1310289	1020325	27.54%	5.766%
10	10.651	1451	1456	1459	rBV	2333271	2036399	54.97%	11.508%
11	11.351	1571	1575	1578	rBV	1020230	888328	23.98%	5.020%
12	11.886	1660	1666	1670	rBV	73612	80673	2.18%	0.456%
13	12.598	1783	1787	1794	rBV	55184	59625	1.61%	0.337%
14	12.951	1842	1847	1850	rBV	2963633	2530567	68.31%	14.300%
15	14.004	2022	2026	2030	rBV	765205	655290	17.69%	3.703%
16	14.898	2173	2178	2185	rBV2	28101	44989	1.21%	0.254%
17	15.492	2274	2279	2284	rBV	504591	597360	16.13%	3.376%




Sum of corrected areas: 17695768

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110223\
Data File : BF136100.D
Acq On : 02 Nov 2023 17:29
Operator : CG\JU
Sample : 05040-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EB-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

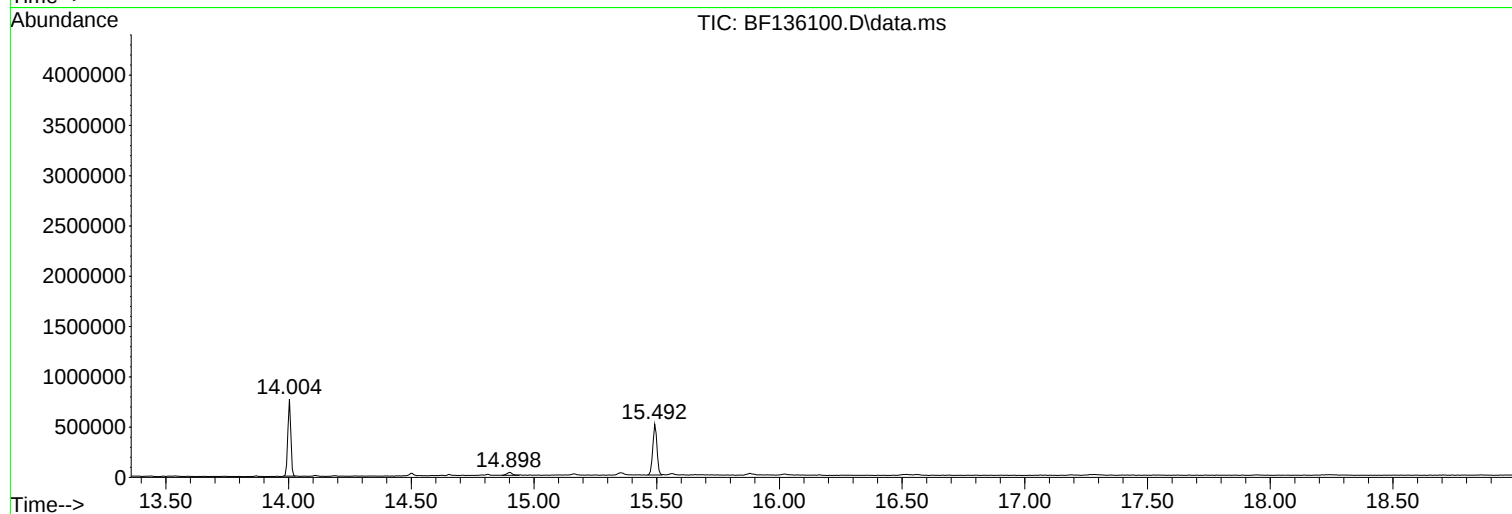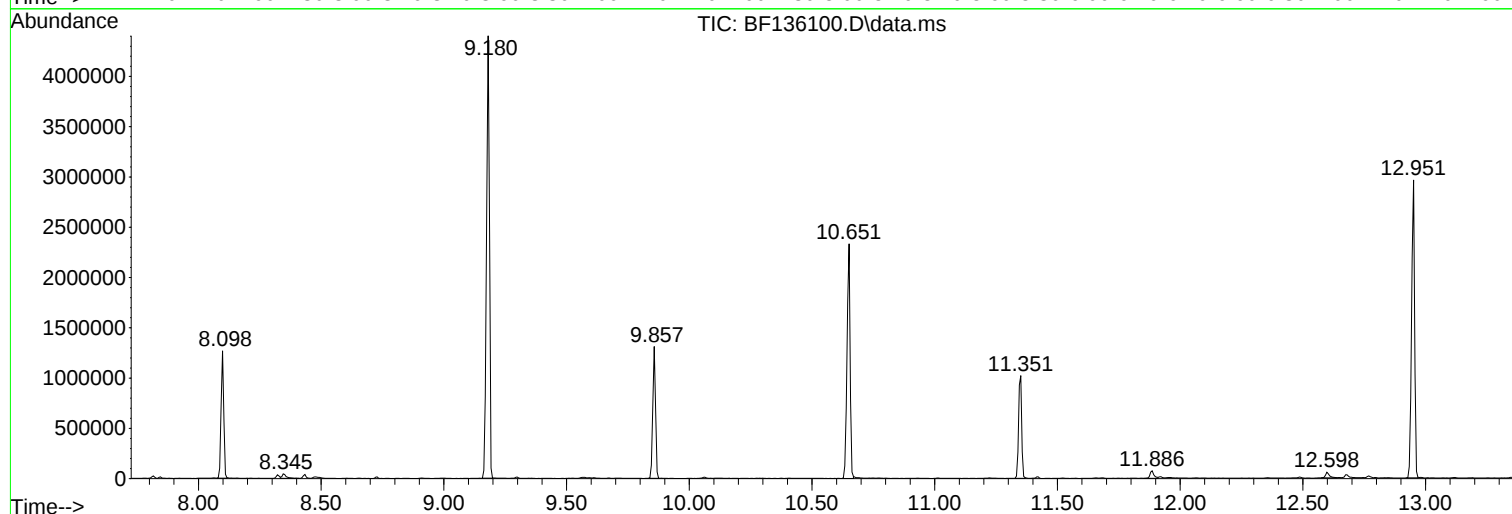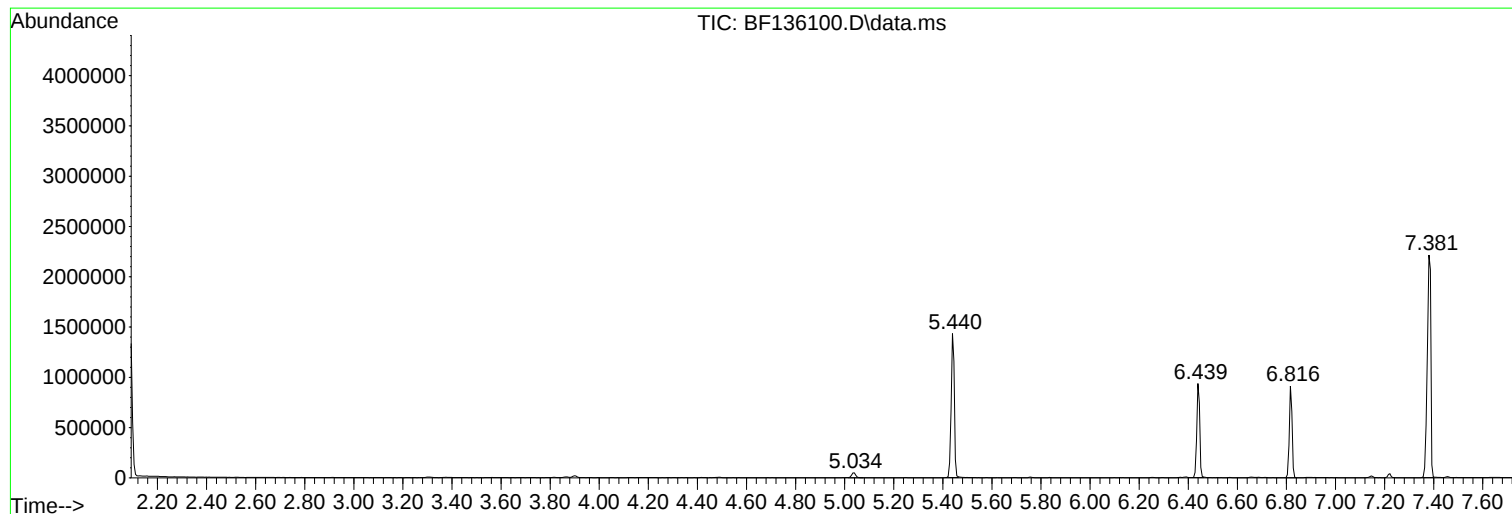

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110223\
Data File : BF136100.D
Acq On : 02 Nov 2023 17:29
Operator : CG\JU
Sample : 05040-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EB-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110223\
Data File : BF136100.D
Acq On : 02 Nov 2023 17:29
Operator : CG\JU
Sample : 05040-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EB-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------