


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110223\
Data File : BF136090.D
Acq On : 02 Nov 2023 12:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 31 01:13:02 2023

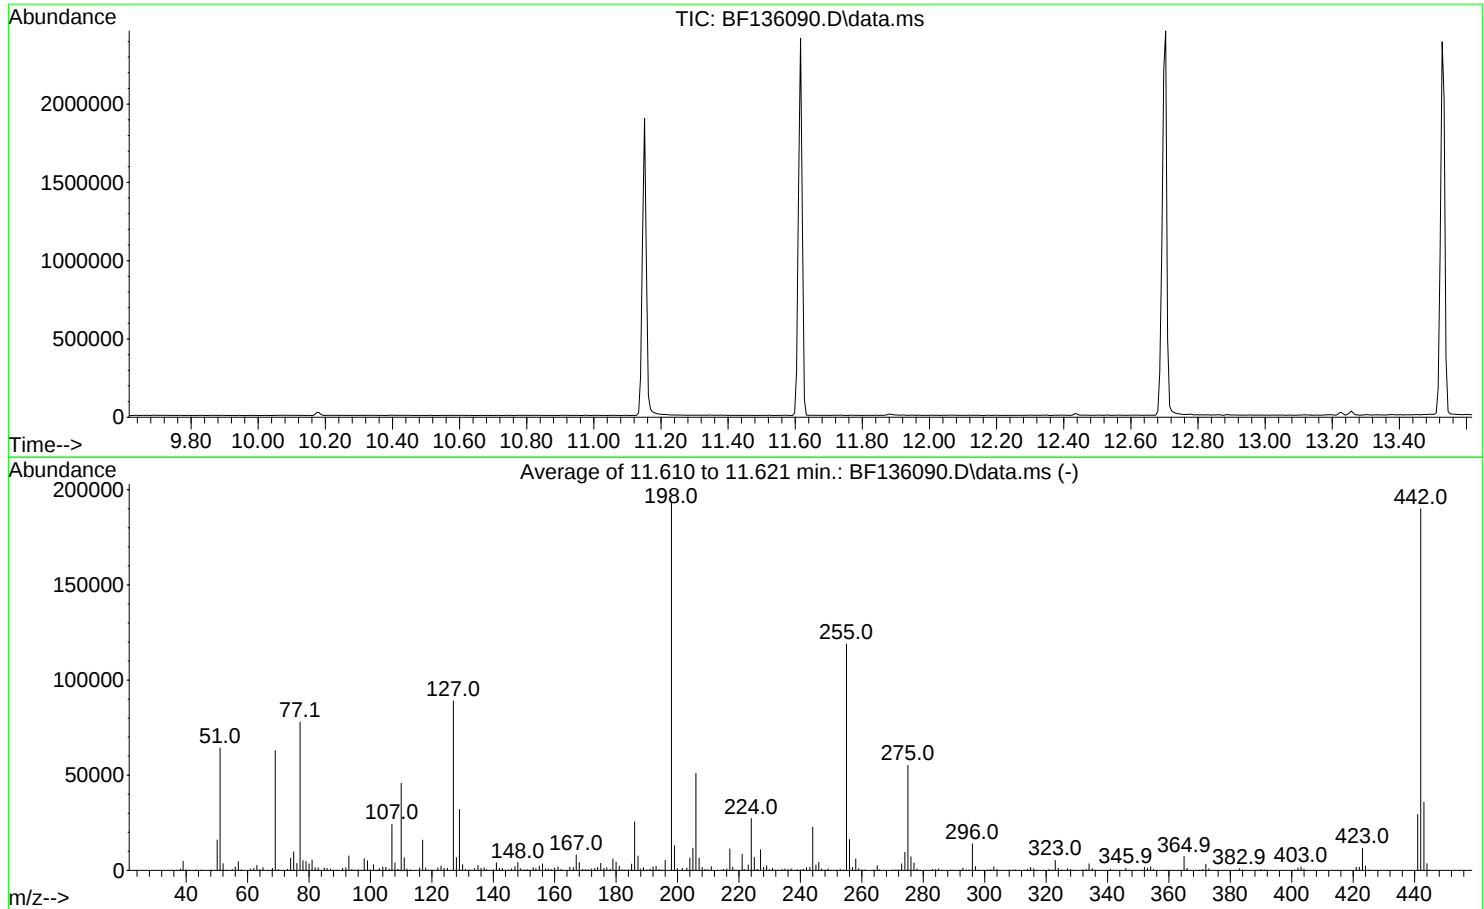




AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	64339	PASS
68	69	0.00	2	1.7	1046	PASS
69	198	0.00	100	32.5	62880	PASS
70	69	0.00	2	0.6	390	PASS
127	198	10	80	46.1	89064	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	193309	PASS
199	198	5	9	6.7	12918	PASS
275	198	10	60	28.6	55232	PASS
365	198	1	100	3.8	7284	PASS
441	198	0.01	100	15.2	29328	PASS
442	442	50	100	100.0	190027	PASS
443	442	15	24	18.8	35819	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110223\
Data File : BF136090.D
Acq On : 02 Nov 2023 12:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 02 19:49:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 01:13:02 2023
Response via : Initial Calibration

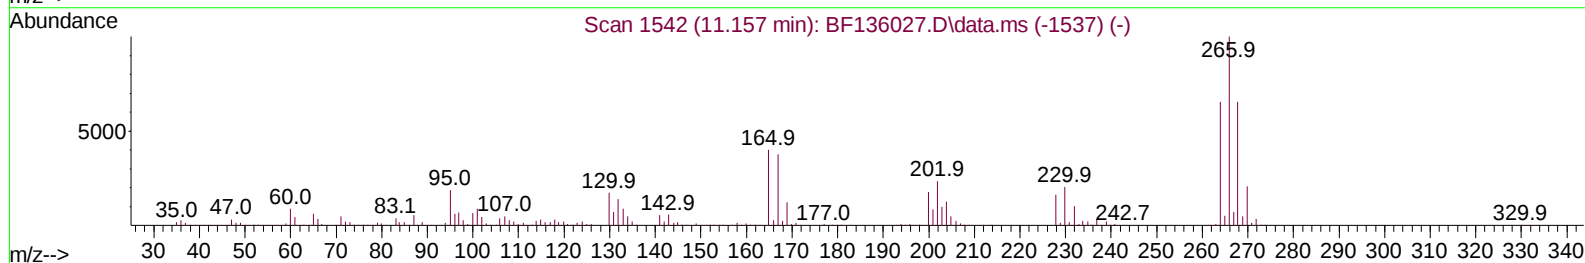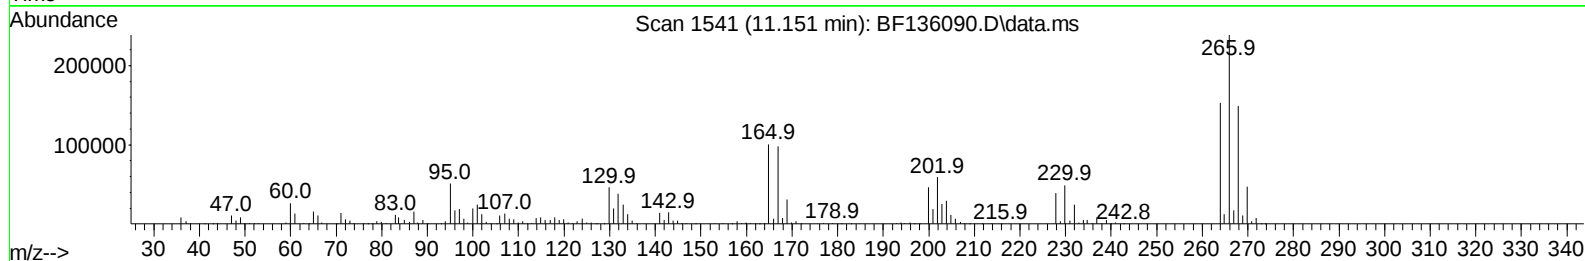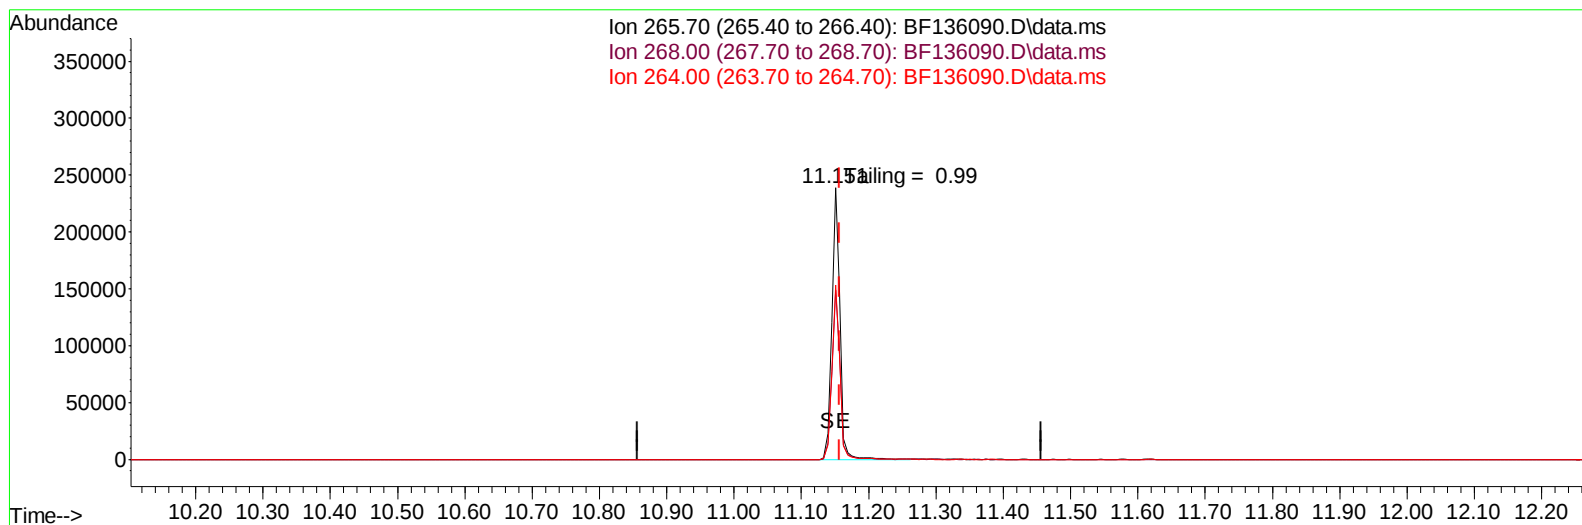

TIC: BF136090.D\data.ms

(70) Pentachlorophenol (C)

11.151min (-0.006) 169744.27 ng




response 201410

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.47
264.00	65.30	64.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110223\
Data File : BF136090.D
Acq On : 02 Nov 2023 12:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 02 19:49:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 01:13:02 2023
Response via : Initial Calibration

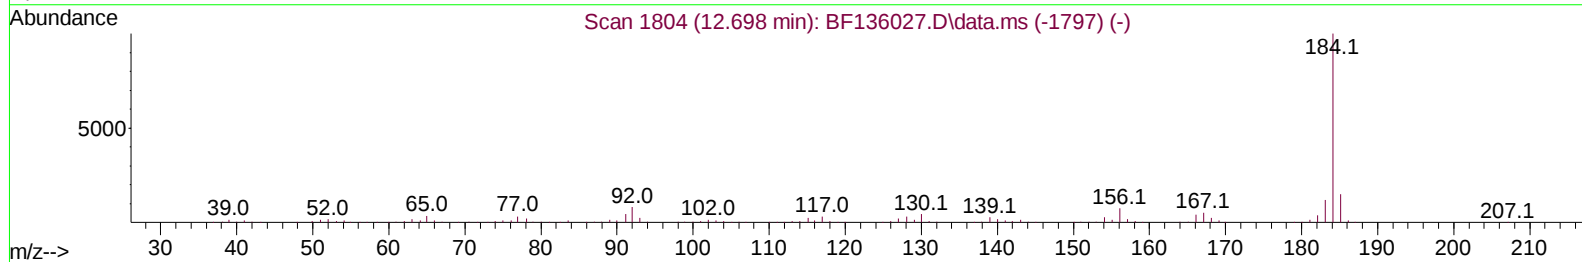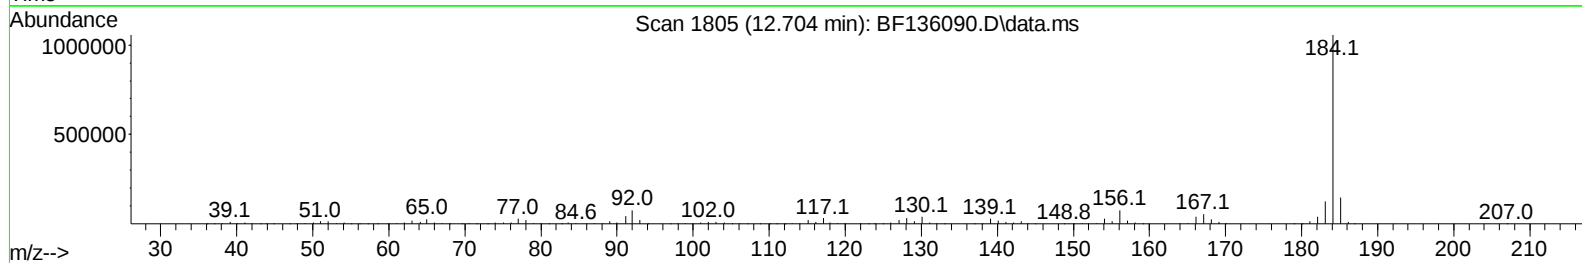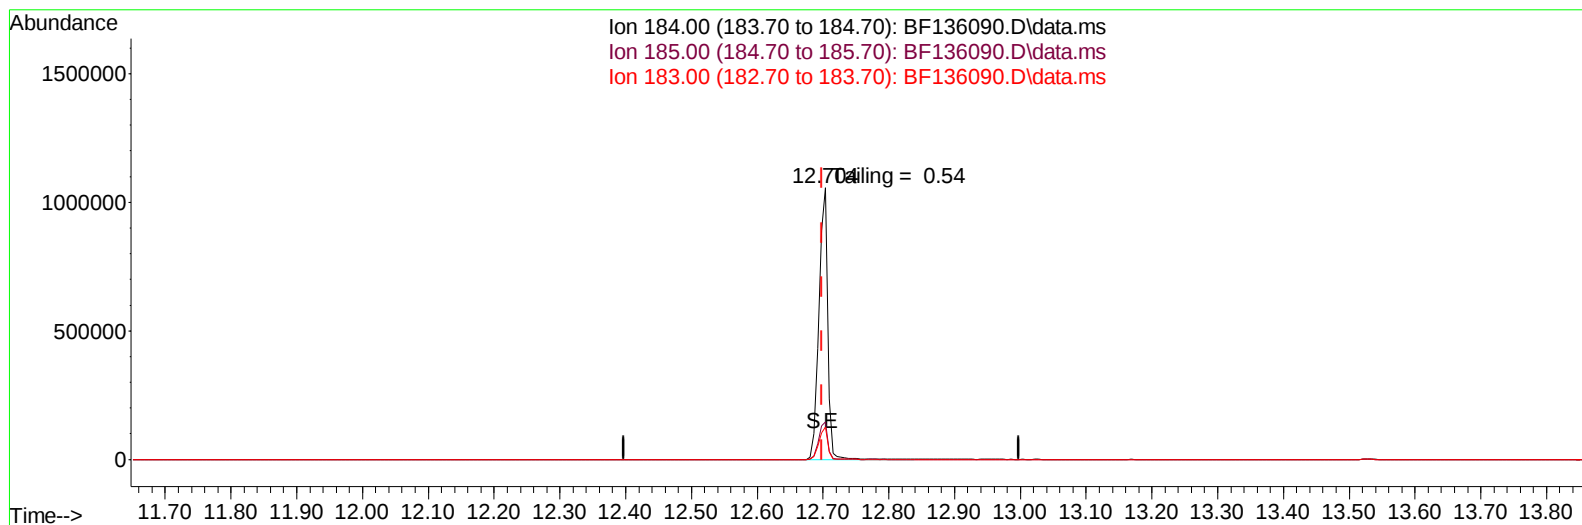

TIC: BF136090.D\data.ms

(77) Benzidine

12.704min (+ 0.006) 529872.60 ng

response 991455

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.79
183.00	11.90	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/2/2023	BNA_F	<u>BF136090.D</u>
Compound Name	Response	Retention Time
DDT	430977	13.527
DDD	7061	13.257
DDE	349	12.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7410	438387	1.69

Instrument :
BNA_F
ClientSampleId :
DFTPP