
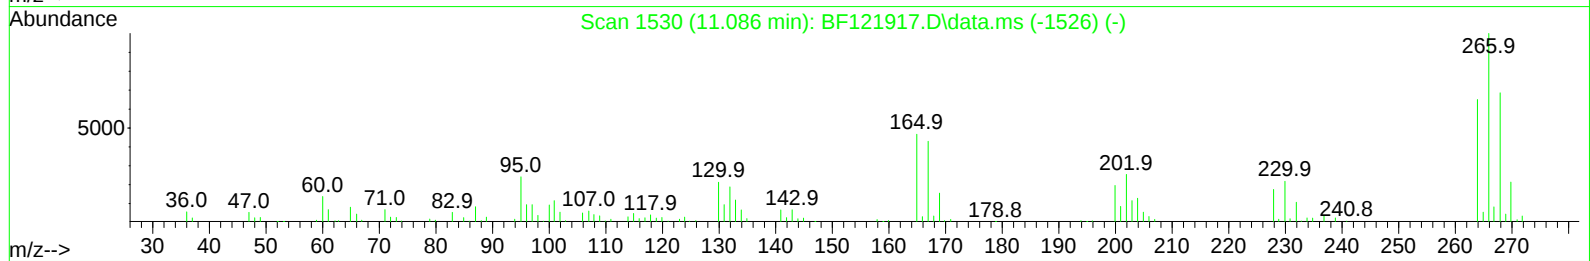
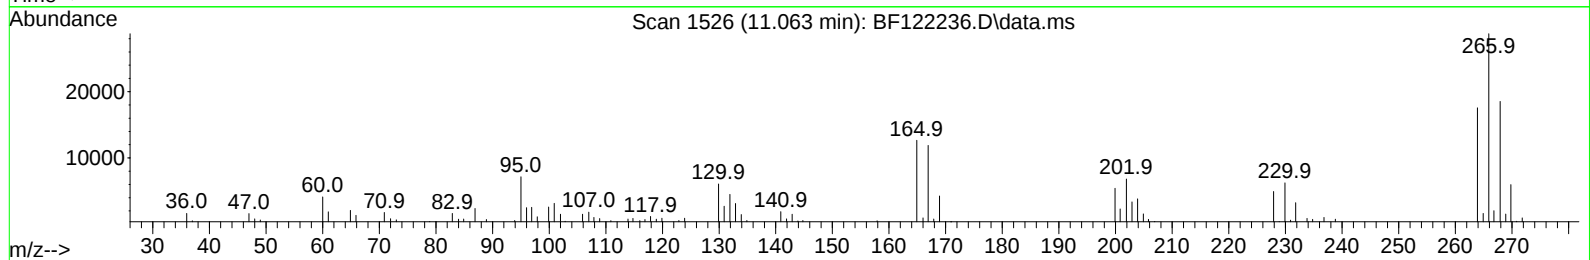


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110320\
Data File : BF122236.D
Acq On : 3 Nov 2020 11:08
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 05:08:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 30 10:16:54 2020
Response via : Initial Calibration

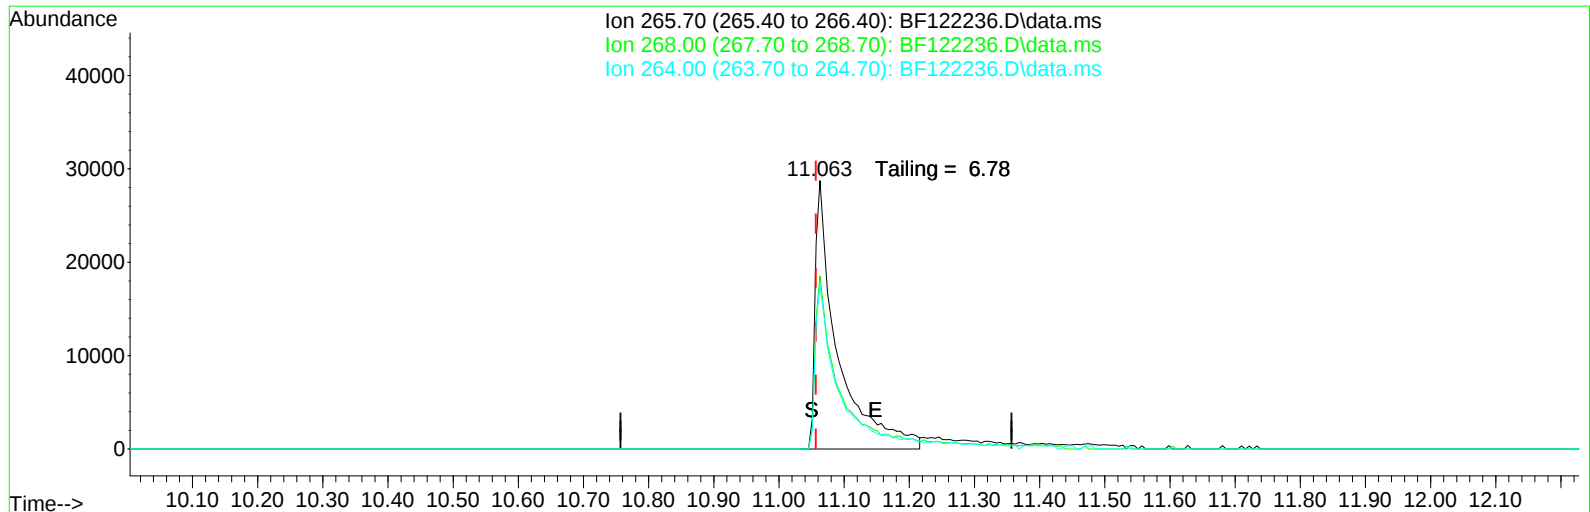

TIC: BF122236.D\data.ms

(70) Pentachlorophenol (C)




11.063min (+ 0.006) 93437.83 ng

response 69334

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	64.46
264.00	62.40	61.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110320\
Data File : BF122236.D
Acq On : 3 Nov 2020 11:08
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 05:08:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 30 10:16:54 2020
Response via : Initial Calibration

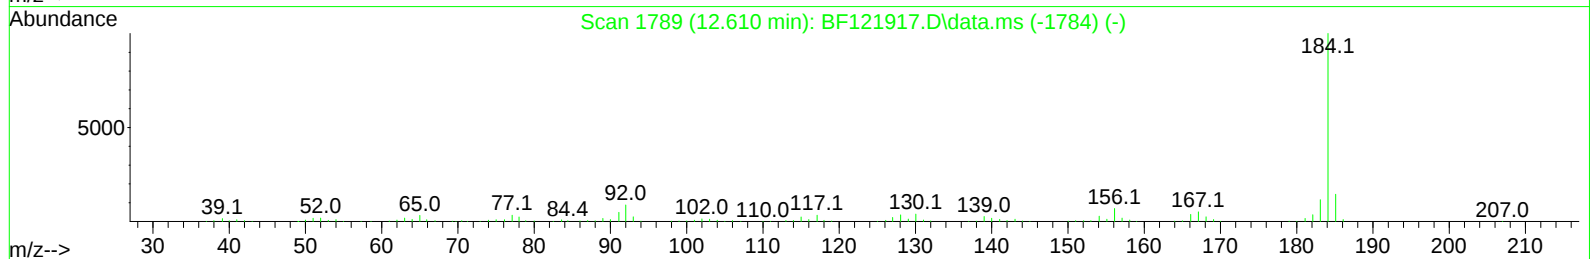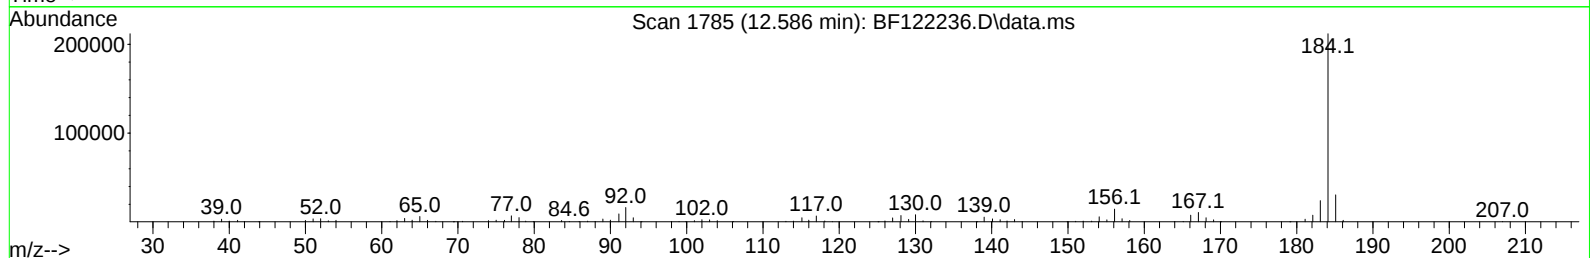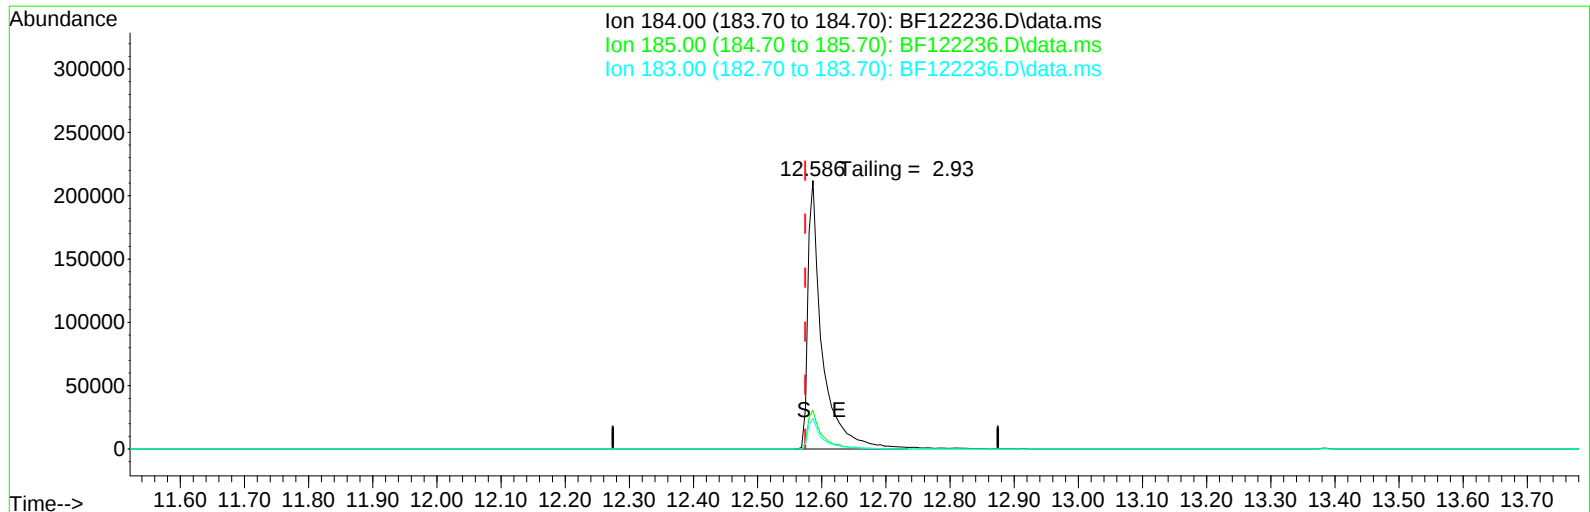

TIC: BF122236.D\data.ms

(77) Benzidine

12.586min (+ 0.012) 0.00 ng

response 330993

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.41
183.00	11.70	11.39
0.00	0.00	0.00