

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110320\
 Data File : BF122243.D
 Acq On : 3 Nov 2020 16:32
 Operator : JU/CG
 Sample : L4607-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OW-05

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122243.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.345	551	554	574	rBV	477409	943724	33.19%	5.571%
2	6.381	727	730	755	rBV	297934	668656	23.52%	3.947%
3	6.710	783	786	797	rVB	464266	480691	16.91%	2.838%
4	7.281	879	883	907	rBV	1572621	1707286	60.04%	10.079%
5	7.992	1001	1004	1024	rVB	600879	635242	22.34%	3.750%
6	9.063	1182	1186	1198	rBV	2550138	2826563	99.41%	16.686%
7	9.186	1202	1207	1222	rVB	494194	564514	19.85%	3.333%
8	9.469	1252	1255	1268	rVB	88730	112892	3.97%	0.666%
9	9.745	1298	1302	1313	rBV	719647	738420	25.97%	4.359%
10	10.333	1398	1402	1413	rBV	86533	156394	5.50%	0.923%
11	10.539	1434	1437	1452	rBV	1731862	1979775	69.63%	11.687%
12	11.233	1552	1555	1565	rBV	766752	757130	26.63%	4.470%
13	11.763	1641	1645	1658	rBV2	238340	325571	11.45%	1.922%
14	12.304	1732	1737	1750	rVB	73769	139009	4.89%	0.821%
15	12.469	1759	1765	1768	rBV	87372	84680	2.98%	0.500%
16	12.545	1775	1778	1787	rBV	88436	120158	4.23%	0.709%
17	12.816	1820	1824	1827	rBV	2979732	2843436	100.00%	16.786%
18	13.374	1916	1919	1922	rBV	34877	30000	1.06%	0.177%
19	13.733	1976	1980	1995	rVB3	148734	345003	12.13%	2.037%
20	13.880	2002	2005	2016	rBV	486425	589733	20.74%	3.481%
21	14.021	2025	2029	2032	rBV	33715	33982	1.20%	0.201%
22	14.321	2077	2080	2085	rBV	41461	43007	1.51%	0.254%
23	14.621	2127	2131	2136	rBV	46290	50471	1.78%	0.298%
24	14.939	2181	2185	2191	rVB	45155	57933	2.04%	0.342%
25	15.292	2241	2245	2247	rBV	31867	37910	1.33%	0.224%
26	15.321	2247	2250	2269	rVB	334636	547142	19.24%	3.230%
27	15.692	2308	2313	2317	rBV	31194	45373	1.60%	0.268%
28	15.810	2330	2333	2342	rVB7	16319	40097	1.41%	0.237%
29	16.157	2388	2392	2397	rBV4	20075	34737	1.22%	0.205%




Sum of corrected areas: 16939529

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110320\
Data File : BF122243.D
Acq On : 3 Nov 2020 16:32
Operator : JU/CG
Sample : L4607-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OW-05

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

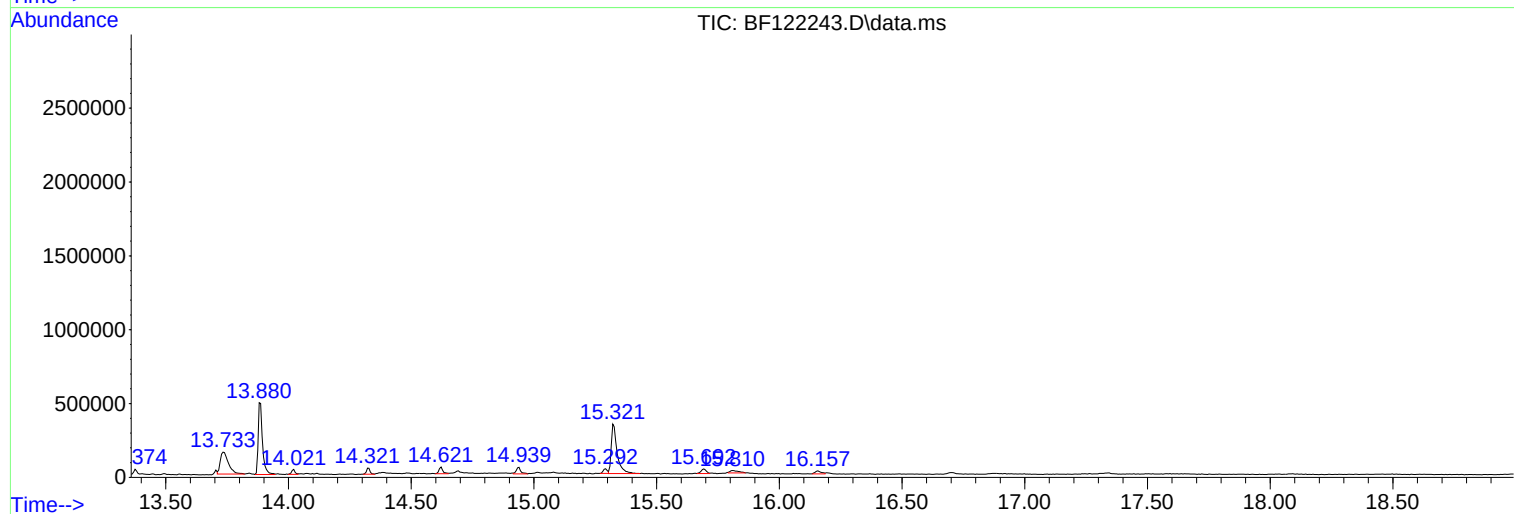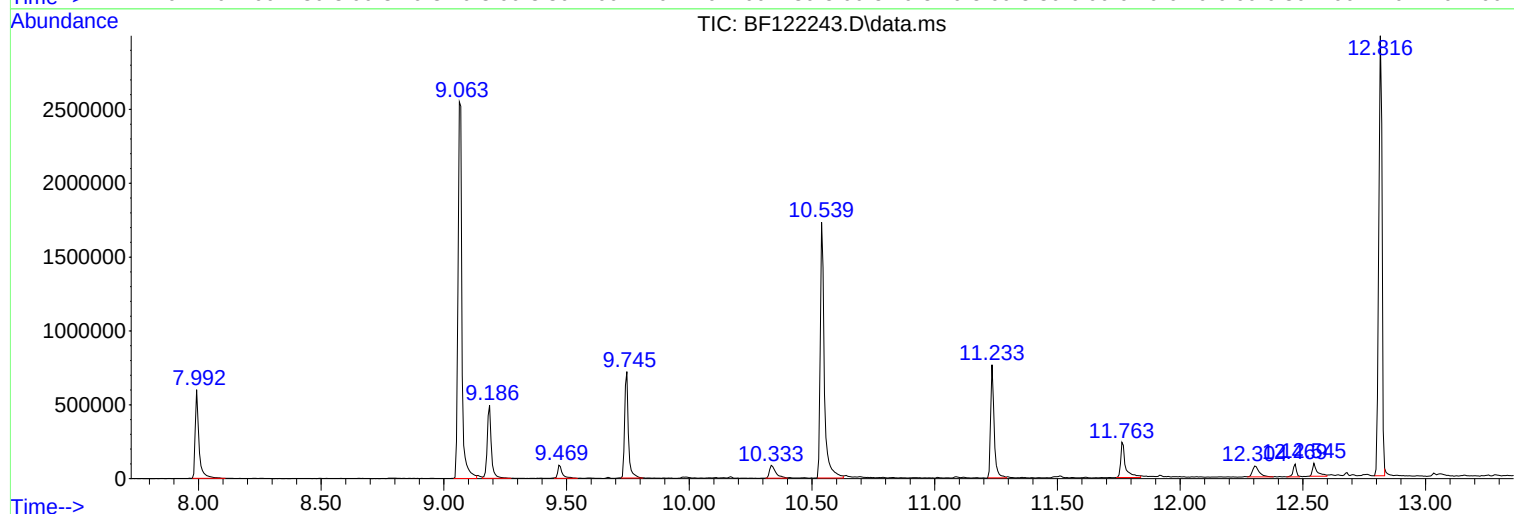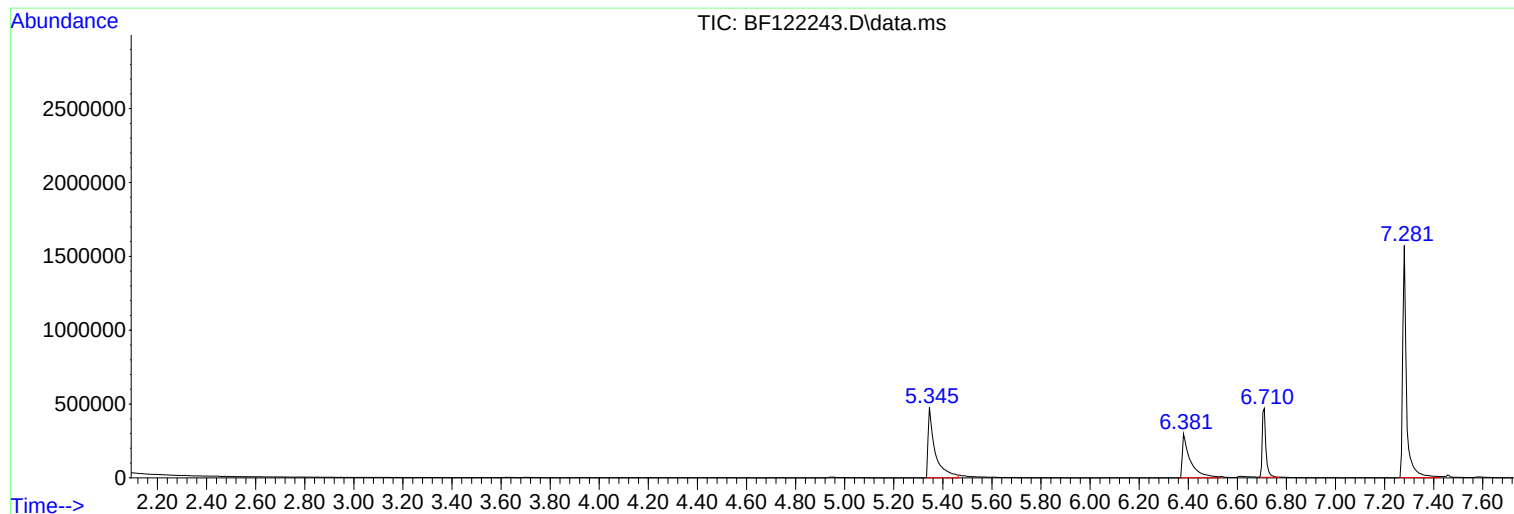

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110320\
Data File : BF122243.D
Acq On : 3 Nov 2020 16:32
Operator : JU/CG
Sample : L4607-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OW-05

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110320\
Data File : BF122243.D
Acq On : 3 Nov 2020 16:32
Operator : JU/CG
Sample : L4607-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OW-05

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
