
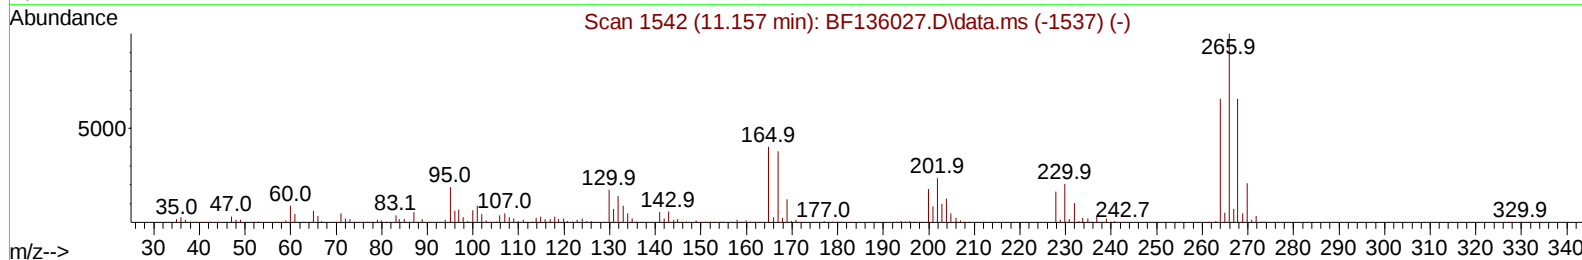
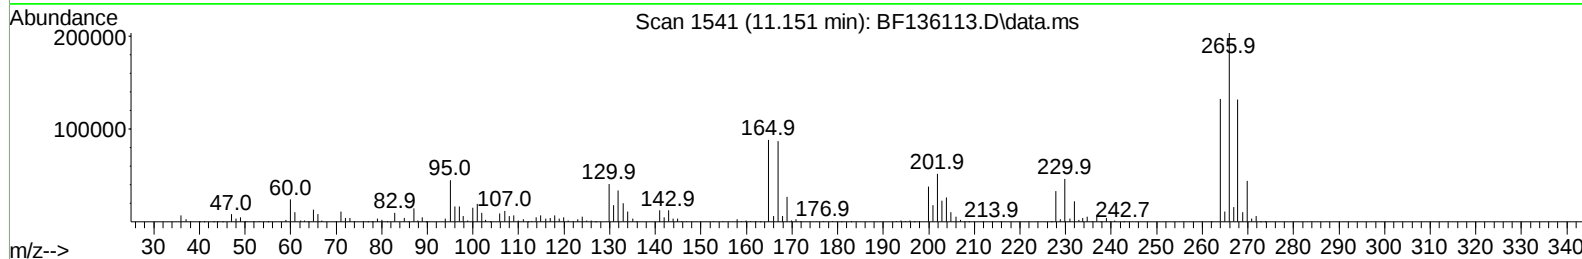


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110323\
Data File : BF136113.D
Acq On : 03 Nov 2023 09:29
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 20:42:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 01:13:02 2023
Response via : Initial Calibration

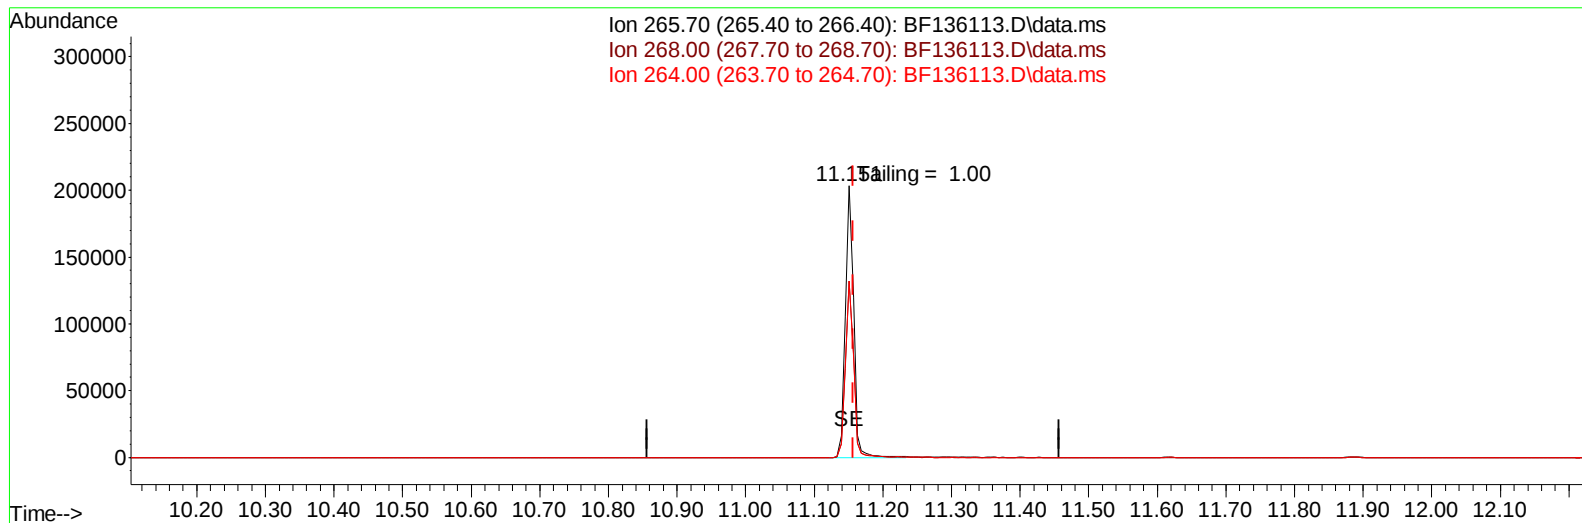

TIC: BF136113.D\data.ms

(70) Pentachlorophenol (C)




11.151min (-0.006) 33621.96 ng

response 169006

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.86
264.00	65.30	65.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110323\
Data File : BF136113.D
Acq On : 03 Nov 2023 09:29
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 20:42:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 01:13:02 2023
Response via : Initial Calibration

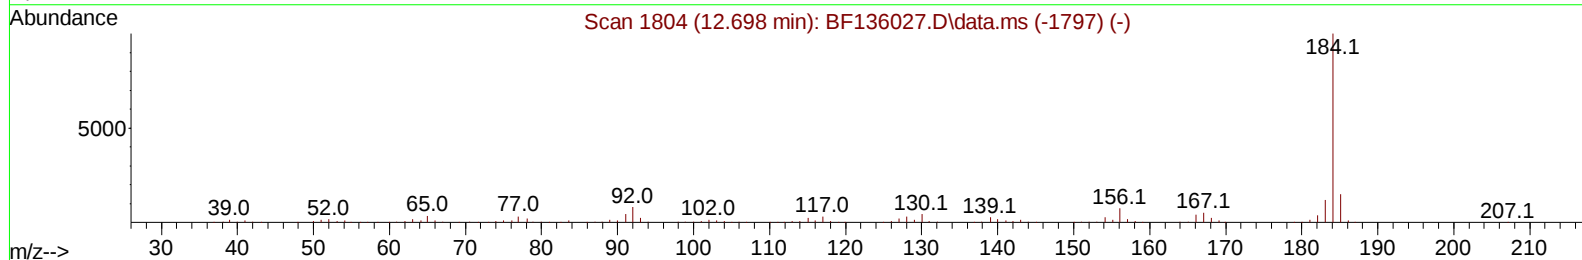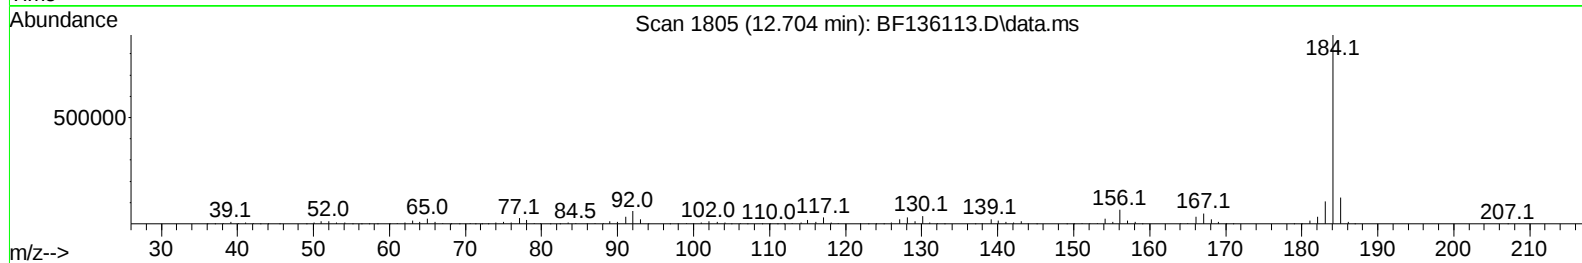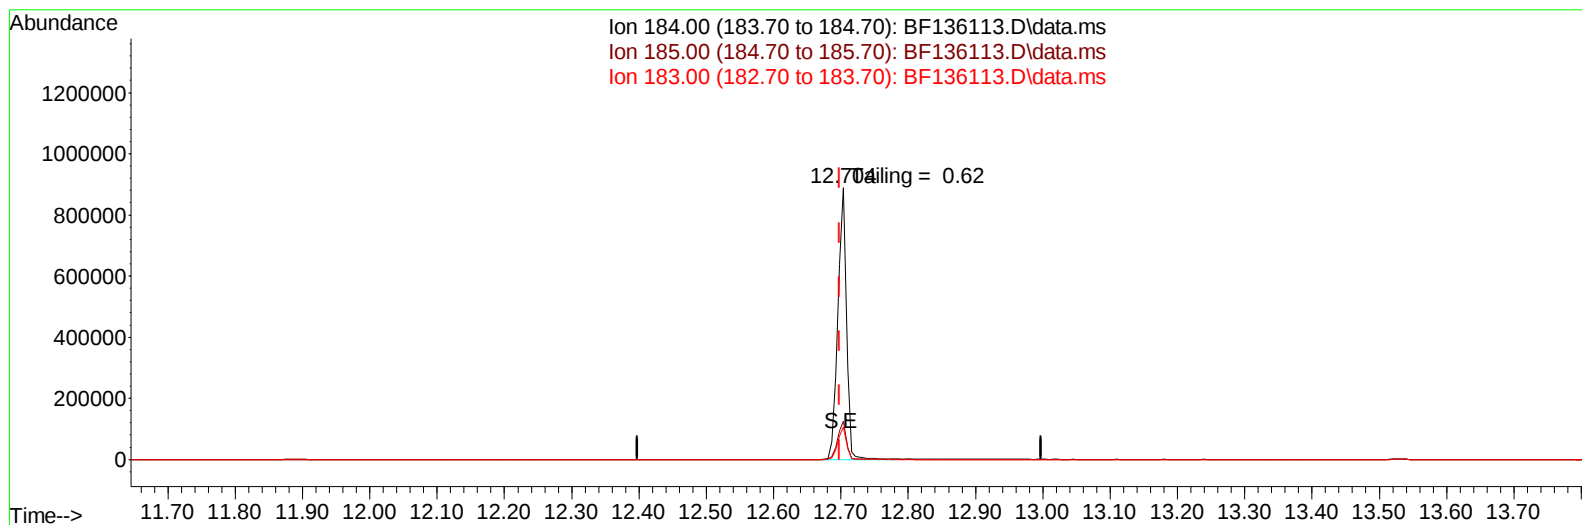

TIC: BF136113.D\data.ms

(77) Benzidine

12.704min (+ 0.006) 0.00 ng

response 784971

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.03
183.00	11.90	11.93
0.00	0.00	0.00