

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110323\
 Data File : BF136117.D
 Acq On : 03 Nov 2023 11:27
 Operator : CG\JU
 Sample : PB156798BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB156798BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136117.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.169	10	14	21	rVB	32457	45793	1.14%	0.190%
2	5.075	504	508	517	rVB	77635	107846	2.69%	0.448%
3	5.457	567	573	576	rBV	2866642	3167393	79.13%	13.158%
4	6.457	736	743	746	rBV	2725692	3109841	77.70%	12.919%
5	6.816	801	804	808	rVB	878840	704171	17.59%	2.925%
6	7.386	894	901	903	rBV	2017507	2095763	52.36%	8.706%
7	8.098	1017	1022	1025	rBV	1223556	937659	23.43%	3.895%
8	9.180	1200	1206	1209	rBV	4342783	3869393	96.67%	16.074%
9	9.857	1317	1321	1324	rBV	1390188	1055873	26.38%	4.386%
10	10.651	1451	1456	1459	rBV	2696047	2432018	60.76%	10.103%
11	11.351	1571	1575	1578	rBV	1275208	1085997	27.13%	4.511%
12	12.957	1842	1848	1851	rBV	3811193	4002533	100.00%	16.627%
13	14.004	2022	2026	2030	rBV	944531	811176	20.27%	3.370%
14	15.492	2273	2279	2288	rBV	528376	647039	16.17%	2.688%




Sum of corrected areas: 24072495

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110323\
Data File : BF136117.D
Acq On : 03 Nov 2023 11:27
Operator : CG\JU
Sample : PB156798BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156798BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

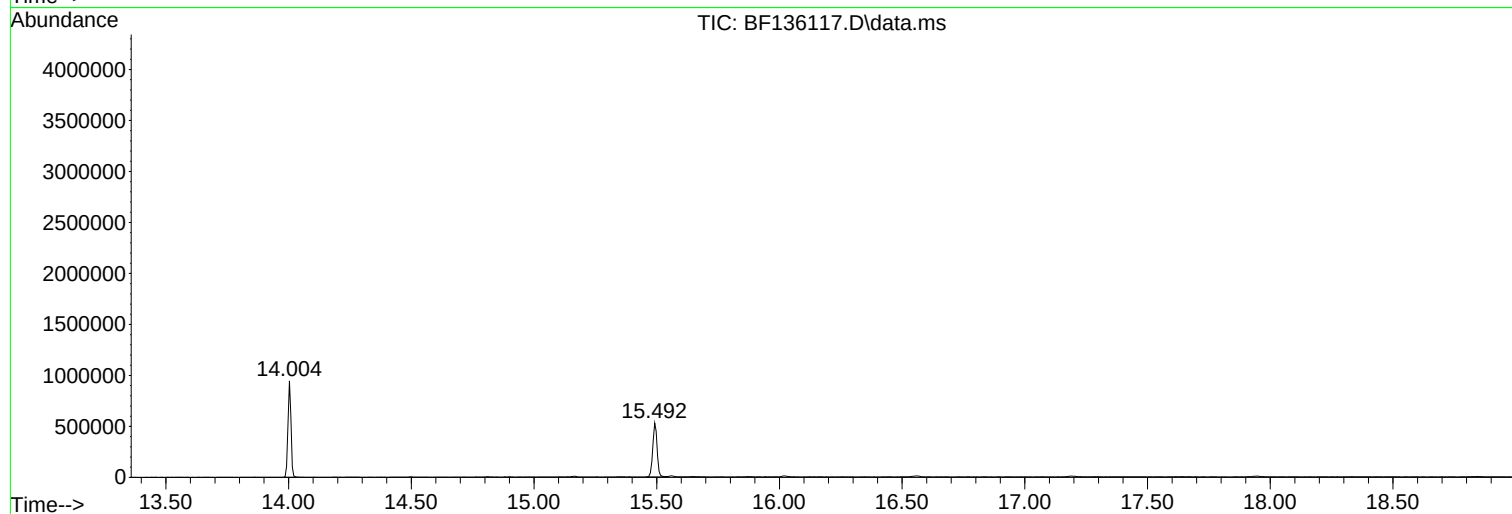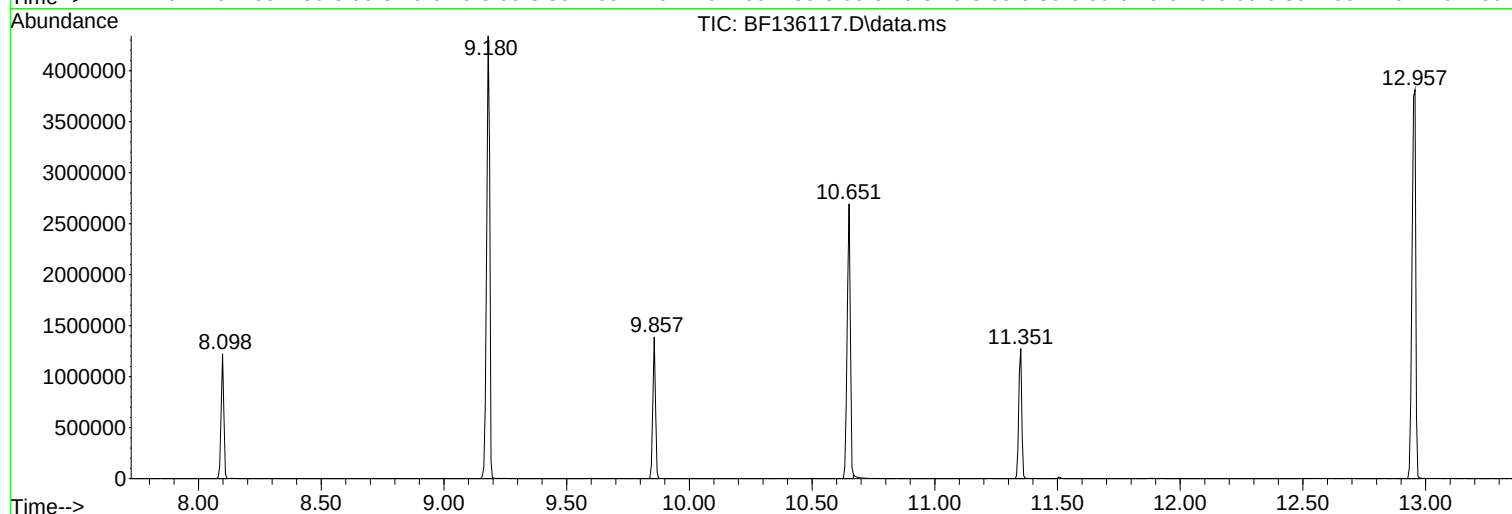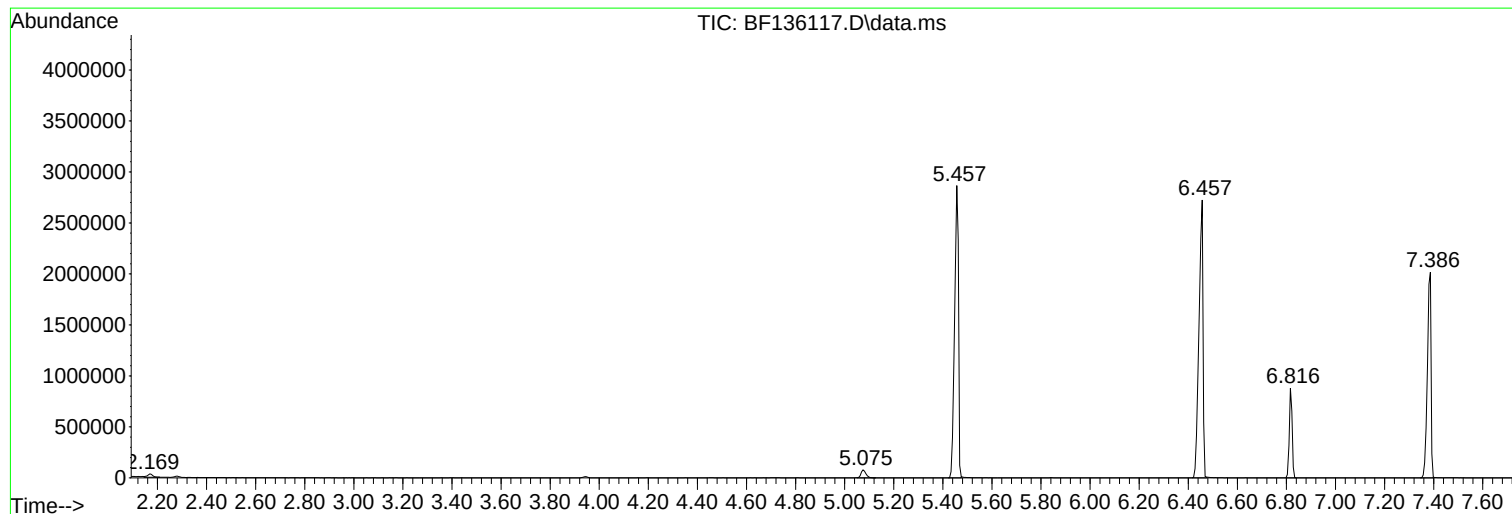

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110323\
Data File : BF136117.D
Acq On : 03 Nov 2023 11:27
Operator : CG\JU
Sample : PB156798BL
Misc :
ALS Vial : 5 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB156798BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
5.075	3.06 ng	107846	1,4-Dichlorobenzene-d4			6.816
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	56
2	2,3-Butanedione, monooxime		101	C4H7NO2	000057-71-6	25
3	2-Pentanol, 2,4-dimethyl-		116	C7H16O	000625-06-9	23
4	Acetone		58	C3H6O	000067-64-1	10
5	1-Propen-2-ol, acetate		100	C5H8O2	000108-22-5	10

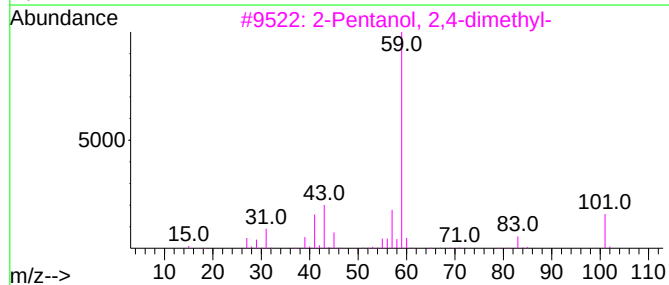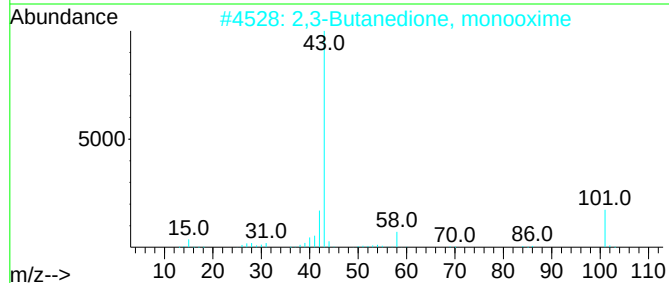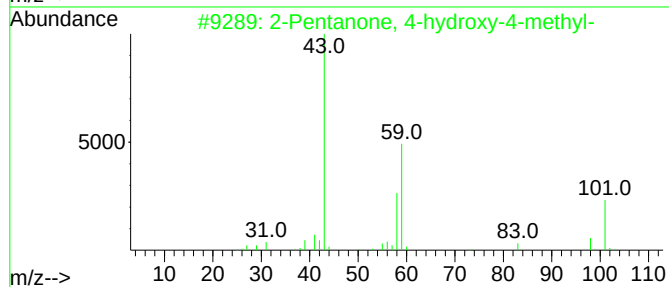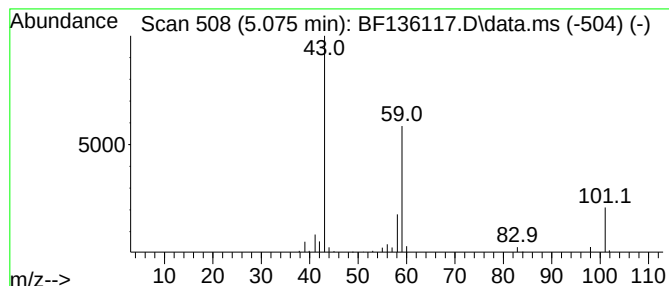

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110323\
Data File : BF136117.D
Acq On : 03 Nov 2023 11:27
Operator : CG\JU
Sample : PB156798BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156798BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.075	3.1	ng	107846	1	6.816	704171	20.0