

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110323\
 Data File : BF136123.D
 Acq On : 03 Nov 2023 14:38
 Operator : CG\JU
 Sample : 05096-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.034	497	501	509	rVB	85546	96481	2.71%	0.557%
2	5.440	566	570	574	rBV	1256391	1188960	33.46%	6.862%
3	6.439	736	740	743	rBV	801002	679986	19.13%	3.924%
4	6.816	801	804	808	rVB	751149	598628	16.84%	3.455%
5	7.381	895	900	903	rBV	1998586	1969971	55.43%	11.369%
6	8.098	1018	1022	1025	rBV	1021083	789257	22.21%	4.555%
7	8.322	1057	1060	1062	rBV	51196	44061	1.24%	0.254%
8	8.345	1062	1064	1073	rVB	69001	68846	1.94%	0.397%
9	9.180	1202	1206	1209	rBV	4372772	3553760	100.00%	20.510%
10	9.857	1317	1321	1324	rBV	1018102	861655	24.25%	4.973%
11	10.645	1451	1455	1459	rBV	2176087	2122965	59.74%	12.252%
12	11.345	1570	1574	1578	rBV	968632	809063	22.77%	4.669%
13	12.951	1842	1847	1850	rBV	3559630	3196755	89.95%	18.449%
14	14.004	2022	2026	2029	rBV	718823	611065	17.19%	3.527%
15	15.492	2273	2279	2287	rBV	582617	735720	20.70%	4.246%




Sum of corrected areas: 17327173

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110323\
Data File : BF136123.D
Acq On : 03 Nov 2023 14:38
Operator : CG\JU
Sample : 05096-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

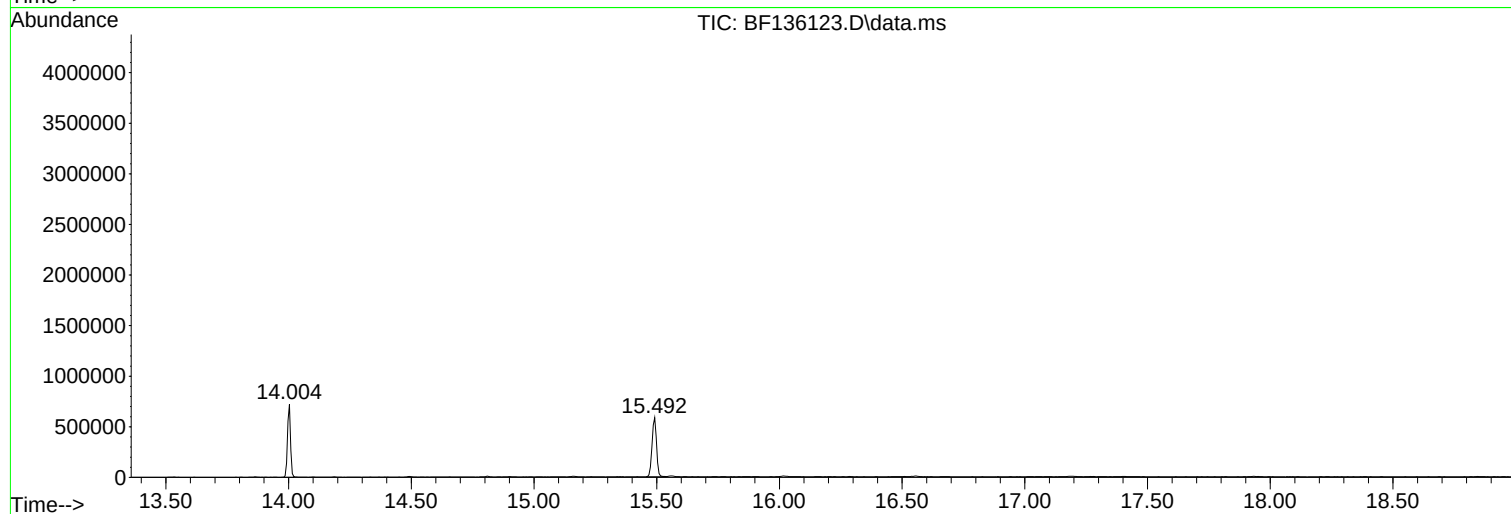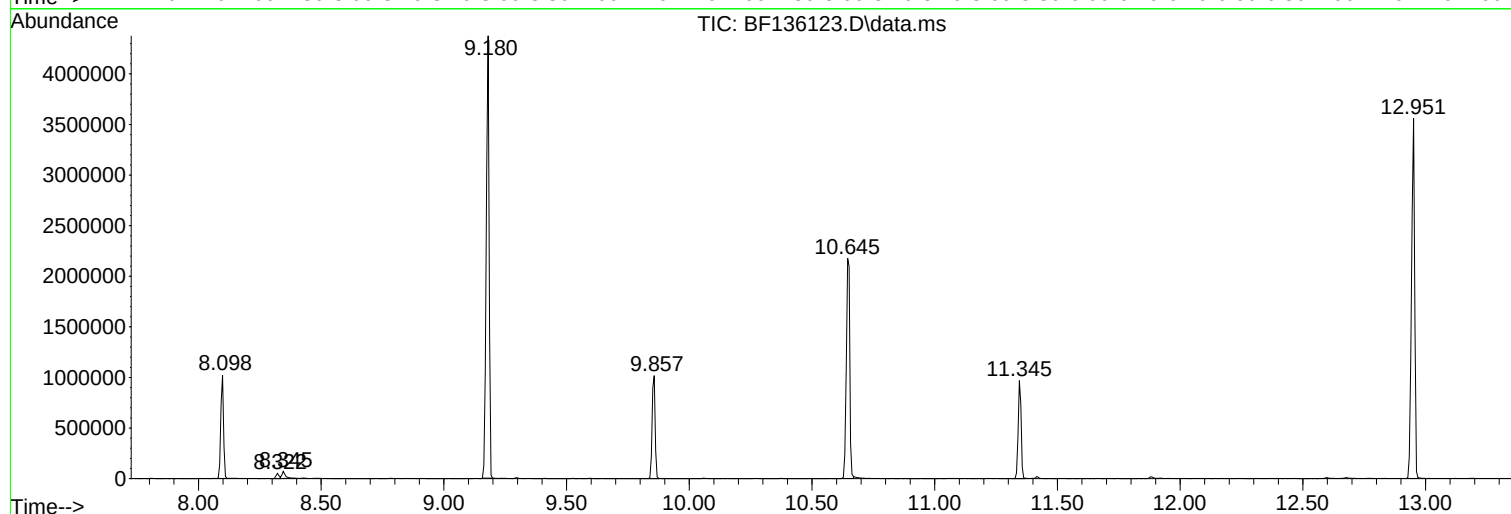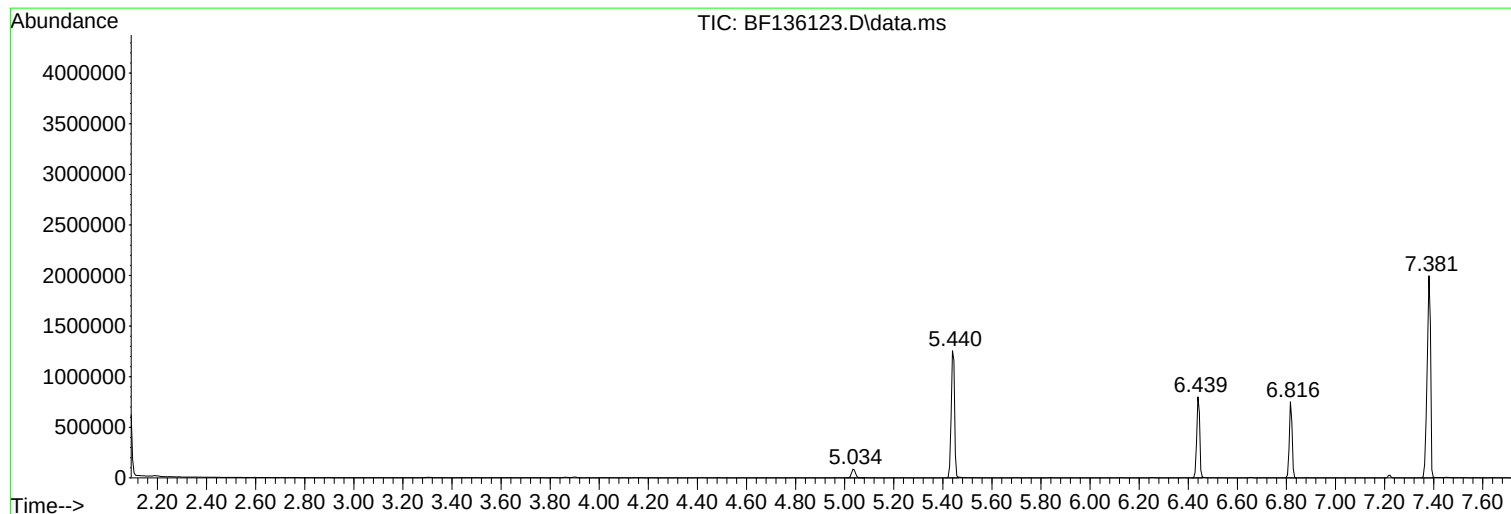

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110323\
Data File : BF136123.D
Acq On : 03 Nov 2023 14:38
Operator : CG\JU
Sample : 05096-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.034	3.22 ng	96481	1,4-Dichlorobenzene-d4	6.816

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59		
2	3-Octanol	130	C8H18O	000589-98-0	33		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	32		
4	3-Hydroxy-3-methyl-2-butanone	102	C5H10O2	000115-22-0	32		
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12		

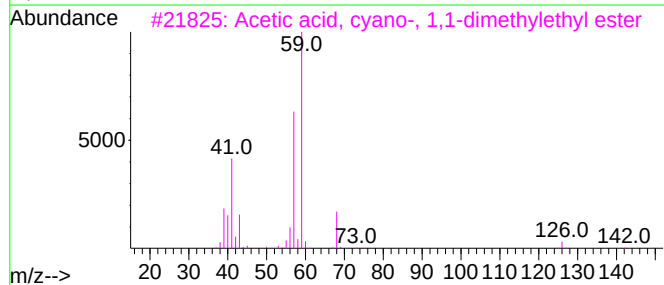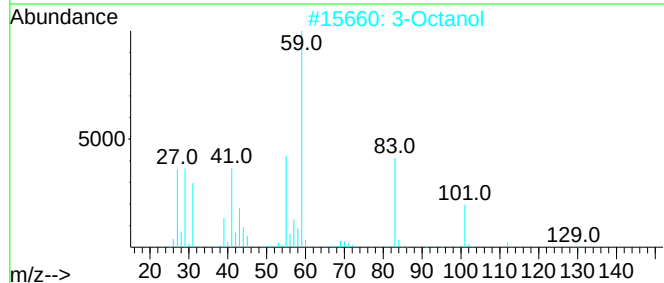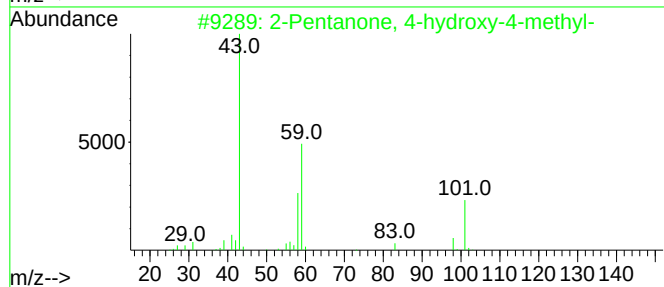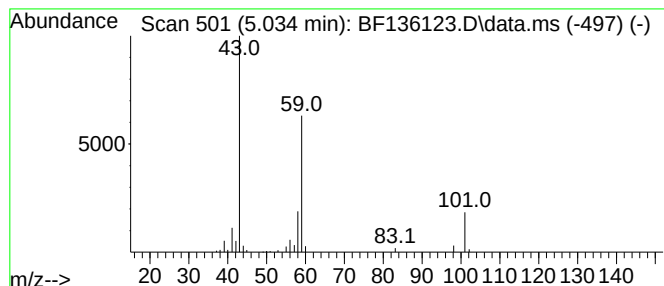

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110323\
Data File : BF136123.D
Acq On : 03 Nov 2023 14:38
Operator : CG\JU
Sample : 05096-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.034	3.2	ng	96481	1	6.816	598628	20.0