


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110323\
Data File : BF136113.D
Acq On : 03 Nov 2023 09:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 31 01:13:02 2023

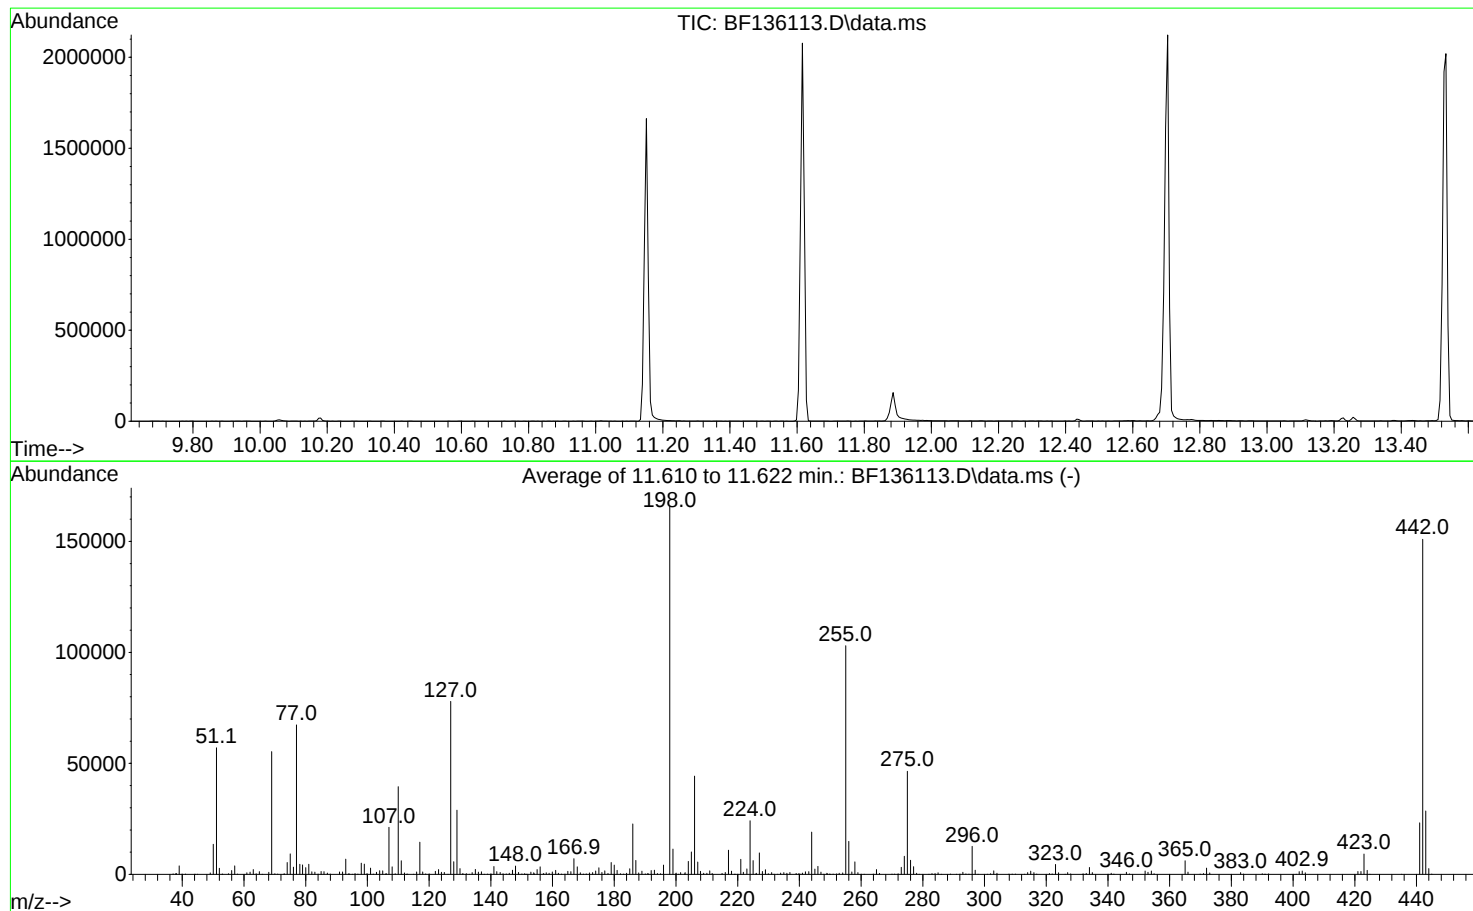




AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	57000	PASS
68	69	0.00	2	1.7	948	PASS
69	198	0.00	100	33.4	55312	PASS
70	69	0.00	2	0.6	306	PASS
127	198	10	80	47.0	77901	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	165709	PASS
199	198	5	9	6.9	11365	PASS
275	198	10	60	28.0	46448	PASS
365	198	1	100	3.7	6167	PASS
441	198	0.01	100	14.0	23220	PASS
442	442	50	100	100.0	150965	PASS
443	442	15	24	18.9	28581	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110323\
 Data File : BF136113.D
 Acq On : 03 Nov 2023 09:29
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 03 20:42:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 31 01:13:02 2023
 Response via : Initial Calibration

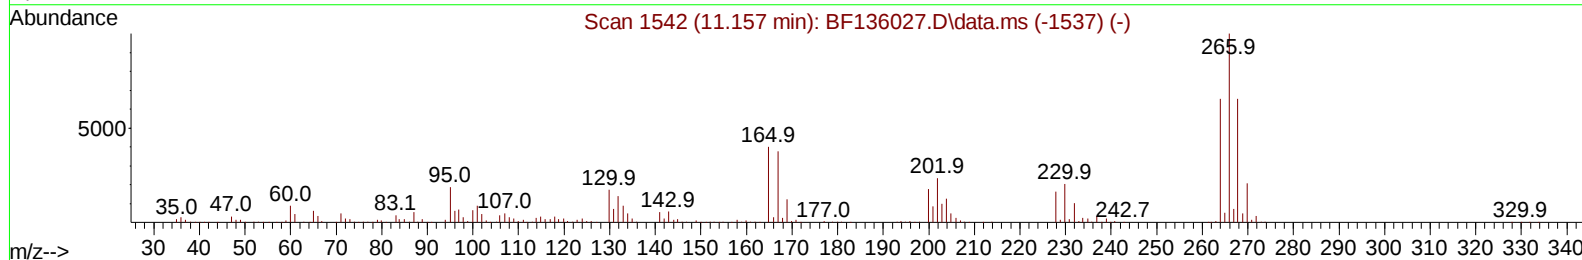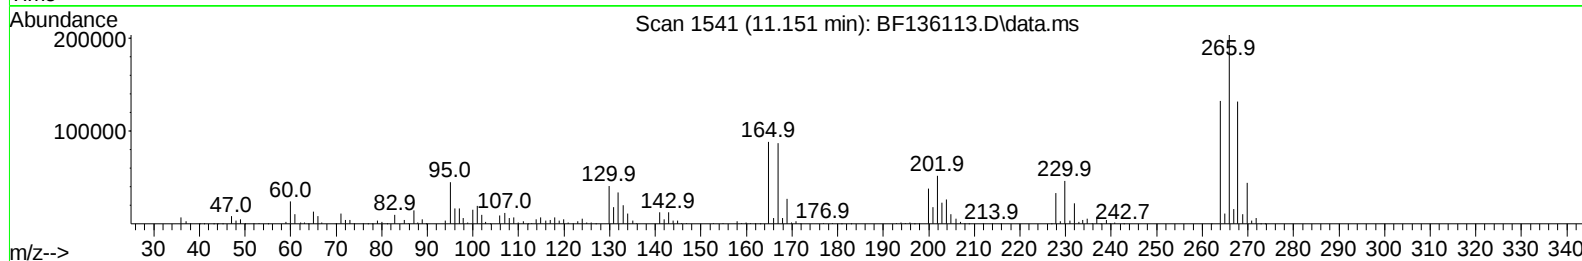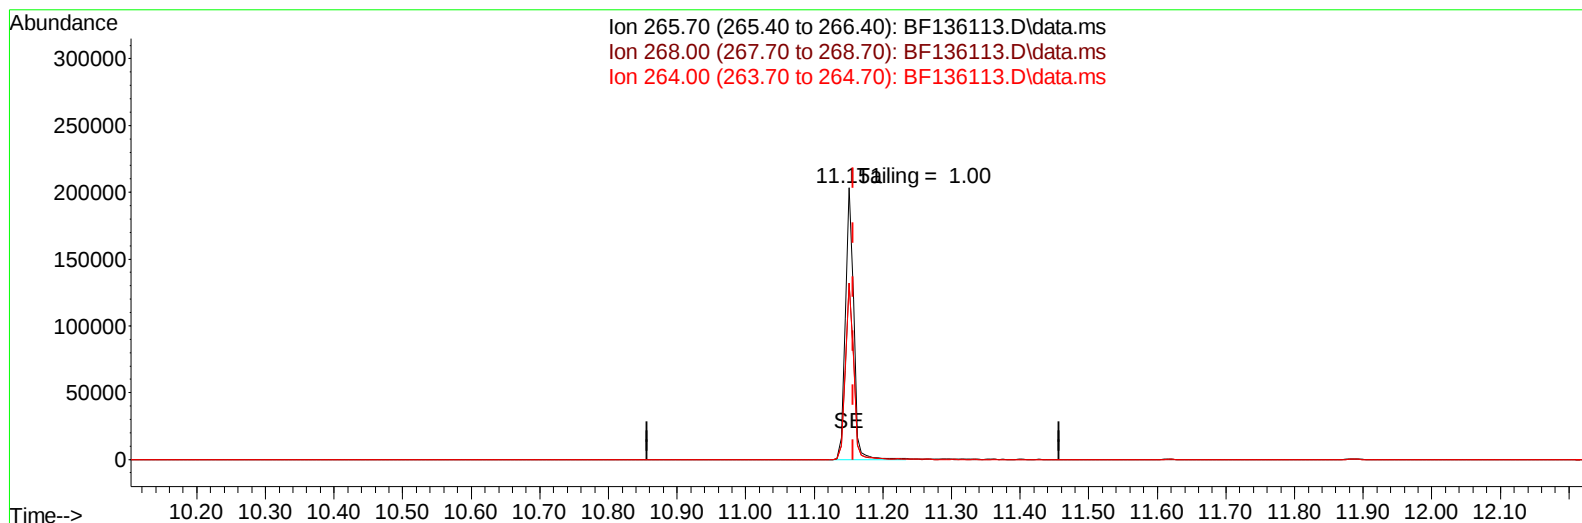

TIC: BF136113.D\data.ms

(70) Pentachlorophenol (C)

11.151min (-0.006) 33621.96 ng




response 169006

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.86
264.00	65.30	65.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110323\
Data File : BF136113.D
Acq On : 03 Nov 2023 09:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 03 20:42:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 01:13:02 2023
Response via : Initial Calibration

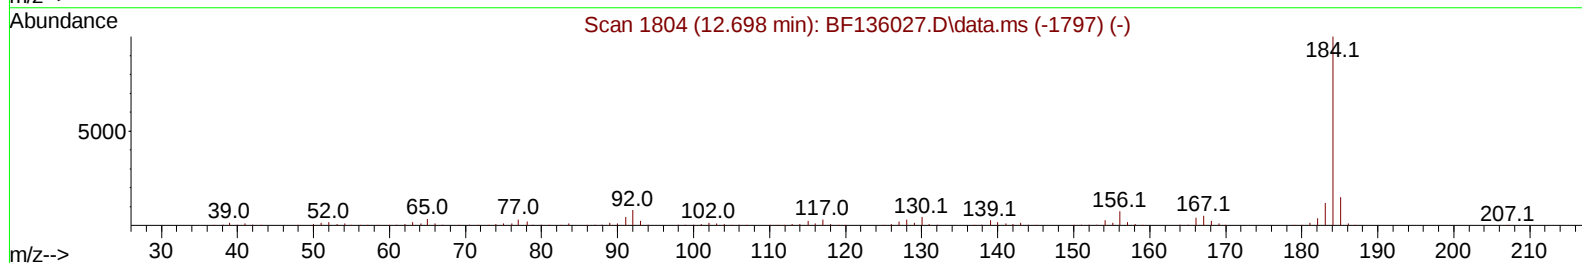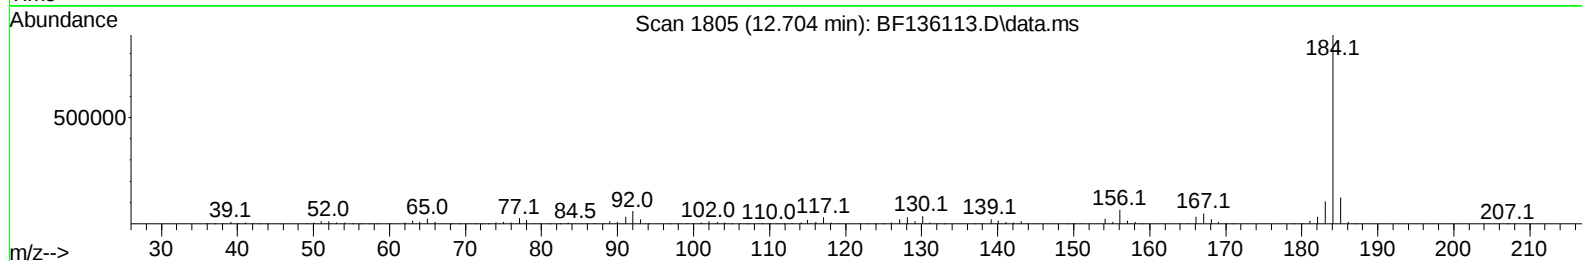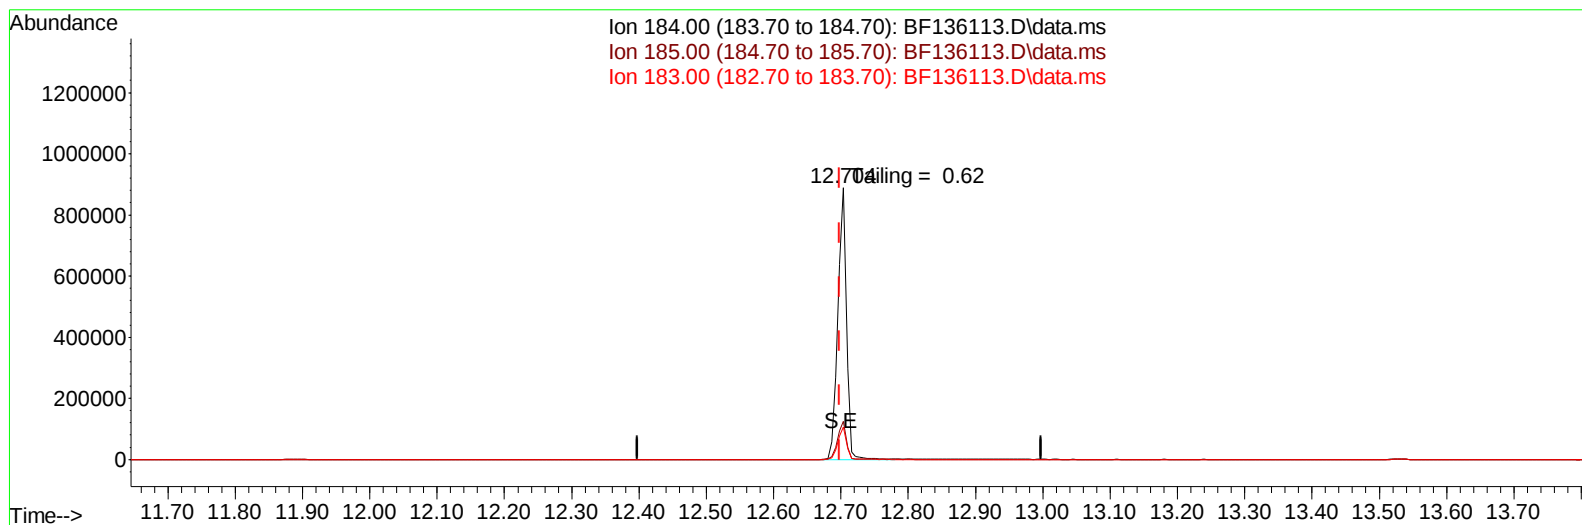

TIC: BF136113.D\data.ms

(77) Benzidine

12.704min (+ 0.006) 0.00 ng

response 784971

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.03
183.00	11.90	11.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/3/2023	BNA_F	<u>BF136113.D</u>
Compound Name	Response	Retention Time
DDT	383117	13.533
DDD	6360	13.257
DDE	314	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6674	389791	1.71

Instrument :
BNA_F
ClientSampleId :
DFTPP